


Data Path : Z:\HPCHEM1\BNA G\DATA\BG082316\
 Data File : BG023864.D
 Acq On : 23 Aug 2016 21:58
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 19:22:14 2016

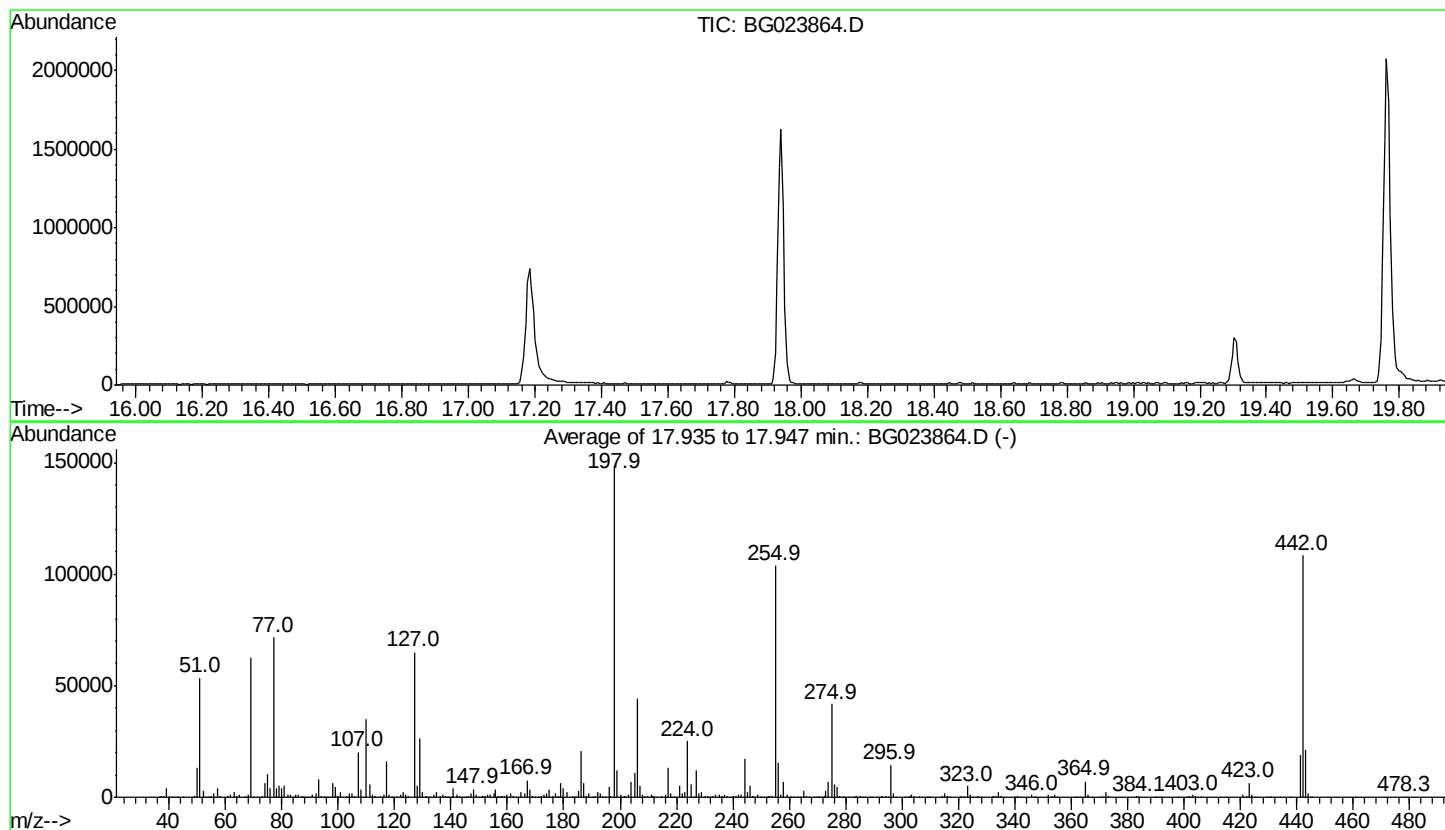

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	53602	PASS
68	69	0.00	2	1.5	945	PASS
69	198	0.00	100	42.1	62592	PASS
70	69	0.00	2	0.1	73	PASS
127	198	10	80	43.7	64877	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148592	PASS
199	198	5	9	8.1	11995	PASS
275	198	10	60	28.1	41813	PASS
365	198	1	100	4.7	6946	PASS
441	442	0.01	24	17.4	18909	PASS
442	198	50	100	72.9	108392	PASS
443	442	15	24	19.7	21394	PASS