

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082319\
 Data File : BG042469.D
 Acq On : 24 Aug 2019 15:59
 Operator : HP/JU
 Sample : K4493-32
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 T9-12-13-K1-K4-(0-1.9)

Quant Time: Aug 26 05:50:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	68556	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	268974	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	183580	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	387080	20.00	ng	0.00
76) Chrysene-d12	21.69	240	384183	20.00	ng	0.00
87) Perylene-d12	24.93	264	440464	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	455910	134.69	ng	0.00
7) Phenol-d6	7.17	99	556392	121.69	ng	0.00
23) Nitrobenzene-d5	9.17	82	410811	105.54	ng	0.00
42) 2,4,6-Tribromophenol	16.16	330	329525	126.29	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	1139946	105.02	ng	0.00
79) Terphenyl-d14	20.02	244	1750448	98.50	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.11	163	44431	3.354	ng	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082319\
Data File : BG042469.D
Acq On : 24 Aug 2019 15:59
Operator : HP/JU
Sample : K4493-32
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
T9-12-13-K1-K4-(0-1.9)

Quant Time: Aug 26 05:50:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

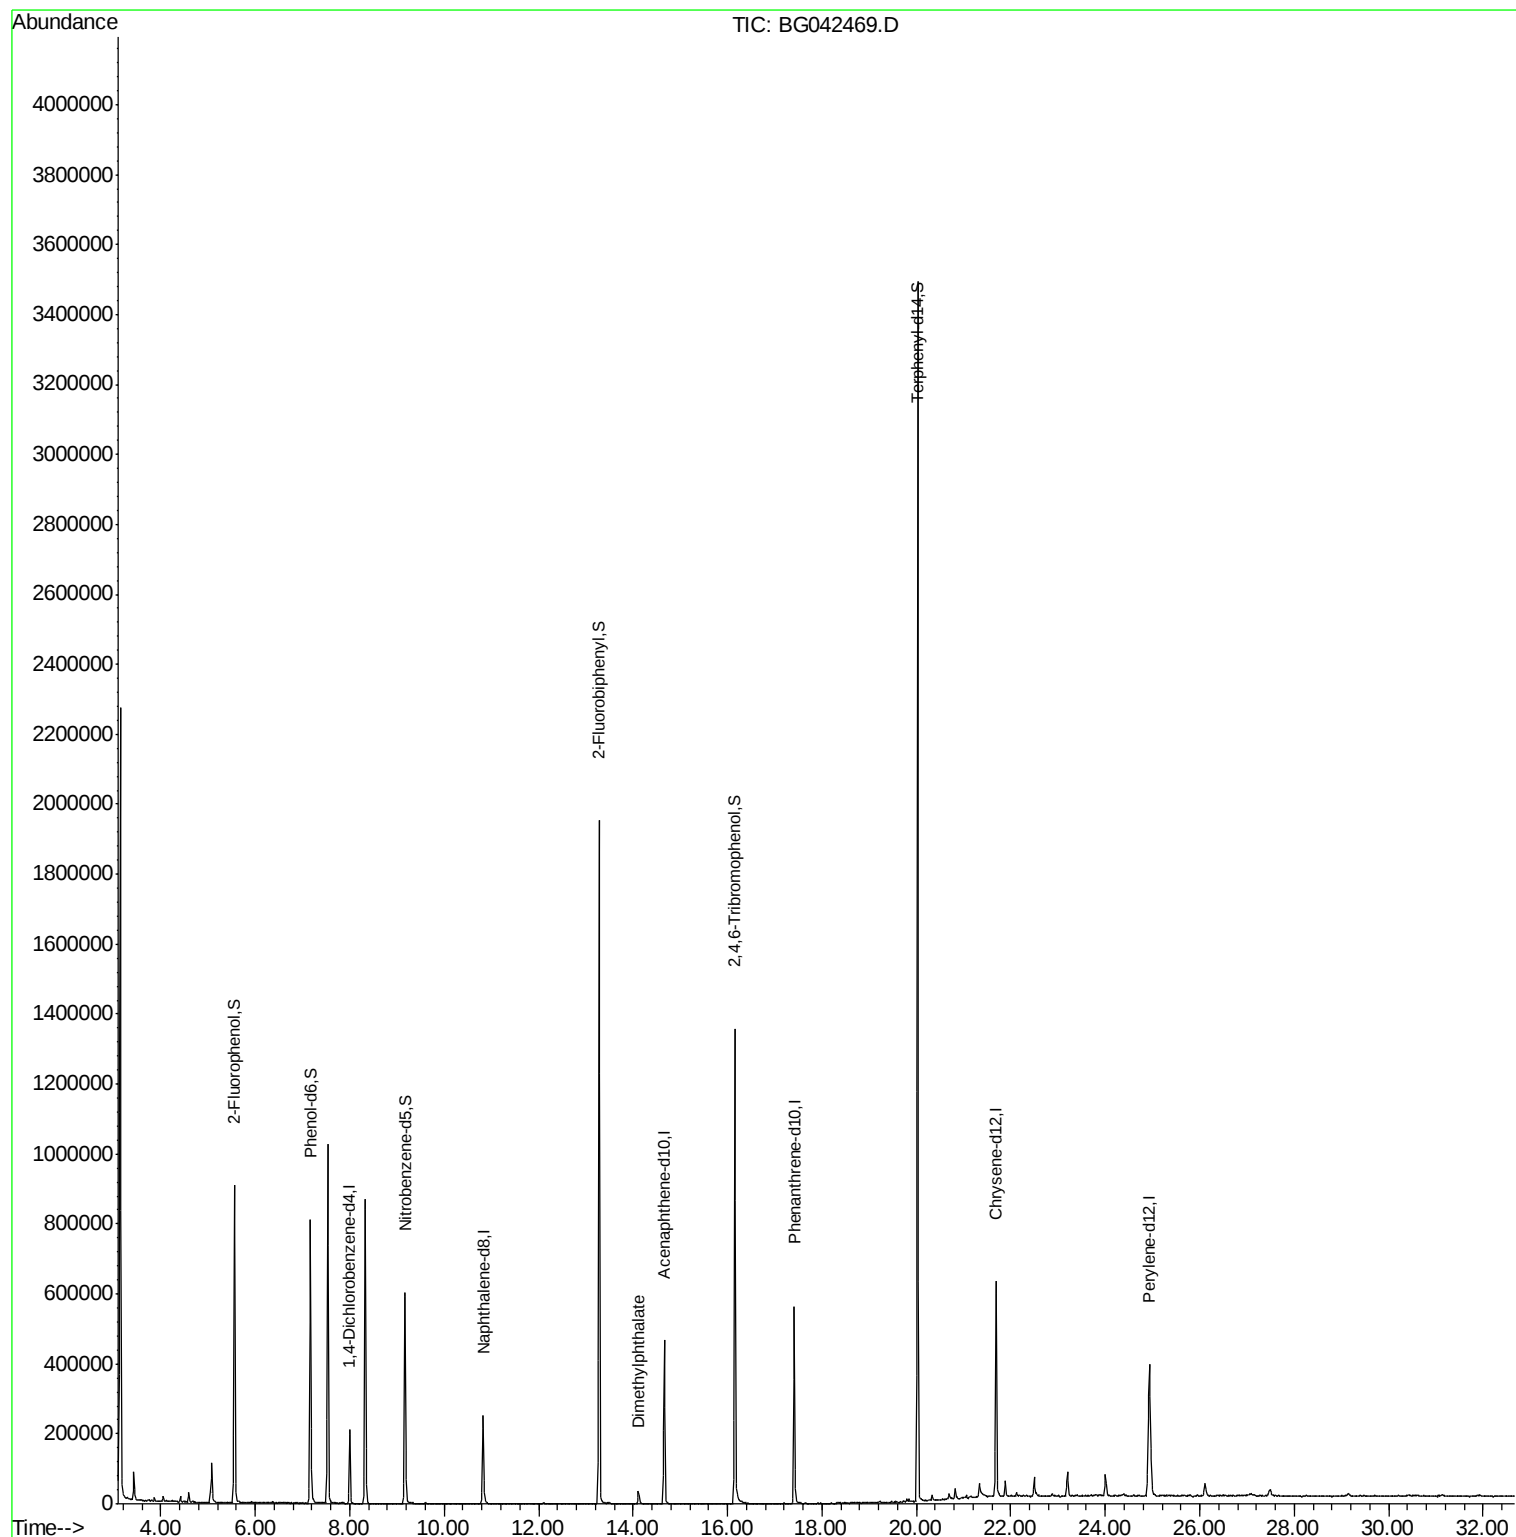




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 836
Delta R.T. -0.00 min
Lab File: BG042469.D
Acq: 24 Aug 2019 15:59

Instrument :
BNA_G
ClientSampleId :
T9-12-13-K1-K4-(0-1.9)

Tot Ion:152 Resp: 68556
Ion Ratio Lower Upper
152 100
150 155.4 125.4 188.0
115 54.6 38.5 57.7

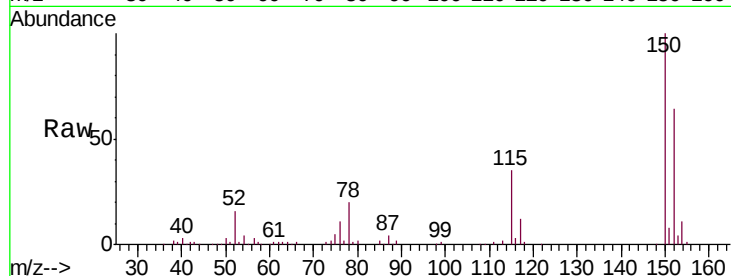


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

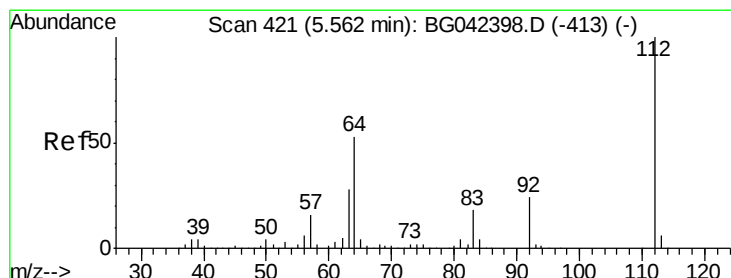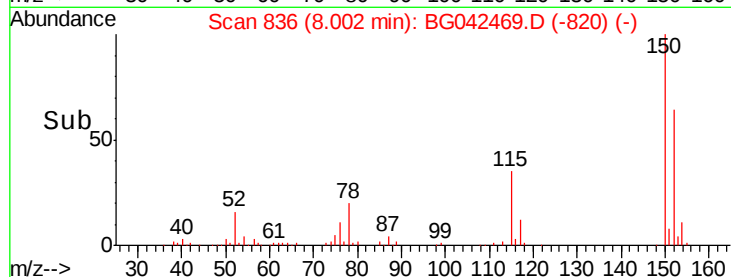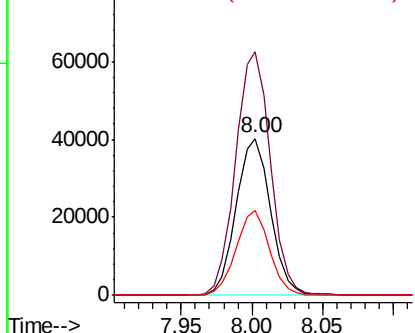



#5


2-Fluorophenol
Concen: 134.686 ng
RT: 5.56 min Scan# 420
Delta R.T. -0.00 min
Lab File: BG042469.D
Acq: 24 Aug 2019 15:59

Tgt Ion:112 Resp: 455910
Ion Ratio Lower Upper
112 100
64 56.0 42.8 64.2
63 28.4 22.7 34.1

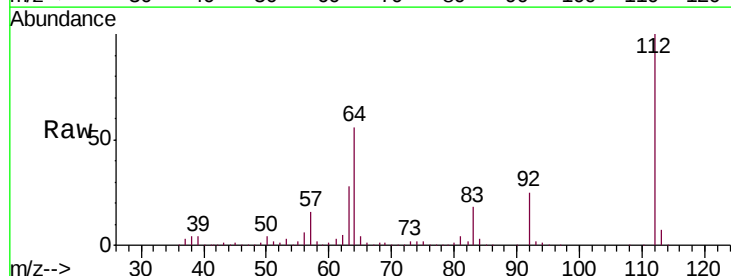

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

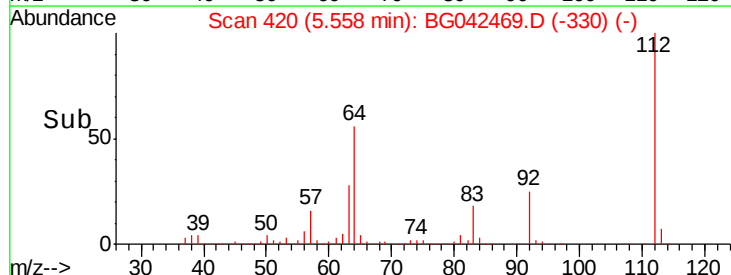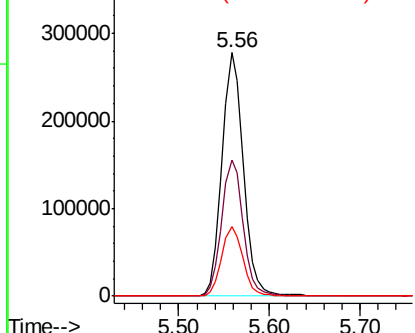

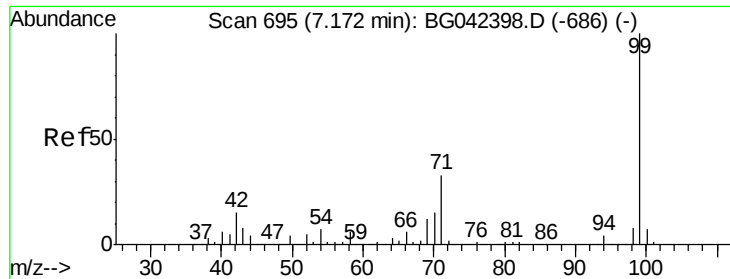

#7

Phenol-d6

Concen: 121.686 ng

RT: 7.17 min Scan# 694

Delta R.T. -0.00 min

Lab File: BG042469.D

Acq: 24 Aug 2019 15:59

Instrument :

BNA_G

ClientSampleId :

T9-12-13-K1-K4-(0-1.9)


Tot Ion: 99 Resp: 556392

Ion Ratio Lower Upper




99 100

42 14.0 12.0 18.0

71 32.3 26.3 39.5

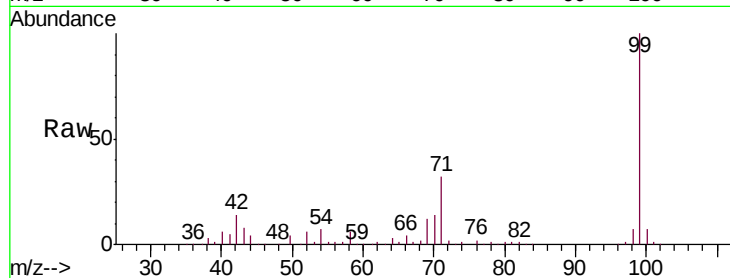

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

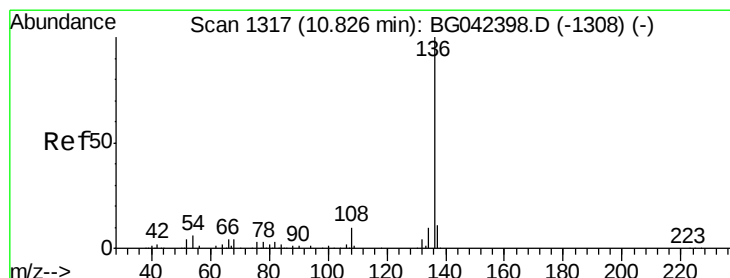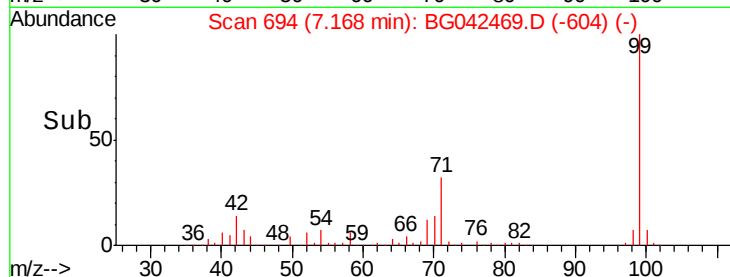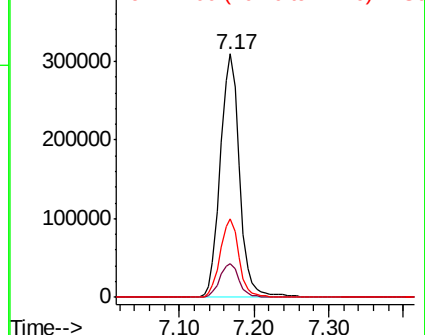

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.00 min

Lab File: BG042469.D

Acq: 24 Aug 2019 15:59

Tgt Ion: 136 Resp: 268974


Ion Ratio Lower Upper

136 100



137 11.5 8.7 13.1

54 7.0 4.9 7.3

68 5.5 3.6 5.4#

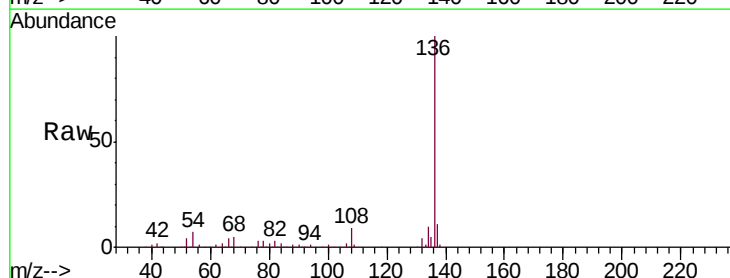

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



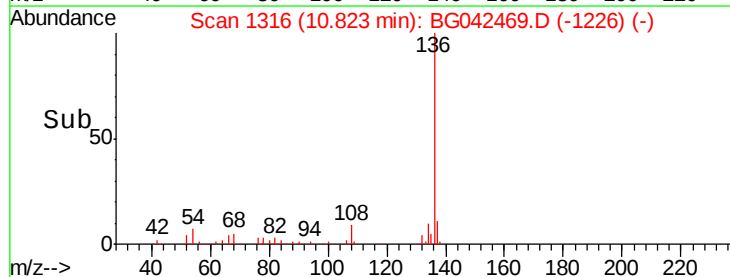
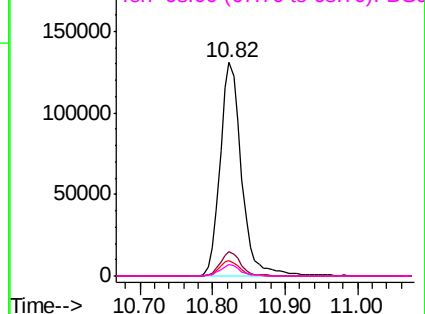




#23
Nitrobenzene-d5
Concen: 105.544 ng
RT: 9.17 min Scan# 1035
Delta R.T. -0.00 min
Lab File: BG042469.D
Acq: 24 Aug 2019 15:59




Instrument :
BNA_G
ClientSampleId :
T9-12-13-K1-K4-(0-1.9)


Tot Ion	82.00	Resp	410811
Ion Ratio	Lower	Upper	
82	100		
128	49.9	40.7	61.1
54	46.3	36.3	54.5

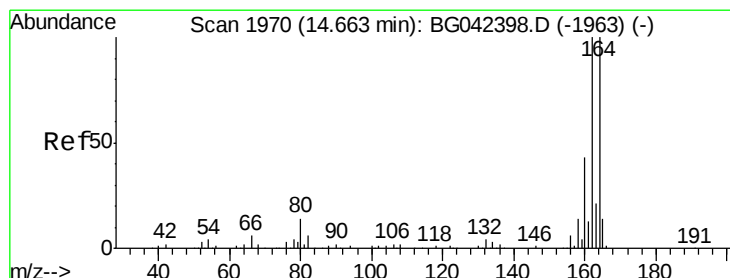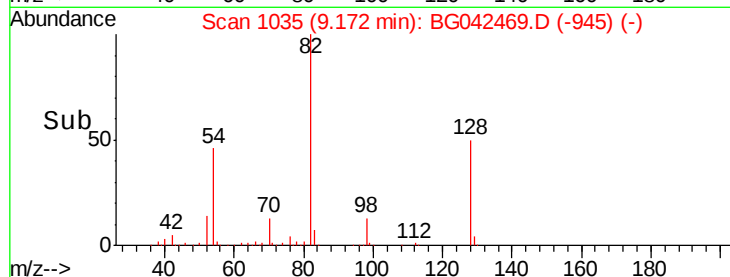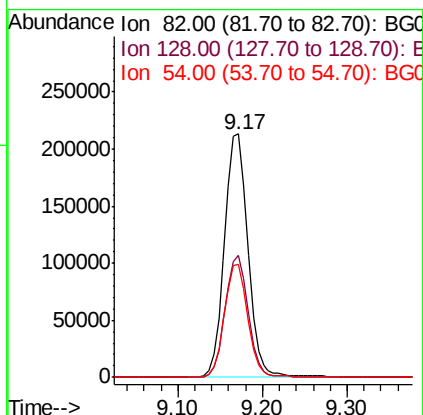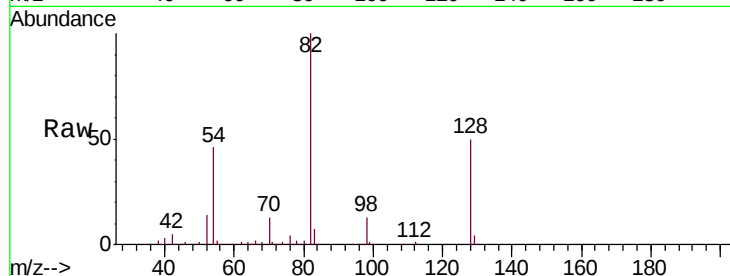

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.66 min Scan# 1969
Delta R.T. -0.00 min
Lab File: BG042469.D
Acq: 24 Aug 2019 15:59

Tgt Ion	164.00	Resp	183580
Ion Ratio	Lower	Upper	
164	100		
162	102.6	79.9	119.9
160	45.9	34.3	51.5

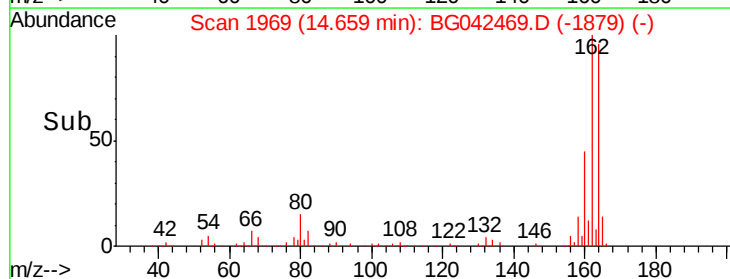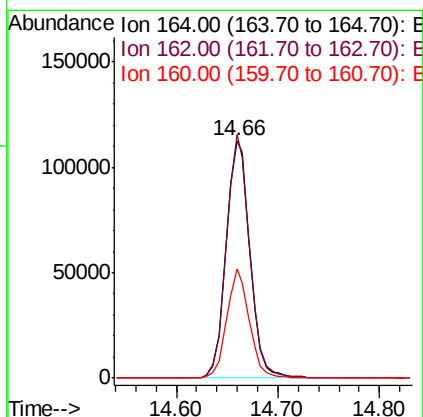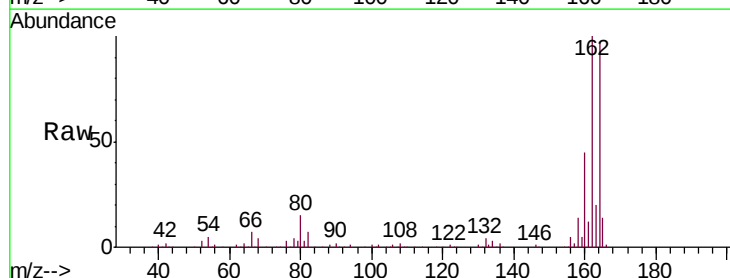

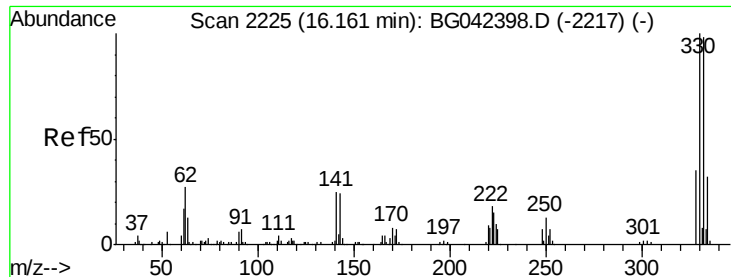

#42

2,4,6-Tribromophenol

Concen: 126.289 ng

RT: 16.16 min Scan# 2224

Delta R.T. -0.00 min

Lab File: BG042469.D

Acq: 24 Aug 2019 15:59

Instrument :

BNA_G

ClientSampleId :

T9-12-13-K1-K4-(0-1.9)


Tot Ion:330 Resp: 329525

Ion Ratio Lower Upper




330 100

332 97.0 77.4 116.0

141 31.0 21.4 32.0

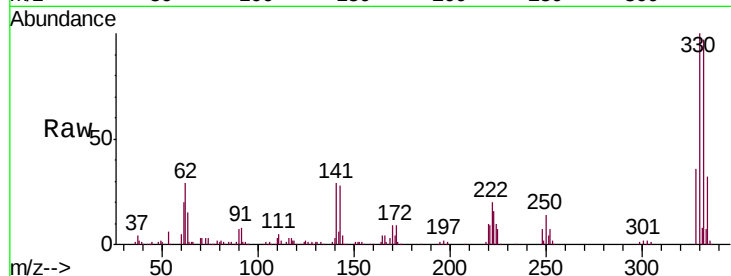

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

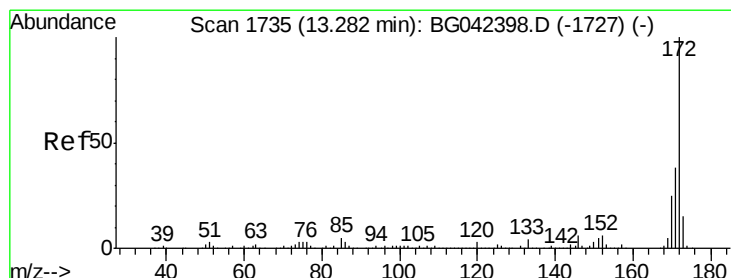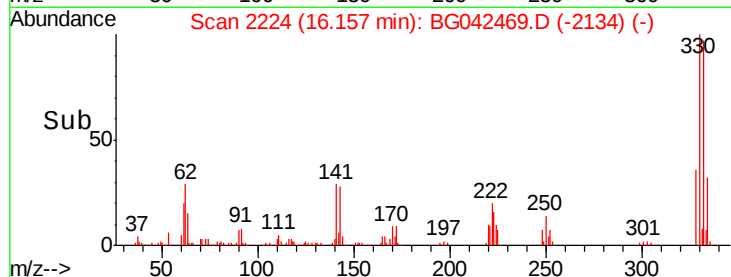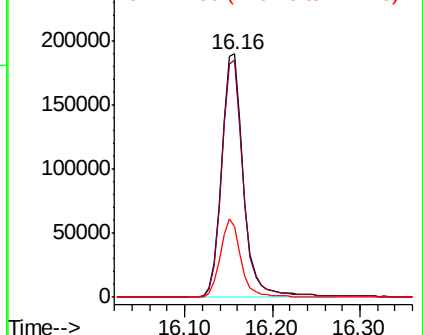

#45

2-Fluorobiphenyl

Concen: 105.021 ng

RT: 13.28 min Scan# 1734

Delta R.T. -0.00 min

Lab File: BG042469.D

Acq: 24 Aug 2019 15:59


Tgt Ion:172 Resp: 1139946

Ion Ratio Lower Upper



172 100


171 38.9 30.5 45.7

170 25.6 20.2 30.2

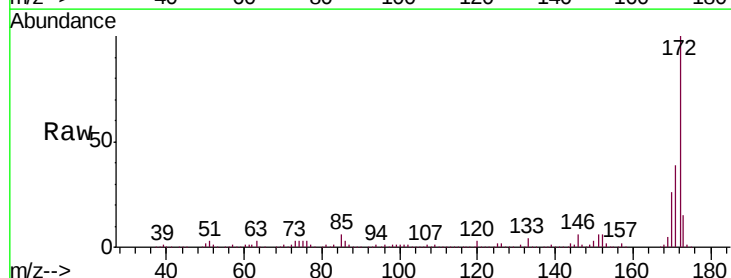

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

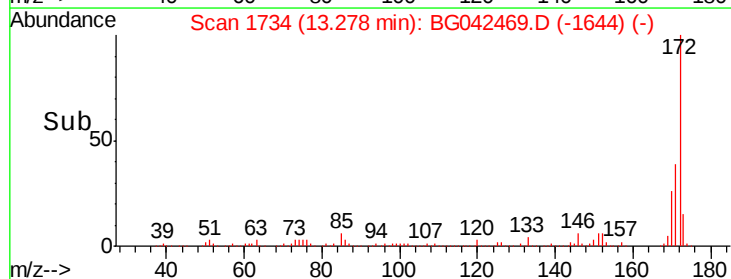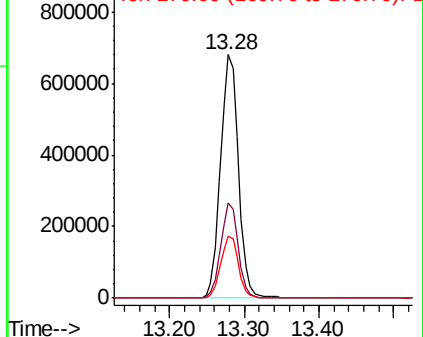

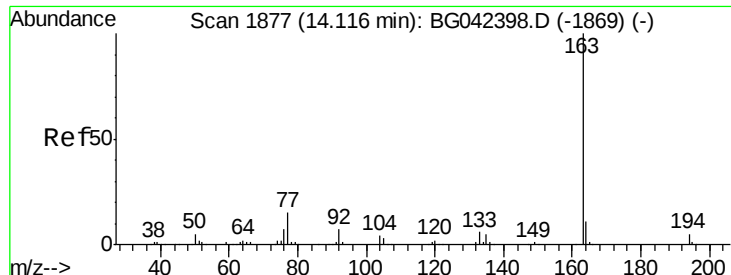

#50

Dimethylphthalate

Concen: 3.354 ng

RT: 14.11 min Scan# 1876

Delta R.T. -0.00 min

Lab File: BG042469.D

Acq: 24 Aug 2019 15:59

Instrument :

BNA_G

ClientSampleId :

T9-12-13-K1-K4-(0-1.9)


Tot Ion:163 Resp: 44431

Ion Ratio Lower Upper

163 100

194 5.5 4.2 6.2




164 9.7 8.8 13.2

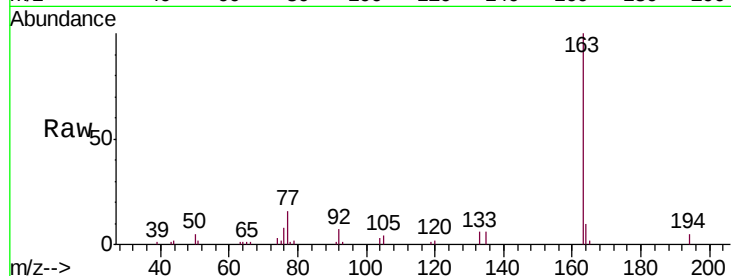

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

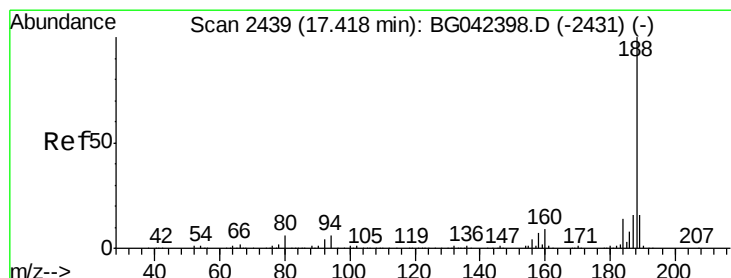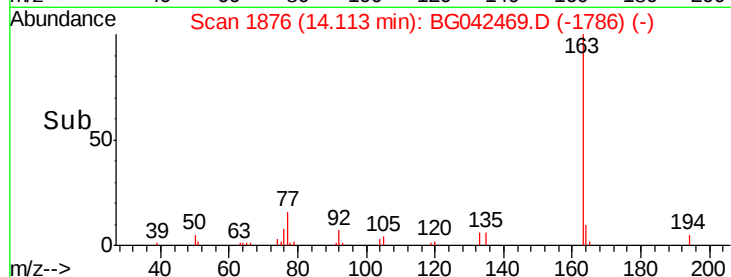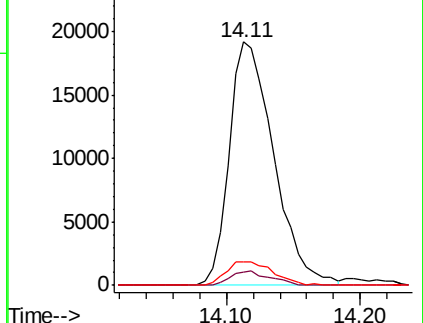

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2438

Delta R.T. -0.00 min

Lab File: BG042469.D

Acq: 24 Aug 2019 15:59


Tgt Ion:188 Resp: 387080

Ion Ratio Lower Upper

188 100

94 6.5 4.5 6.7



80 7.4 4.9 7.3#

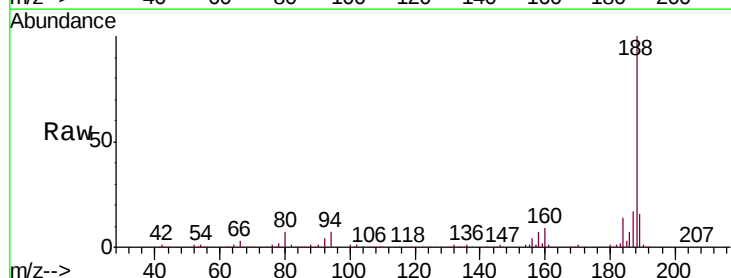


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



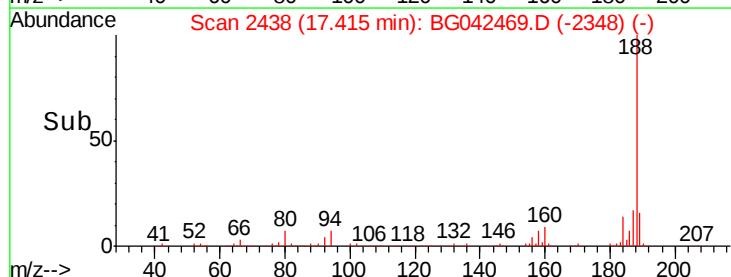
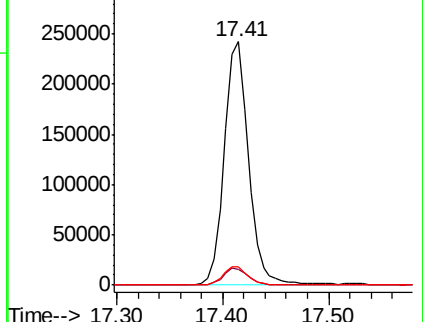


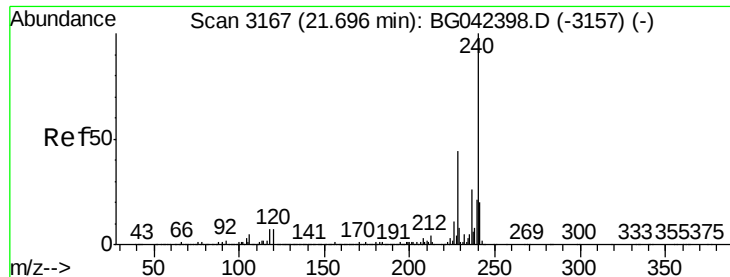

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.69 min Scan# 3165
Delta R.T. -0.01 min
Lab File: BG042469.D
Acq: 24 Aug 2019 15:59




Instrument :
BNA_G
ClientSampleId :
T9-12-13-K1-K4-(0-1.9)


Tot Ion:240 Resp: 384183
Ion Ratio Lower Upper
240 100
120 8.3 5.7 8.5
236 25.4 21.0 31.4

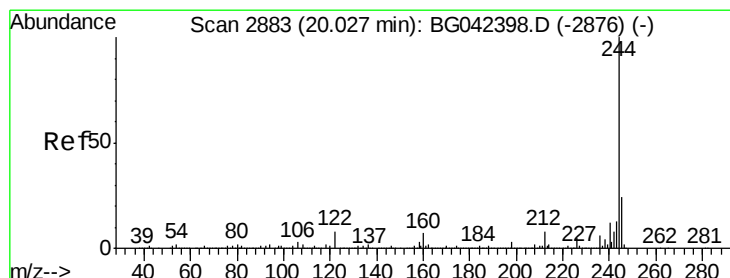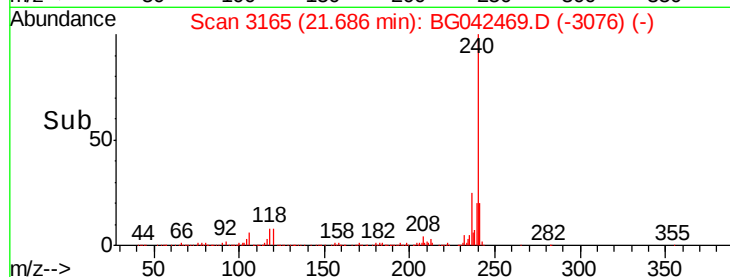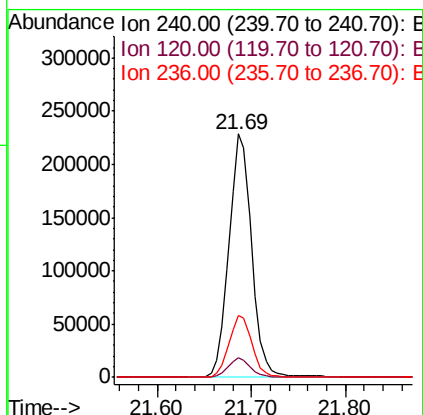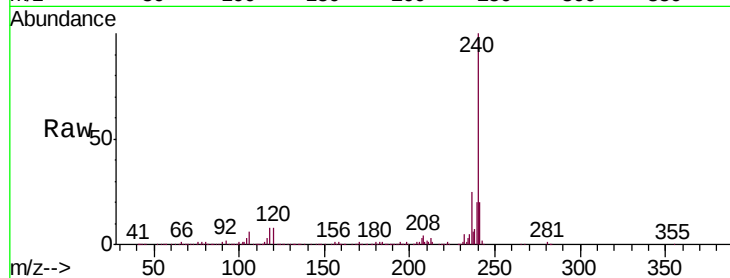

#79
Terphenyl-d14
Concen: 98.503 ng
RT: 20.02 min Scan# 2882
Delta R.T. -0.00 min
Lab File: BG042469.D
Acq: 24 Aug 2019 15:59

Tgt Ion:244 Resp: 1750448
Ion Ratio Lower Upper
244 100
212 8.5 6.0 9.0
122 10.5 6.7 10.1#

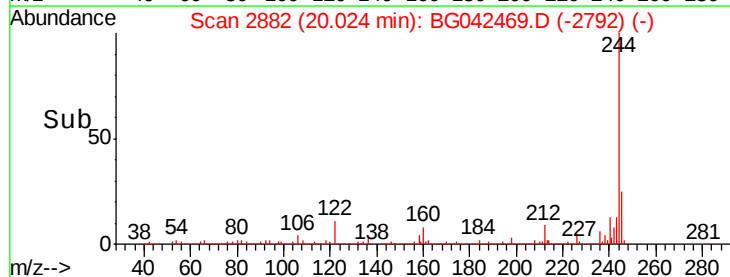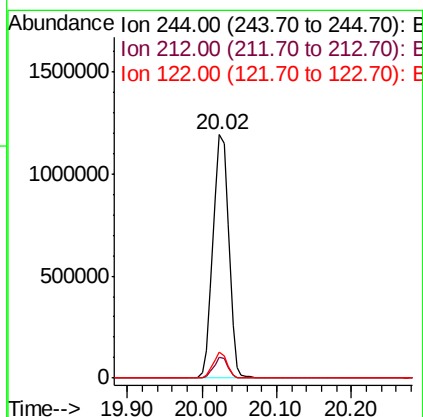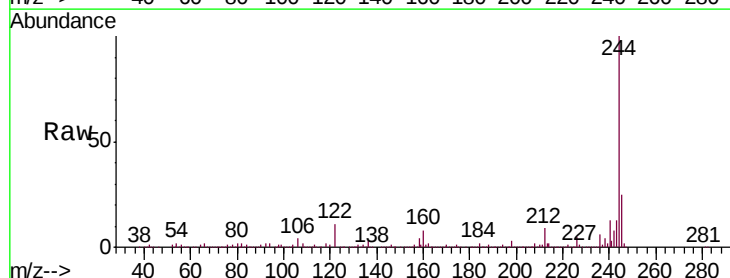

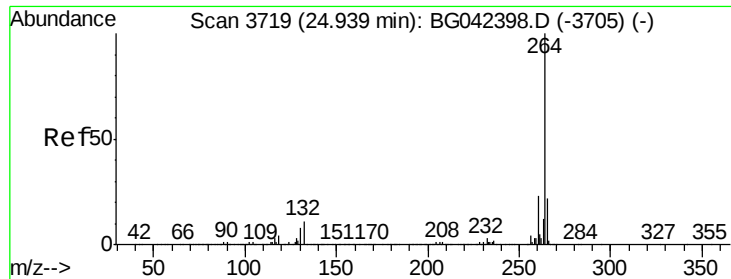

#87
Pervlone-d12
Concen: 20.000 ng
RT: 24.93 min Scan# 3717
Delta R.T. -0.01 min
Lab File: BG042469.D
Acq: 24 Aug 2019 15:59

Instrument :
BNA_G
ClientSampleId :
T9-12-13-K1-K4-(0-1.9)

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.7	18.5	27.7
265	22.6	17.6	26.4

