

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082319\
 Data File : BG042426.D
 Acq On : 23 Aug 2019 9:46
 Operator : HP/JU
 Sample : PB122423BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB122423BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.558	413	420	435	rBV	1525473	2556803	44.68%	8.390%
2	7.168	686	694	718	rBV	1474989	2679631	46.83%	8.793%
3	7.538	748	757	775	rBV	1537500	2791052	48.77%	9.159%
4	8.002	828	836	847	rBV	325556	557402	9.74%	1.829%
5	8.325	882	891	902	rBV	1212628	2189841	38.27%	7.186%
6	9.171	1026	1035	1058	rBV	730205	1378190	24.08%	4.522%
7	10.828	1309	1317	1339	rBV	309382	646658	11.30%	2.122%
8	13.284	1727	1735	1748	rBV	2233674	3714876	64.92%	12.190%
9	14.665	1962	1970	1983	rBV	612048	980780	17.14%	3.218%
10	16.157	2216	2224	2246	rBV	1566462	2666693	46.60%	8.750%
11	17.415	2431	2438	2453	rBV2	698739	1173834	20.51%	3.852%
12	20.029	2877	2883	2897	rBV	4209269	5722416	100.00%	18.778%
13	21.692	3159	3166	3175	rBV	816125	1424756	24.90%	4.675%
14	22.503	3299	3304	3309	rBV	42830	77654	1.36%	0.255%
15	23.202	3417	3423	3433	rVB3	65238	139787	2.44%	0.459%
16	24.019	3556	3562	3570	rVB3	59132	140214	2.45%	0.460%
17	24.929	3708	3717	3736	rVB3	533393	1634197	28.56%	5.362%


Sum of corrected areas: 30474784

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082319\
Data File : BG042426.D
Acq On : 23 Aug 2019 9:46
Operator : HP/JU
Sample : PB122423BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122423BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

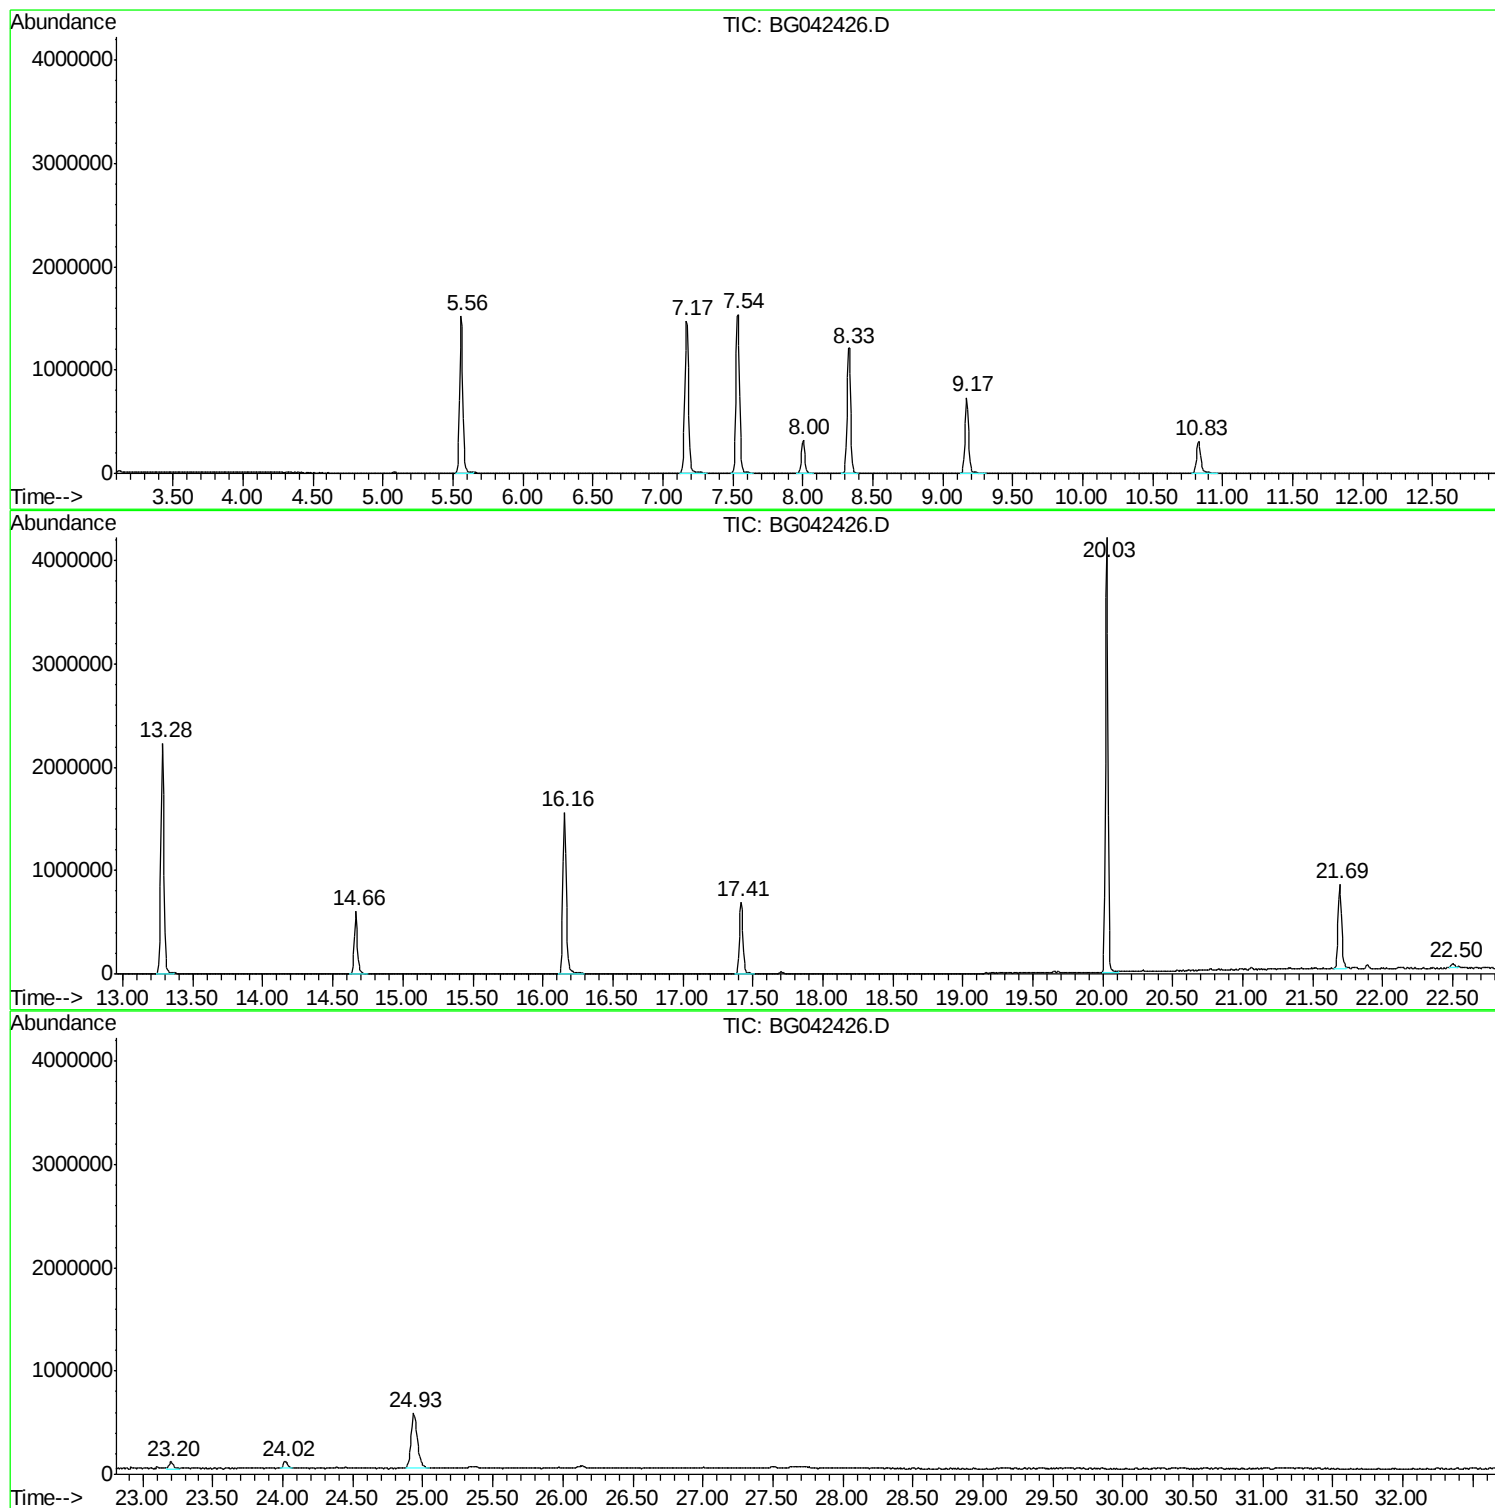

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082319\
Data File : BG042426.D
Acq On : 23 Aug 2019 9:46
Operator : HP/JU
Sample : PB122423BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122423BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.54 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.54	100.15 ng	2791050	1,4-Dichlorobenzene-d4	8.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	43
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
4		Xenon	132	Xe	007440-63-3	9
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

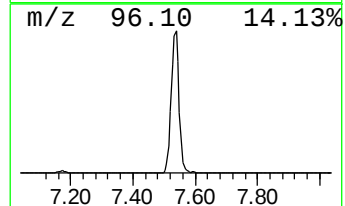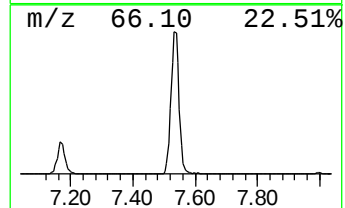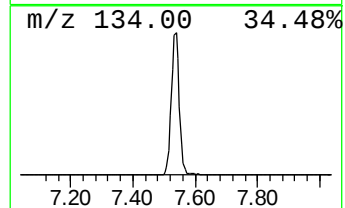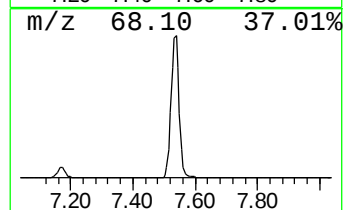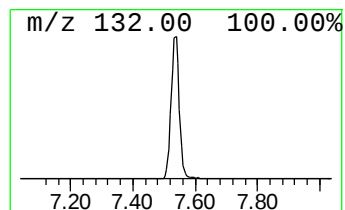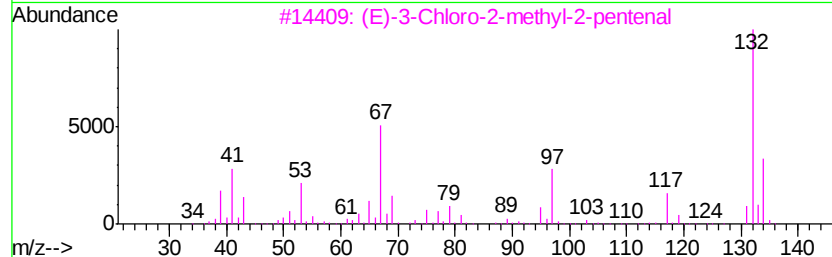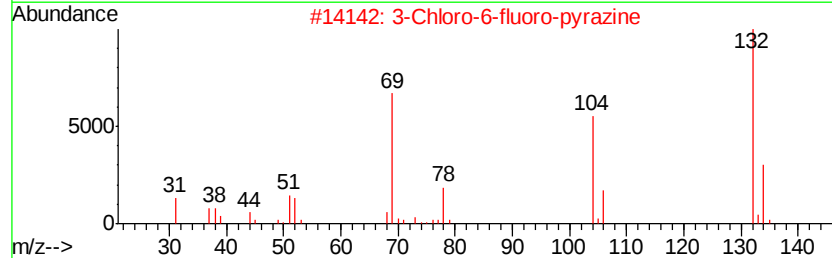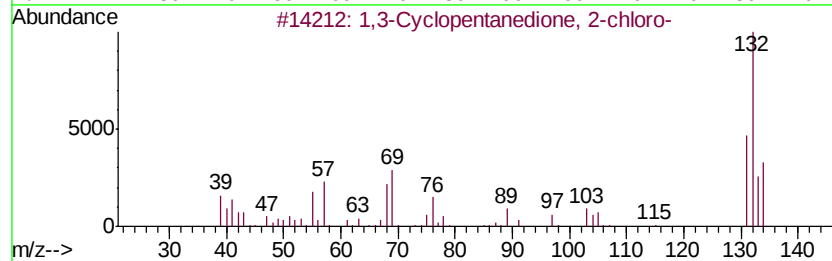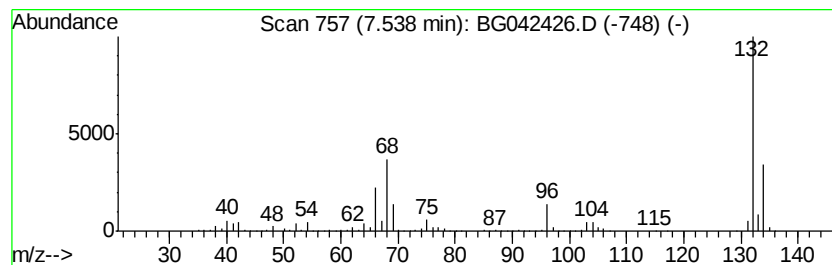

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082319\
Data File : BG042426.D
Acq On : 23 Aug 2019 9:46
Operator : HP/JU
Sample : PB122423BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122423BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.54	7.54	100.2	ng	2791050	1	8.00	557402	20.0