

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082319\
 Data File : BG042437.D
 Acq On : 23 Aug 2019 17:30
 Operator : HP/JU
 Sample : K4086-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NB-08-082019

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.142	3	9	28	rVB	2669904	5105180	92.17%	13.440%
2	3.435	54	59	71	rVB	111906	156603	2.83%	0.412%
3	4.593	252	256	262	rBV2	45446	74870	1.35%	0.197%
4	5.057	329	335	336	rBV	49770	69750	1.26%	0.184%
5	5.086	336	340	353	rVB2	179432	296136	5.35%	0.780%
6	5.562	414	421	437	rBV	1587797	2583542	46.64%	6.802%
7	7.172	684	695	712	rBV	1423557	2579020	46.56%	6.790%
8	7.542	749	758	771	rBV	1762371	3147082	56.82%	8.285%
9	8.006	830	837	845	rBV	381534	650028	11.74%	1.711%
10	8.330	884	892	902	rBV	1539321	2711586	48.96%	7.139%
11	9.176	1026	1036	1059	rBV	1017032	1934972	34.94%	5.094%
12	10.827	1309	1317	1334	rBV	471348	851700	15.38%	2.242%
13	13.283	1728	1735	1756	rBV	2676446	4217161	76.14%	11.102%
14	14.663	1961	1970	1979	rBV2	637072	1058554	19.11%	2.787%
15	16.156	2217	2224	2236	rBV	1752822	2861995	51.67%	7.535%
16	17.419	2432	2439	2445	rBV	716082	1105989	19.97%	2.912%
17	20.034	2878	2884	2891	rBV	3871553	5538735	100.00%	14.582%
18	21.696	3161	3167	3175	rVB	769512	1353141	24.43%	3.562%
19	24.575	3655	3657	3663	rVB6	88515	62718	1.13%	0.165%
20	24.940	3714	3719	3733	rVB3	522072	1558778	28.14%	4.104%
21	32.019	4922	4924	4931	rVB8	59657	66443	1.20%	0.175%


Sum of corrected areas: 37983983

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082319\
Data File : BG042437.D
Acq On : 23 Aug 2019 17:30
Operator : HP/JU
Sample : K4086-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NB-08-082019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

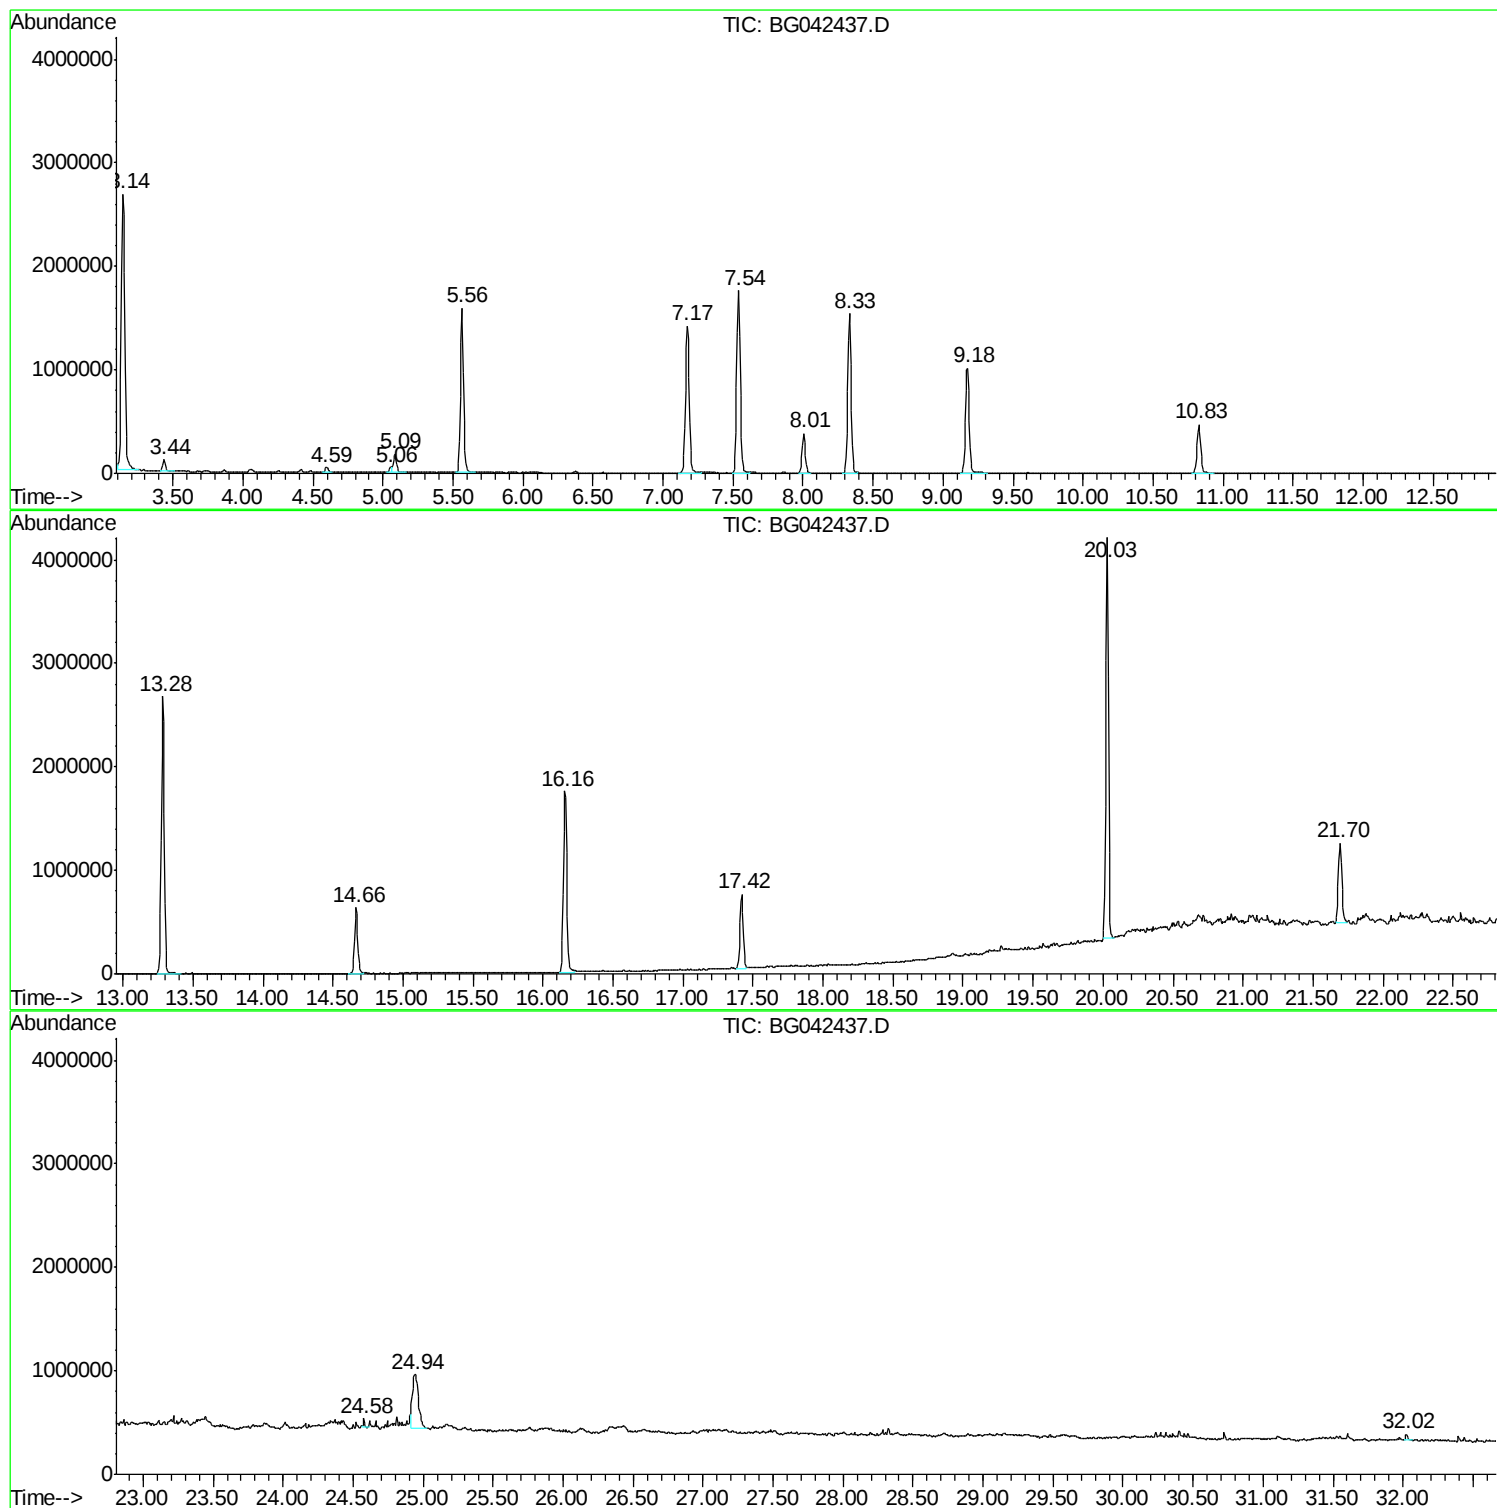

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082319\
Data File : BG042437.D
Acq On : 23 Aug 2019 17:30
Operator : HP/JU
Sample : K4086-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NB-08-082019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082319\
Data File : BG042437.D
Acq On : 23 Aug 2019 17:30
Operator : HP/JU
Sample : K4086-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NB-08-082019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc