


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082319\
 Data File : BG042434.D
 Acq On : 23 Aug 2019 14:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 22 14:29:15 2019

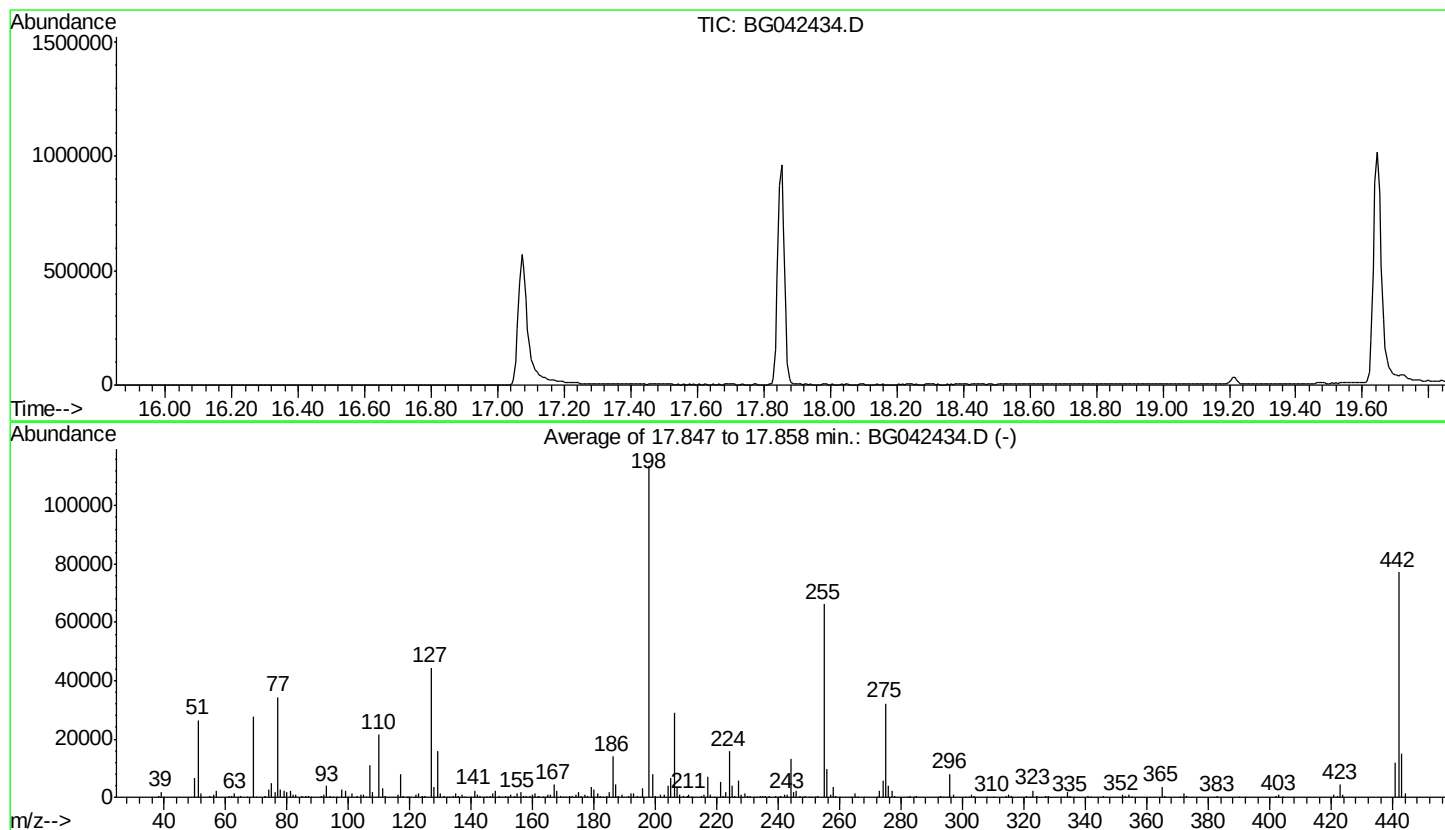

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.3	26458	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	24.5	27890	PASS
70	69	0.00	2	0.6	163	PASS
127	198	10	80	39.1	44445	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	113797	PASS
199	198	5	9	6.8	7792	PASS
275	198	10	60	28.2	32117	PASS
365	198	1	100	3.1	3526	PASS
441	198	0.01	100	10.6	12033	PASS
442	198	50	100	67.9	77240	PASS
443	442	15	24	19.1	14755	PASS