

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082321\
 Data File : BG049934.D
 Acq On : 23 Aug 2021 15:27
 Operator : CG/JU
 Sample : M3463-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-20-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	418	425	435	rBV	363932	612320	2.90%	1.227%
2	7.156	692	701	711	rBV	398519	692372	3.27%	1.387%
3	9.153	1034	1041	1052	rVB	314305	566489	2.68%	1.135%
4	10.804	1315	1322	1333	rVB	148071	252981	1.20%	0.507%
5	13.259	1731	1740	1747	rBV	582996	913481	4.32%	1.830%
6	14.640	1969	1975	1983	rVB2	218026	344457	1.63%	0.690%
7	16.137	2223	2230	2239	rVB	493772	747728	3.54%	1.498%
8	17.395	2438	2444	2451	rBV	267342	406461	1.92%	0.814%
9	19.086	2717	2732	2743	rBV	1969935	7717391	36.50%	15.459%
10	19.227	2743	2756	2762	rVV	2725119	8791112	41.58%	17.609%
11	19.380	2762	2782	2785	rVB	5641275	21142608	100.00%	42.350%
12	19.468	2790	2797	2804	rVB	920296	1502829	7.11%	3.010%
13	20.003	2883	2888	2894	rVB	762076	947545	4.48%	1.898%
14	21.260	3095	3102	3106	rBV2	142777	292859	1.39%	0.587%
15	21.319	3106	3112	3117	rVV	280620	585725	2.77%	1.173%
16	21.383	3118	3123	3130	rVV	713235	998359	4.72%	2.000%
17	21.671	3164	3172	3179	rVB	233296	509544	2.41%	1.021%
18	22.505	3308	3314	3325	rVB4	177487	459196	2.17%	0.920%
19	24.908	3716	3723	3733	rVB3	147581	435180	2.06%	0.872%
20	29.484	4493	4502	4520	rVB10	182561	823968	3.90%	1.650%
21	30.418	4650	4661	4678	rVB10	234272	1180622	5.58%	2.365%


Sum of corrected areas: 49923227

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082321\
Data File : BG049934.D
Acq On : 23 Aug 2021 15:27
Operator : CG/JU
Sample : M3463-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-20-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

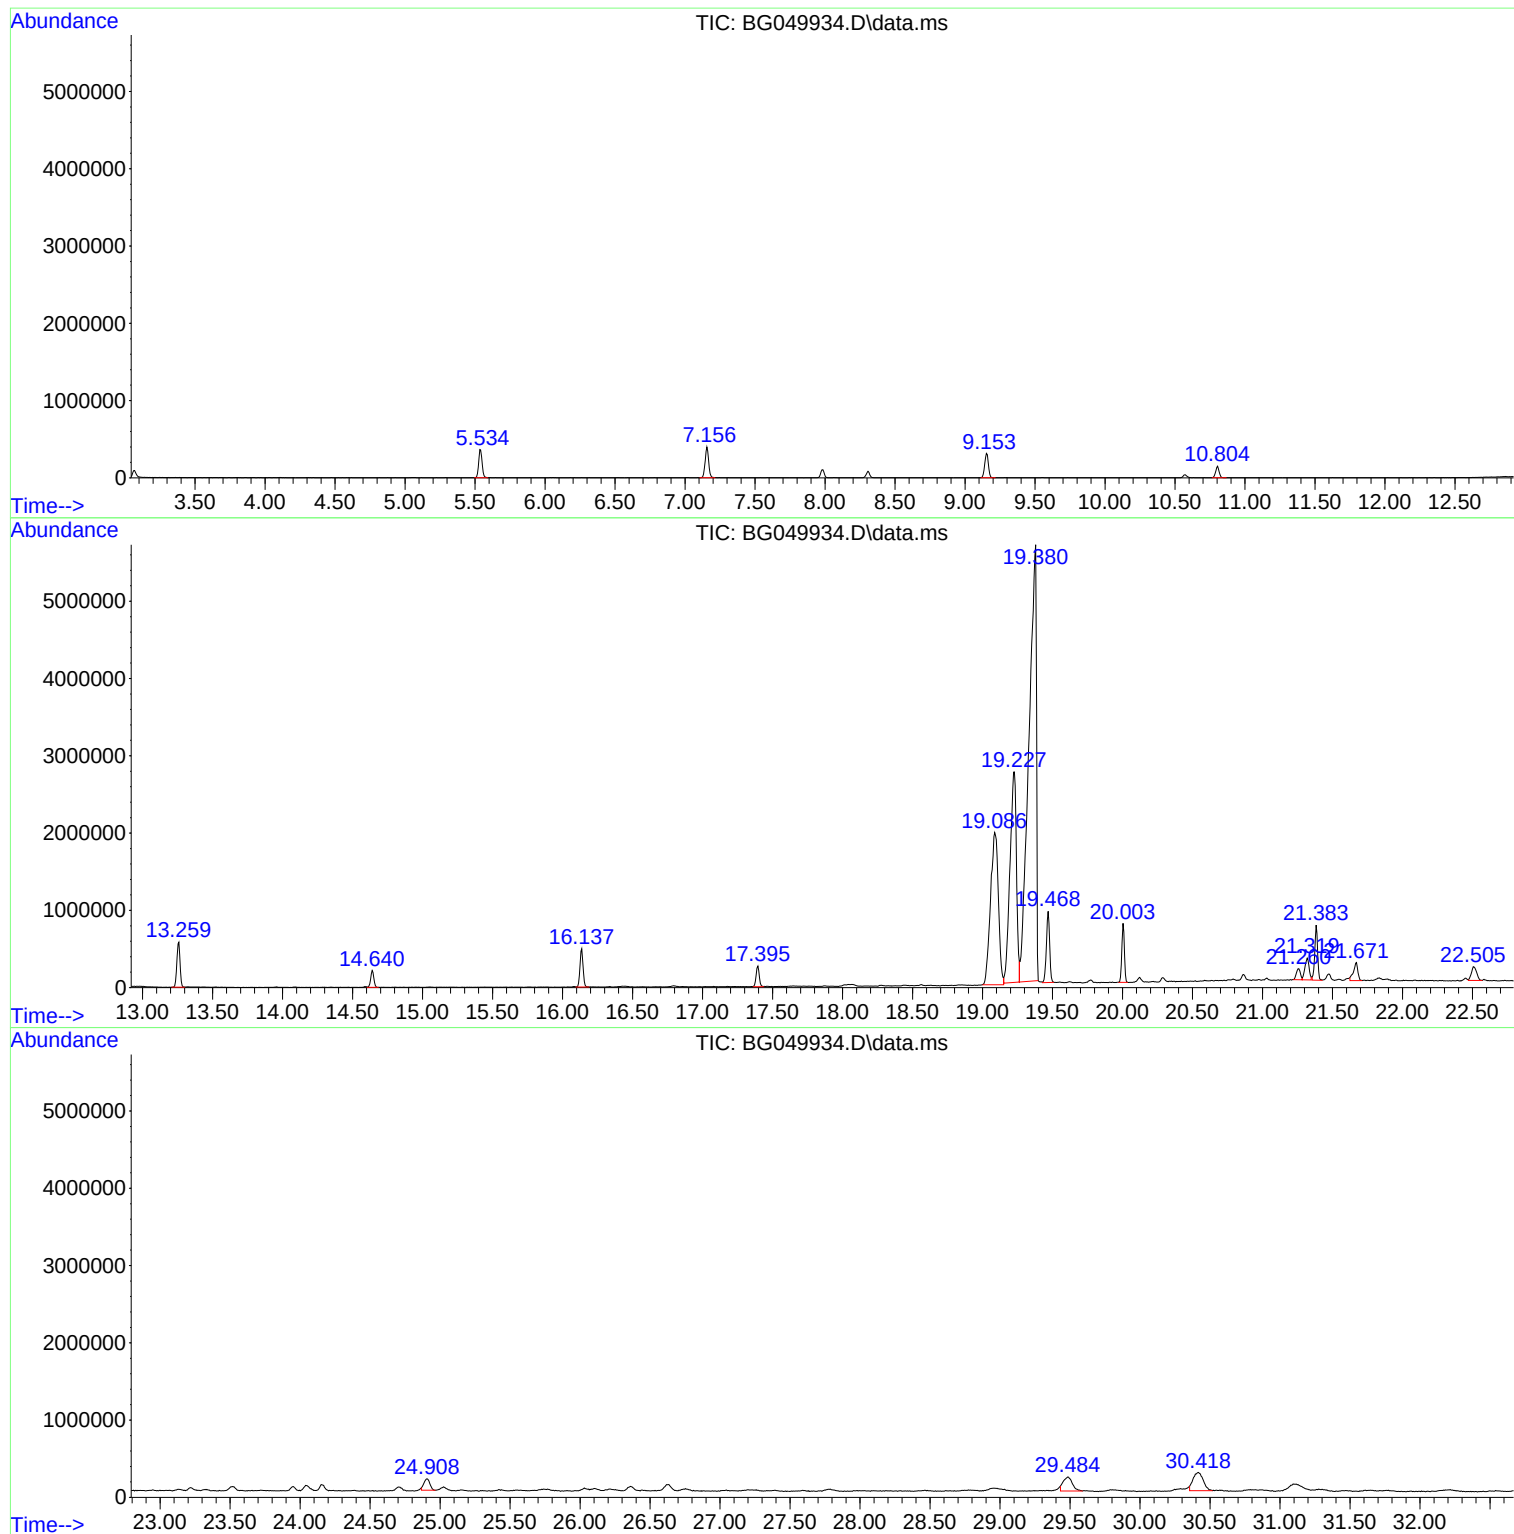

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082321\
Data File : BG049934.D
Acq On : 23 Aug 2021 15:27
Operator : CG/JU
Sample : M3463-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-20-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082321\
Data File : BG049934.D
Acq On : 23 Aug 2021 15:27
Operator : CG/JU
Sample : M3463-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-20-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------