


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082321\
 Data File : BG049930.D
 Acq On : 23 Aug 2021 11:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 23 16:13:24 2021

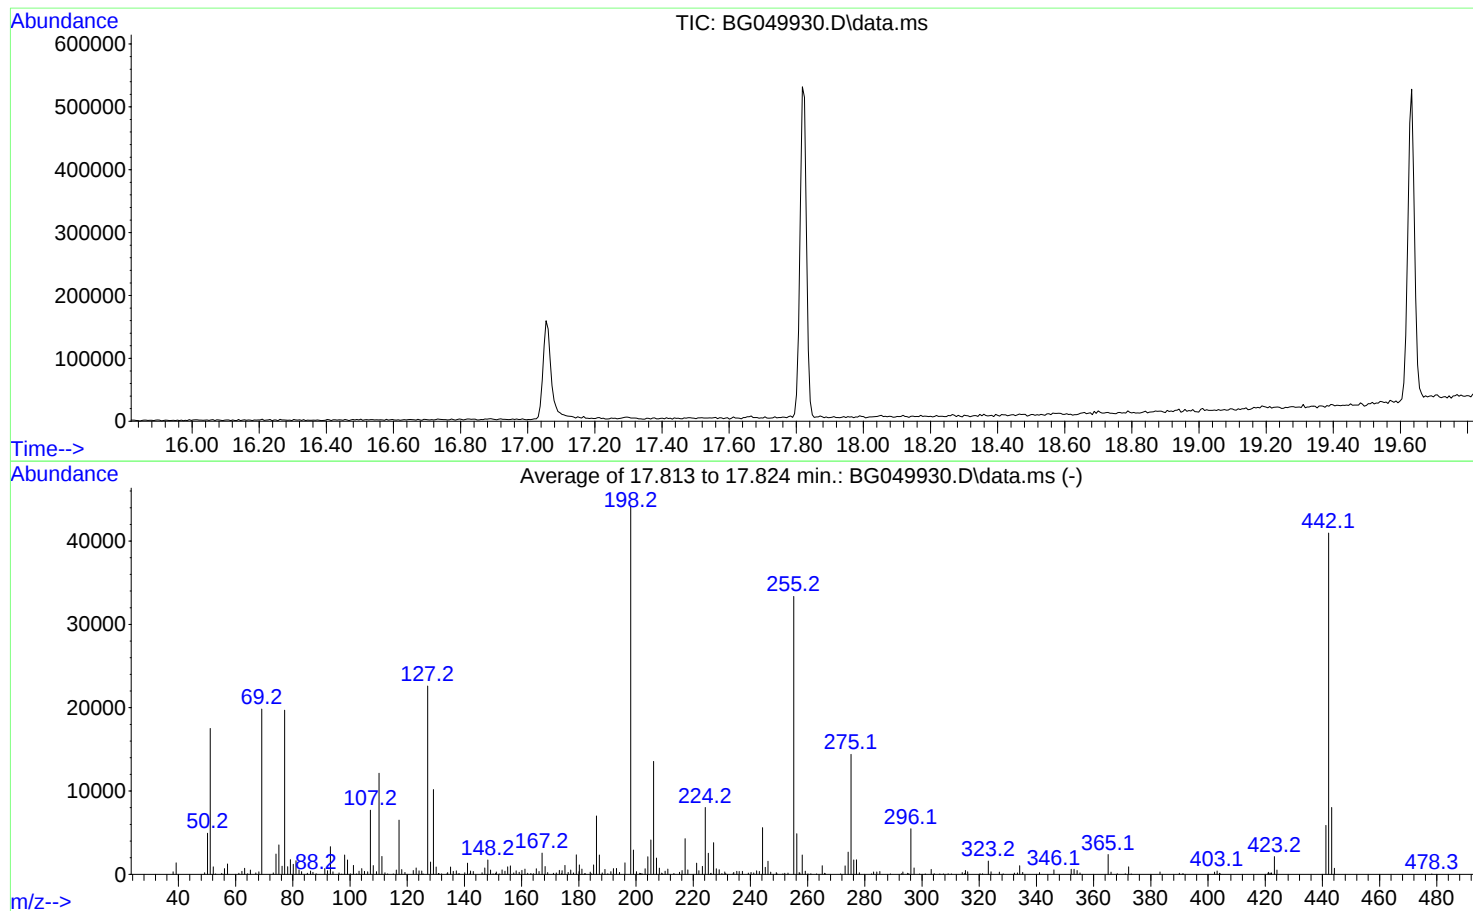




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	17507	PASS
68	69	0.00	2	1.6	312	PASS
69	198	0.00	100	44.9	19837	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	22592	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44147	PASS
199	198	5	9	6.6	2927	PASS
275	198	10	60	32.6	14407	PASS
365	198	1	100	5.4	2389	PASS
441	198	0.01	100	13.3	5877	PASS
442	442	50	100	100.0	40965	PASS
443	442	15	24	19.6	8036	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082321\
Data File : BG049930.D
Acq On : 23 Aug 2021 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 23 12:21:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 21 05:13:22 2021
Response via : Initial Calibration

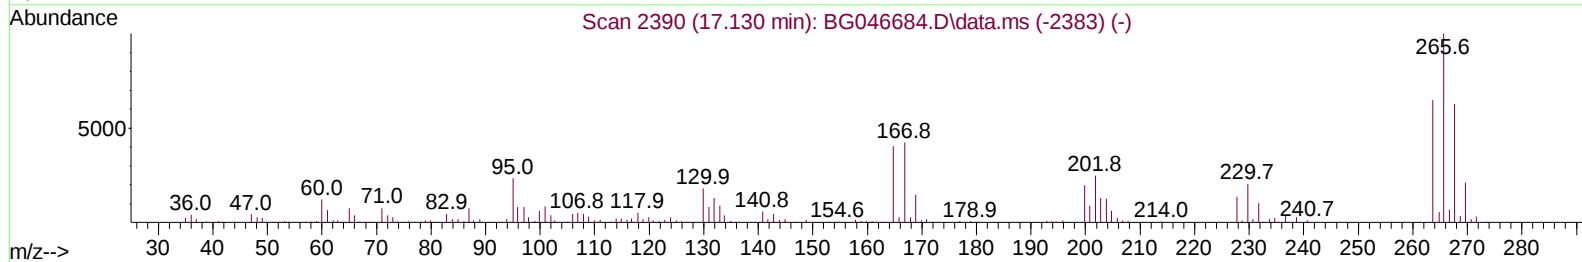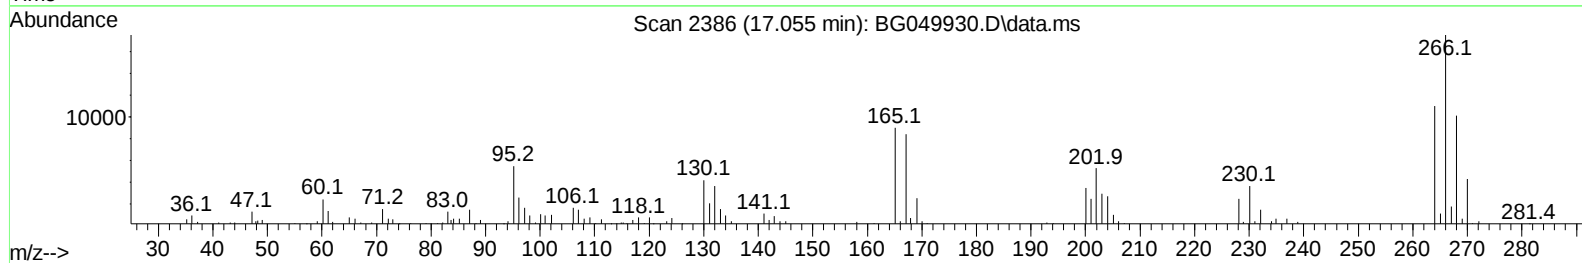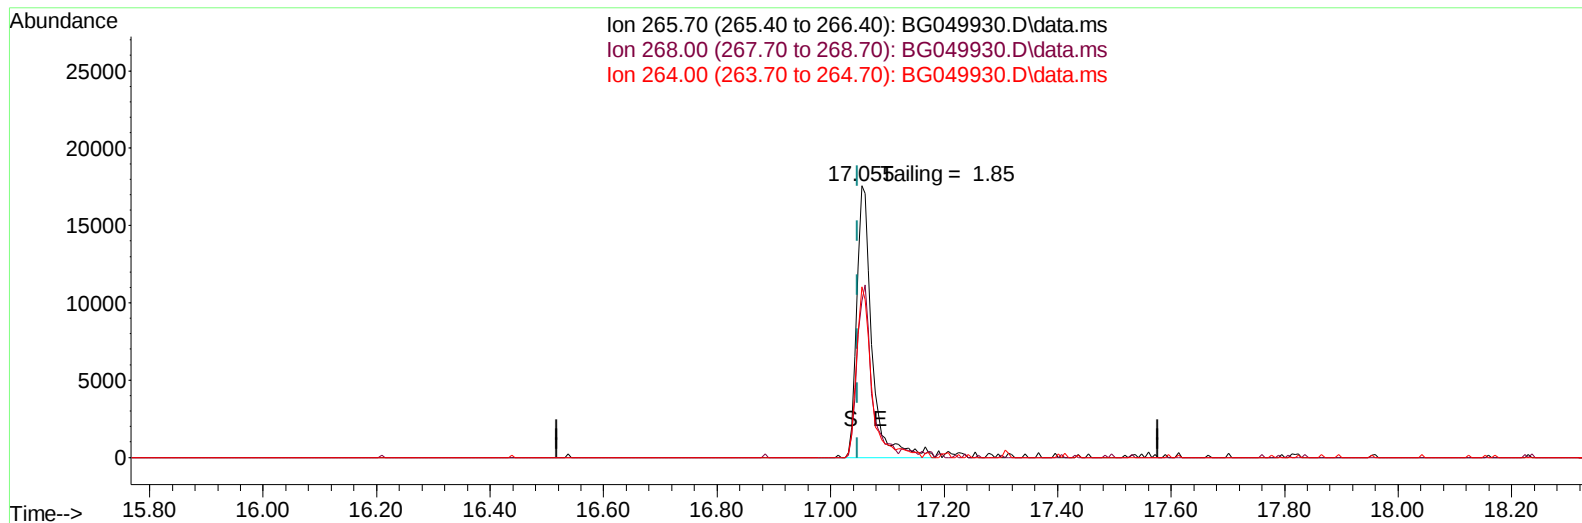

TIC: BG049930.D\data.ms

(70) Pentachlorophenol (C)

17.055min (+ 0.008) 58621.07 ng




response 30436

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	57.71
264.00	61.30	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082321\
Data File : BG049930.D
Acq On : 23 Aug 2021 11:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 23 12:21:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 21 05:13:22 2021
Response via : Initial Calibration

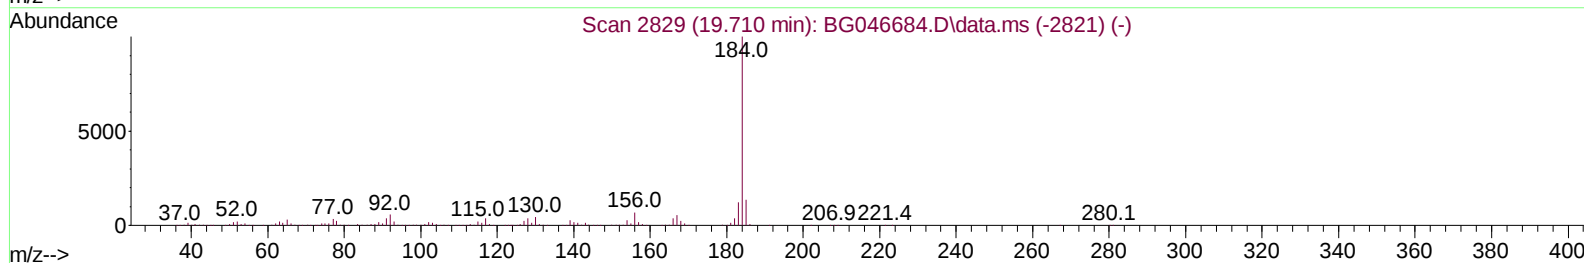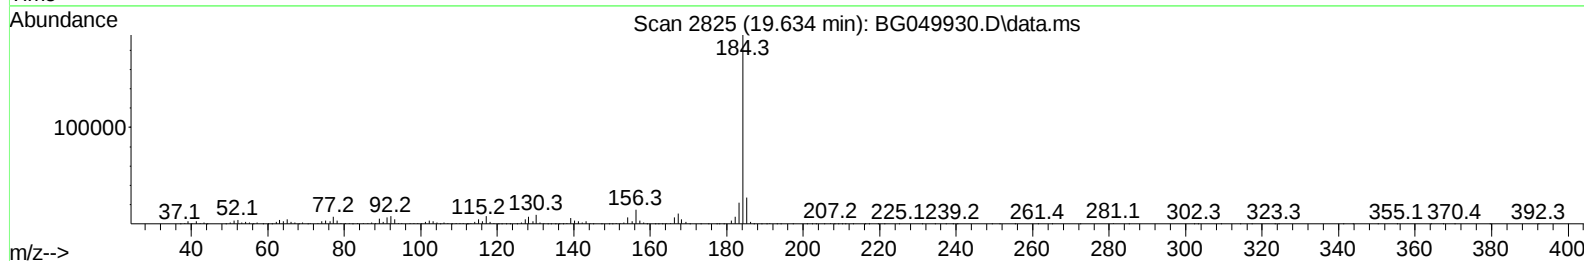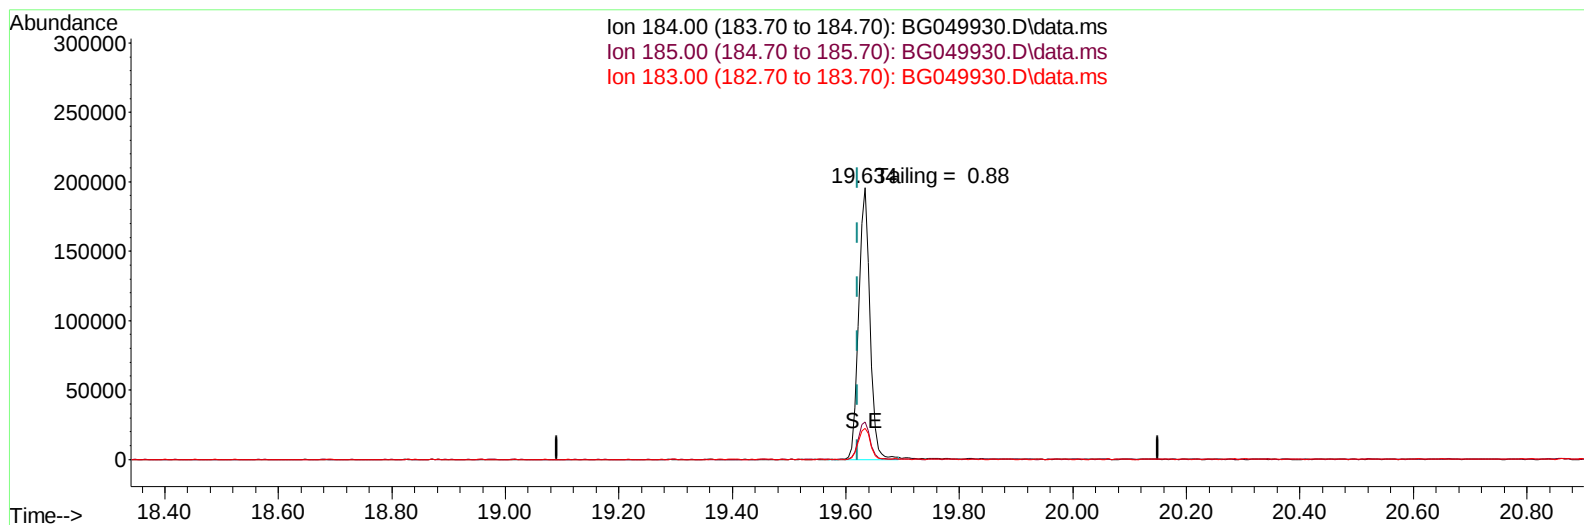

TIC: BG049930.D\data.ms

(77) Benzidine

19.634min (+ 0.013) 66281.90 ng

response 270027

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.89
183.00	11.70	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2021	BNA_G	BG049930.D
Compound Name	Response	Retention Time
DDT	116212	20.86
DDD	9155	20.421
DDE	575	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9730	125942	7.73

Instrument :
BNA_G
ClientSampleId :
DFTPP