


Data Path : Z:\HPCHEM1\BNA G\Data\BG082416\
 Data File : BG023880.D
 Acq On : 24 Aug 2016 9:07
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 24 17:42:04 2016

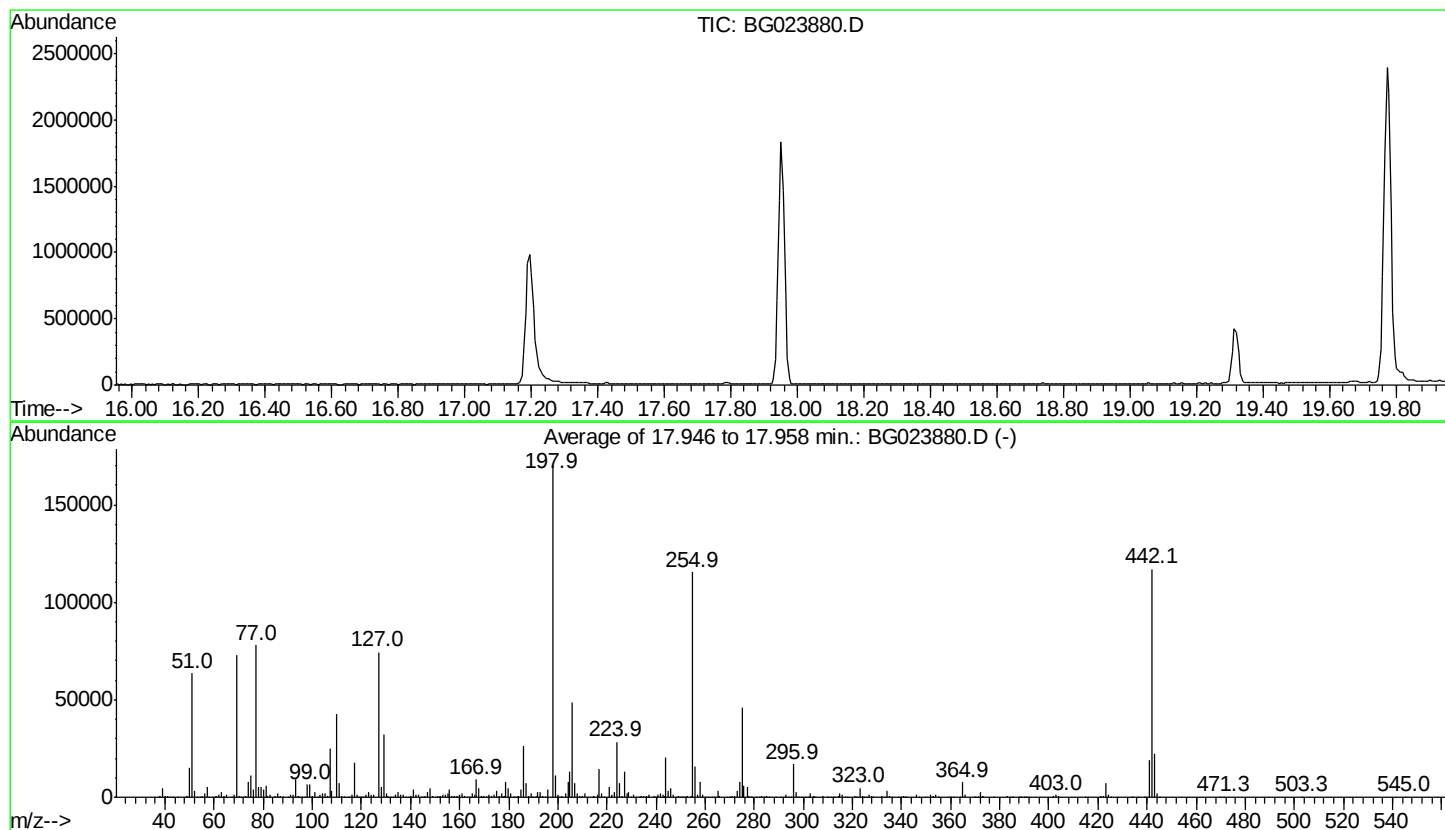

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	63504	PASS
68	69	0.00	2	1.7	1240	PASS
69	198	0.00	100	42.9	72926	PASS
70	69	0.00	2	0.5	399	PASS
127	198	10	80	43.6	74189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	170048	PASS
199	198	5	9	6.6	11178	PASS
275	198	10	60	27.2	46208	PASS
365	198	1	100	4.5	7709	PASS
441	442	0.01	24	16.3	19105	PASS
442	198	50	100	68.7	116901	PASS
443	442	15	24	19.1	22308	PASS