

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082417\
 Data File : BG028457.D
 Acq On : 24 Aug 2017 12:12
 Operator : SJ/JU
 Sample : PB101780BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK80

Quant Time: Aug 25 01:08:05 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 01:07:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	31384	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	129847	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	93798	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.70	188	266646	20.00	ng/ul	0.00
75) Chrysene-d12	22.03	240	330482	20.00	ng/ul	0.00
83) Perylene-d12	25.54	264	319612	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.82	96	4969	7.37	ng/uL	0.00
5) Phenol-d5	7.50	99	95577	27.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.65	67	61738	28.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.87	132	69833	32.12	ng/ul	0.00
13) 4-Methylphenol-d8	9.04	113	80586	27.97	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	37463	36.90	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	43416	39.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	79690	34.60	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	104592	40.80	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	329948	39.55	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	331218	35.21	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	48706	36.72	ng/ul	0.00
57) Fluorene-d10	15.94	176	257029	34.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	53843	31.08	ng/ul	0.00
70) Anthracene-d10	17.80	188	459914	35.97	ng/ul	0.00
76) Pyrene-d10	20.07	212	548055	32.34	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	550108	36.77	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.03	70	2818	1.207	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082417\
Data File : BG028457.D
Acq On : 24 Aug 2017 12:12
Operator : SJ/JU
Sample : PB101780BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK80

Quant Time: Aug 25 01:08:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 01:07:54 2017
Response via : Initial Calibration

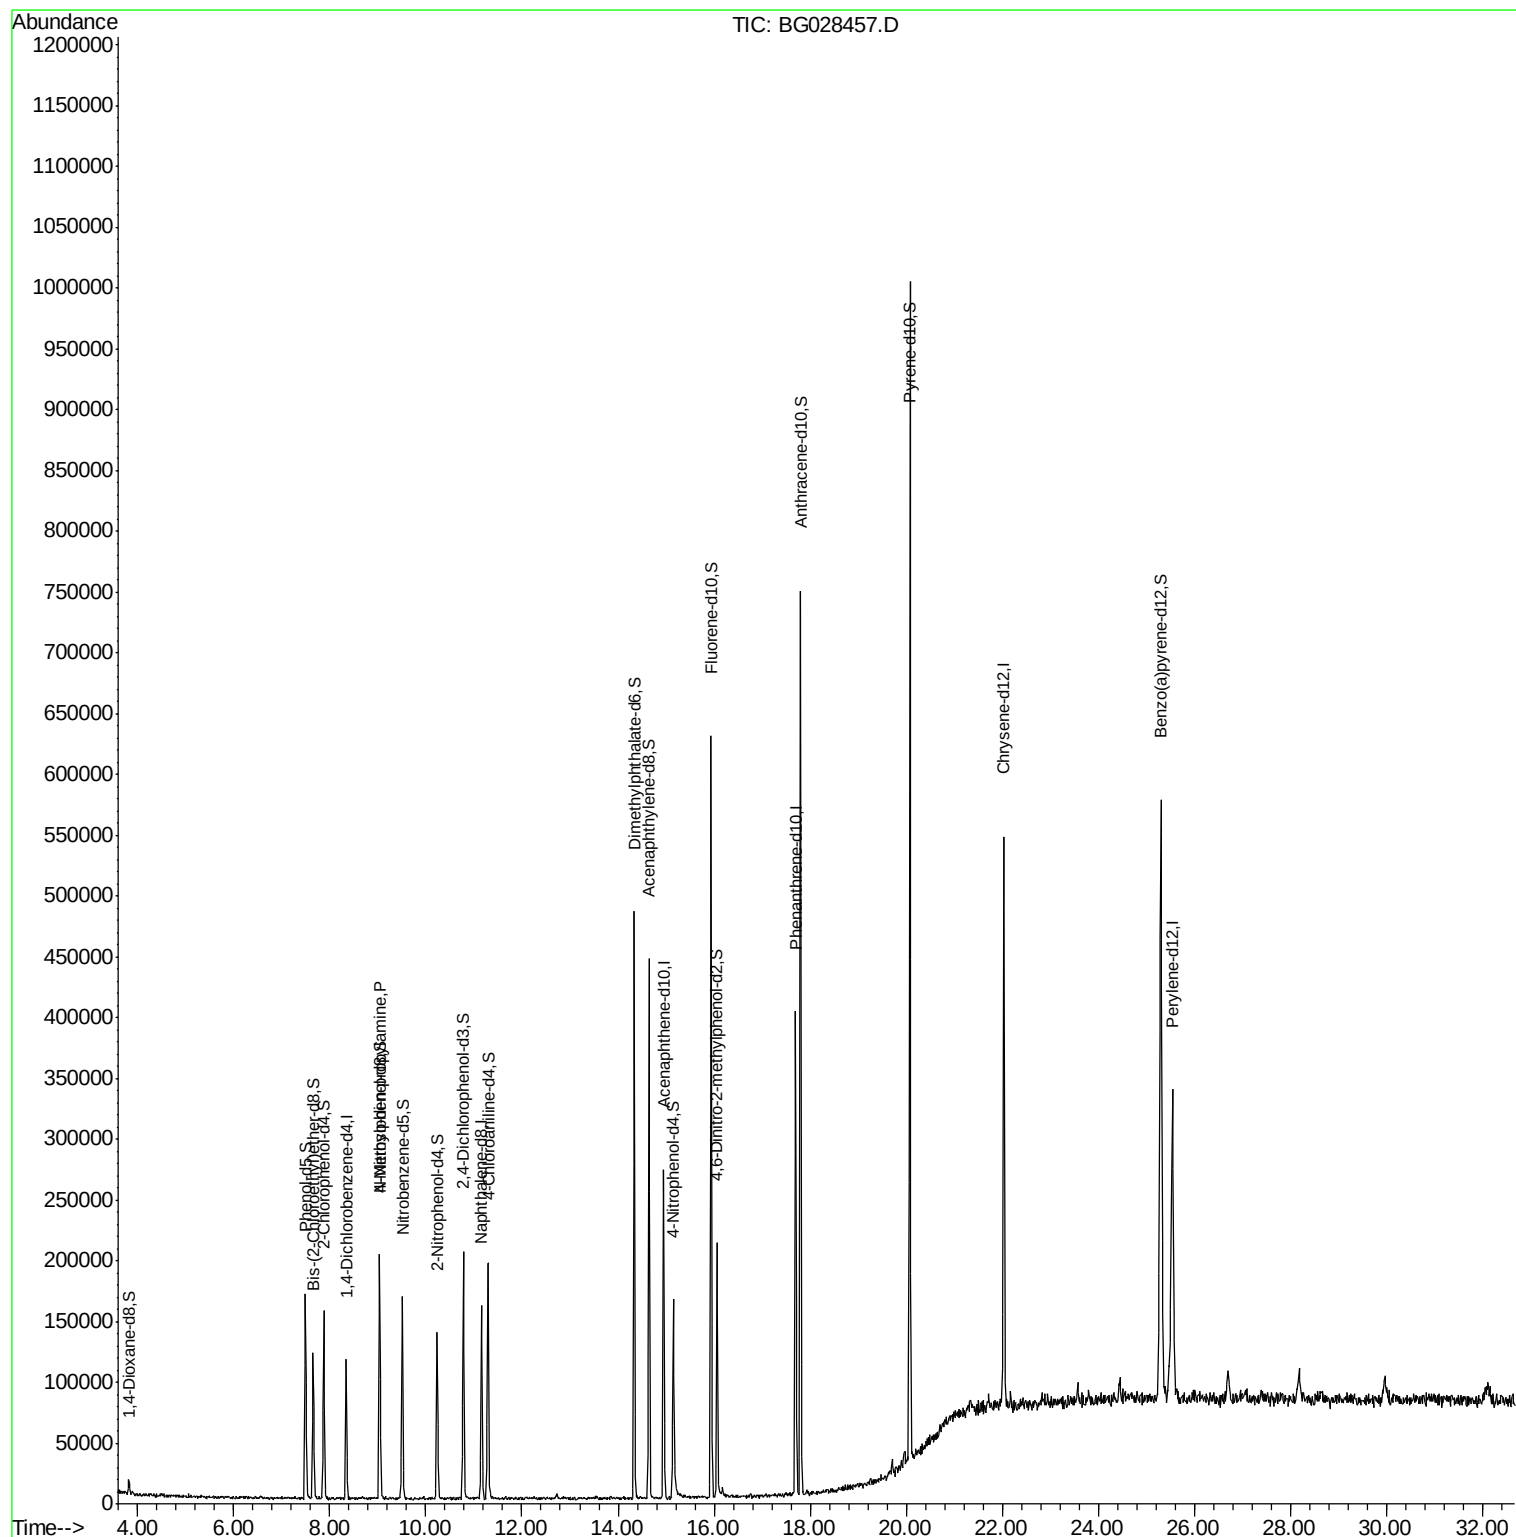

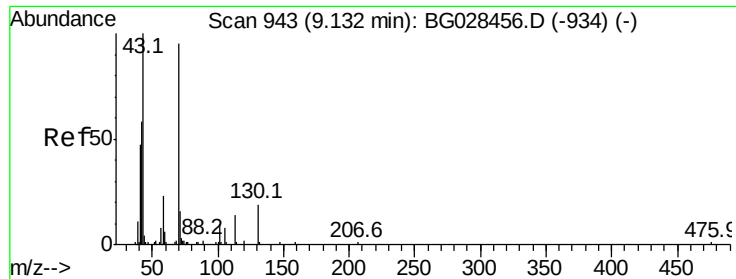

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.207 ng/ul
 RT: 9.03 min Scan# 927
 Delta R.T. -0.10 min
 Lab File: BG028457.D
 Acq: 24 Aug 2017 12:12

Instrument :
 BNA_G
 ClientSampleId :
 SBLK80

Tot Ion:	70	Resp:	2818
Ion	Ratio	Lower	Upper
70	100		
42	261.8	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

