

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082417\
 Data File : BG028472.D
 Acq On : 24 Aug 2017 22:45
 Operator : SJ/JU
 Sample : I4840-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0AH9

Quant Time: Aug 25 03:53:14 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 03:52:53 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	44115	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	187277	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	135634	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.70	188	353284	20.00	ng/ul	0.00
75) Chrysene-d12	22.03	240	420431	20.00	ng/ul	0.00
83) Perylene-d12	25.52	264	411197	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.82	96	2460	2.60	ng/uL	0.00
5) Phenol-d5	7.49	99	58058	11.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.65	67	38218	12.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.87	132	42590	13.93	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	45406	11.21	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	22837	15.59	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	26101	16.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	49960	15.04	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	83368	22.55	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	179554	14.88	ng/ul	0.00
46) Acenaphthylene-d8	14.64	160	200022	14.71	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	25118	13.10	ng/ul	0.00
57) Fluorene-d10	15.94	176	148729	13.74	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.05	200	27890	12.15	ng/ul	0.00
70) Anthracene-d10	17.79	188	261040	15.41	ng/ul	0.00
76) Pyrene-d10	20.07	212	318662	14.78	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.28	264	306272	15.91	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.38	163	34765	3.130	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082417\
Data File : BG028472.D
Acq On : 24 Aug 2017 22:45
Operator : SJ/JU
Sample : I4840-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B0AH9

Quant Time: Aug 25 03:53:14 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 03:52:53 2017
Response via : Initial Calibration

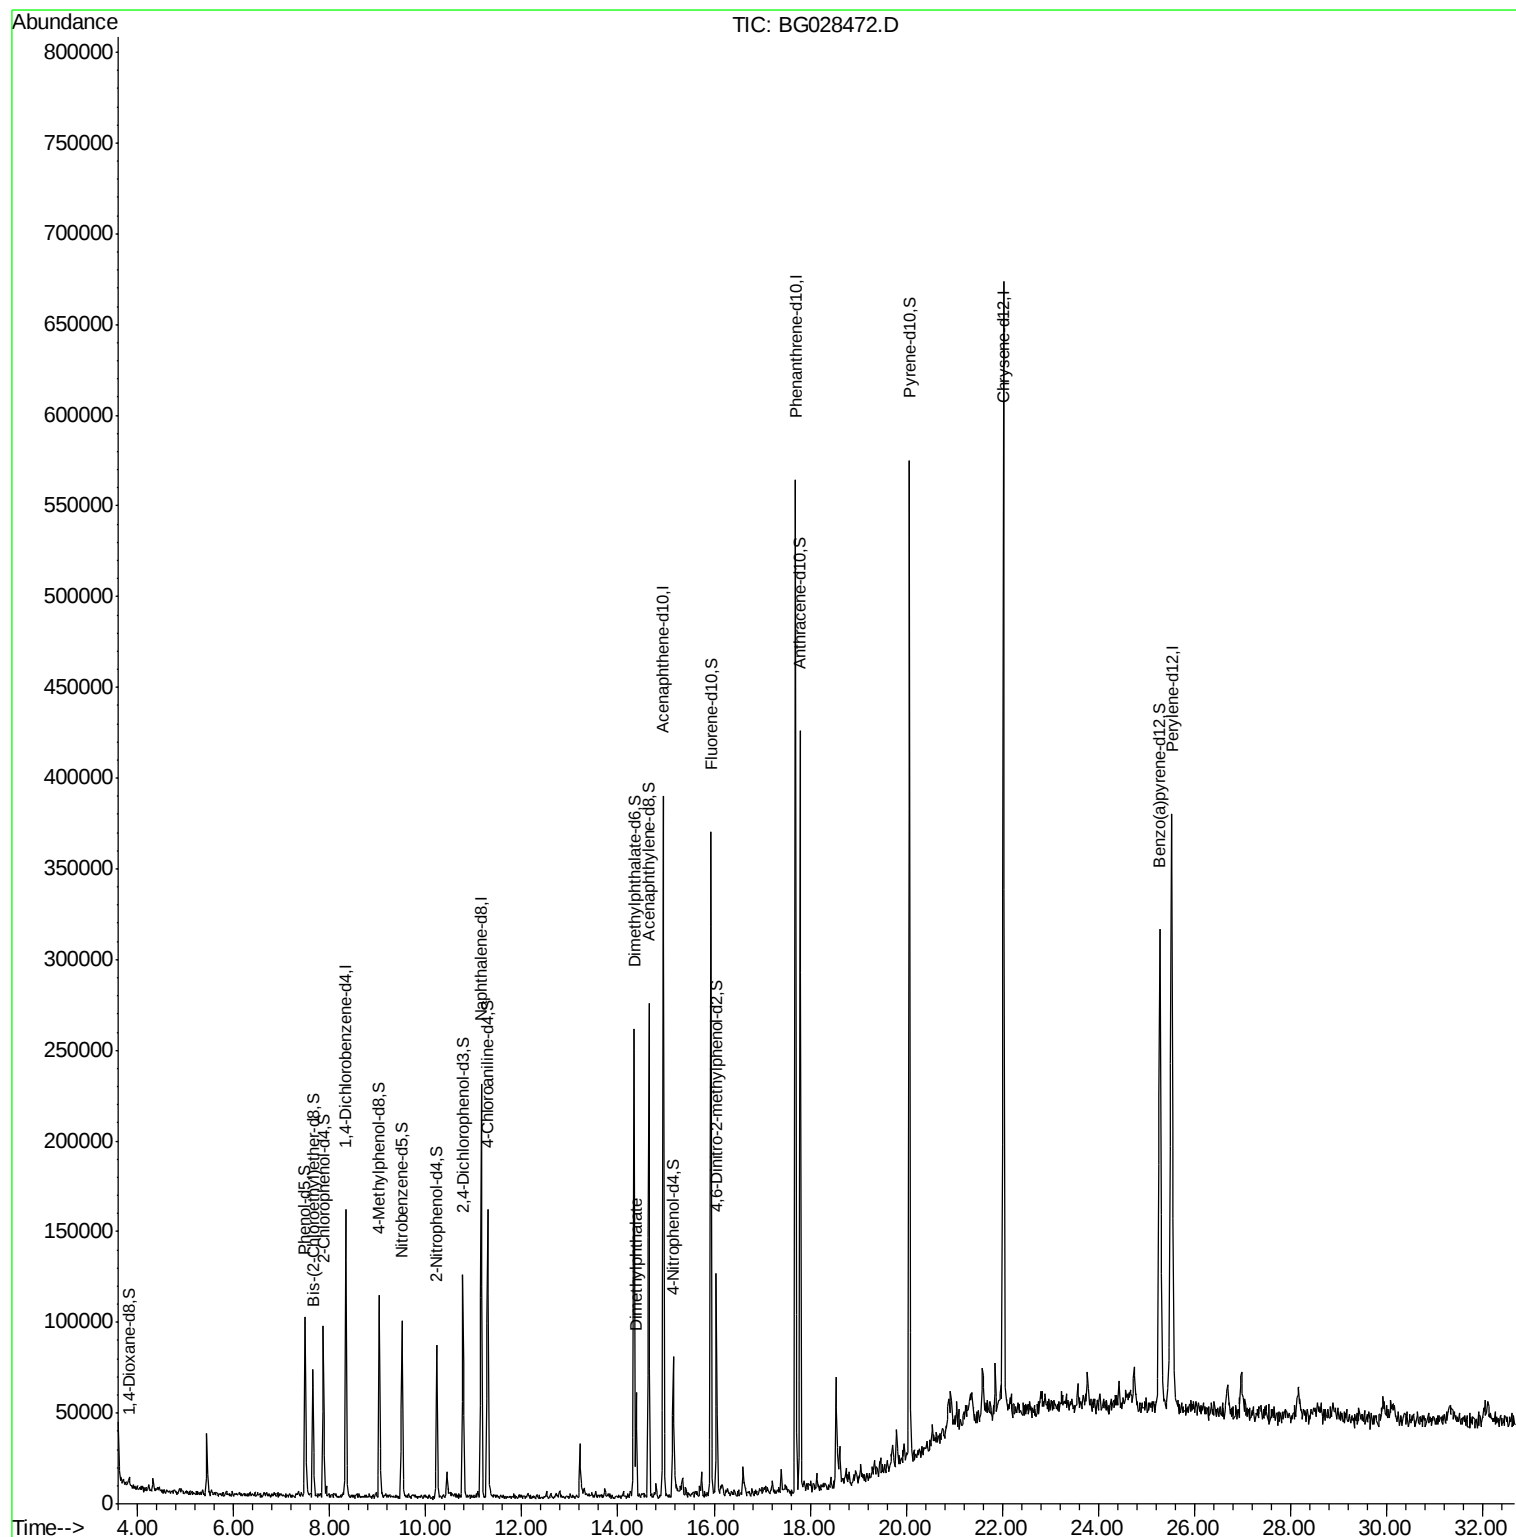

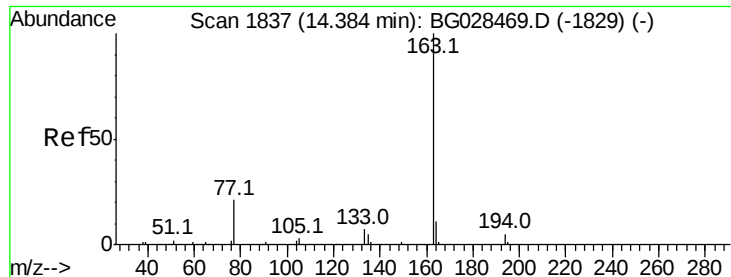

#44

Dimethylphthalate

Concen: 3.130 ng/ul

RT: 14.38 min Scan# 1837

Delta R.T. 0.00 min

Lab File: BG028472.D

Acq: 24 Aug 2017 22:45

Instrument :

BNA_G

ClientSampleId :

B0AH9


Tot Ion:163 Resp: 34765

Ion Ratio Lower Upper

163 100

194 5.0 3.4 5.0

164 9.8 9.0 13.4

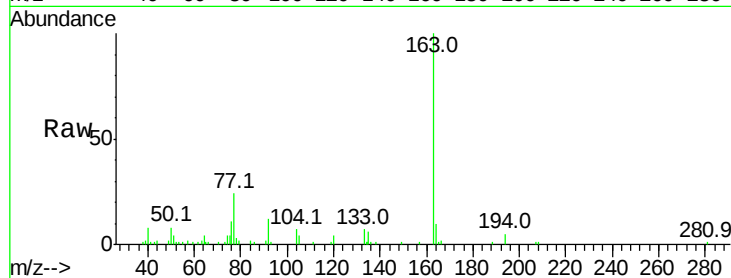

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

