
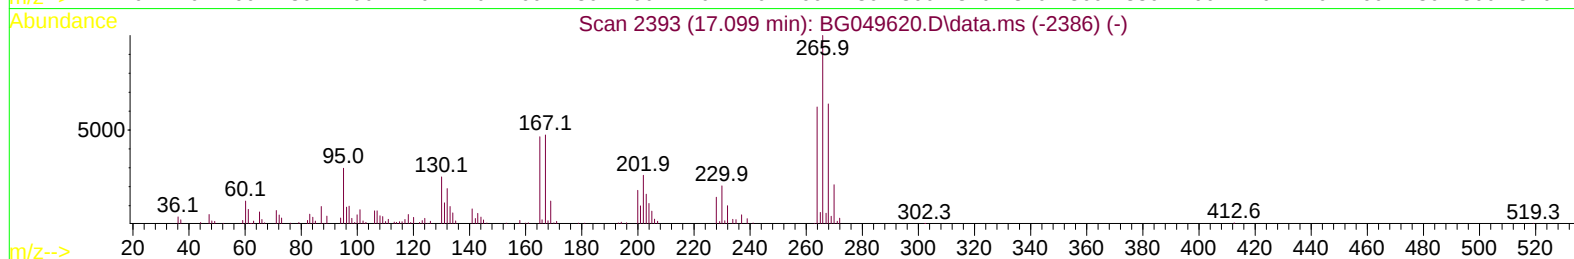
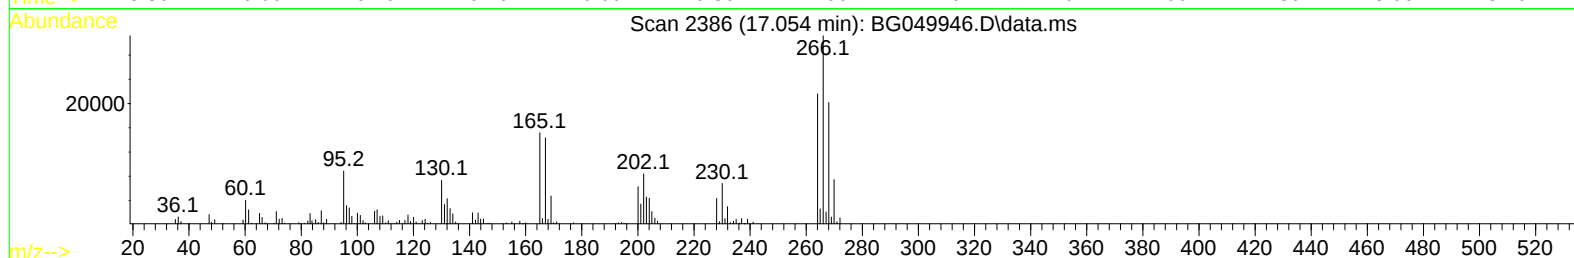


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049946.D
Acq On : 24 Aug 2021 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 11:13:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 16:13:24 2021
Response via : Initial Calibration

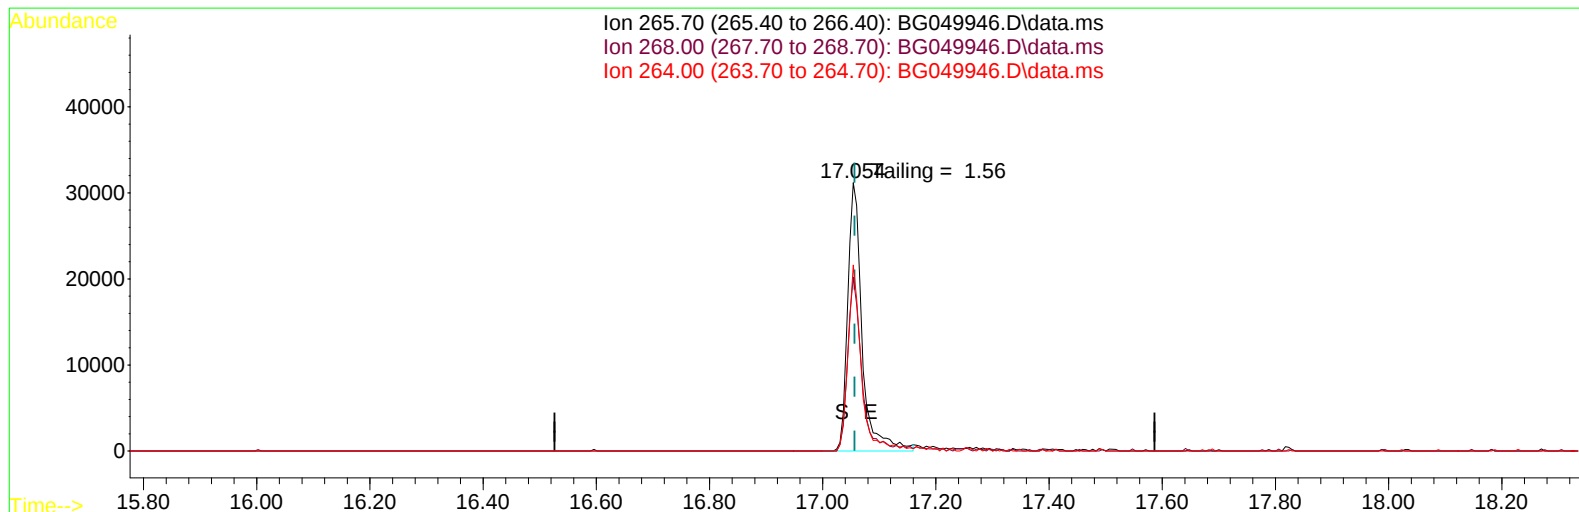

TIC: BG049946.D\data.ms

(70) Pentachlorophenol (C)




17.054min (-0.002) 17628.98 ng

response 54794

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.71
264.00	61.30	69.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049946.D
 Acq On : 24 Aug 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 11:13:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 16:13:24 2021
 Response via : Initial Calibration

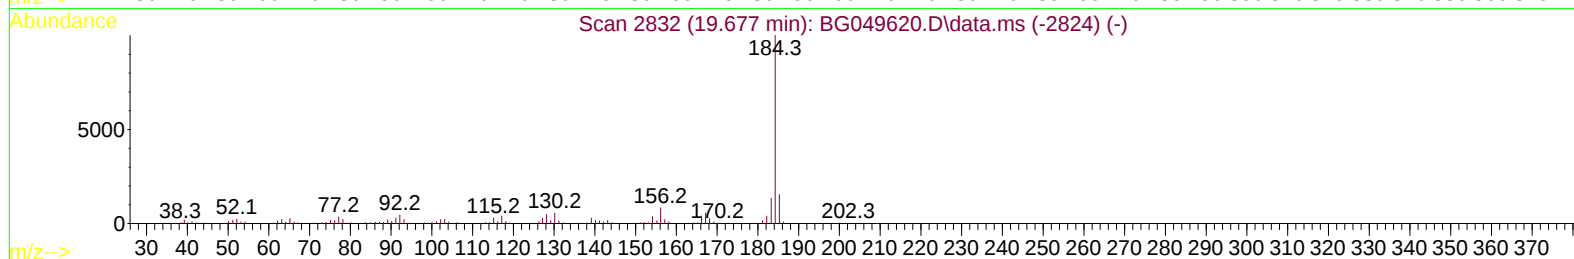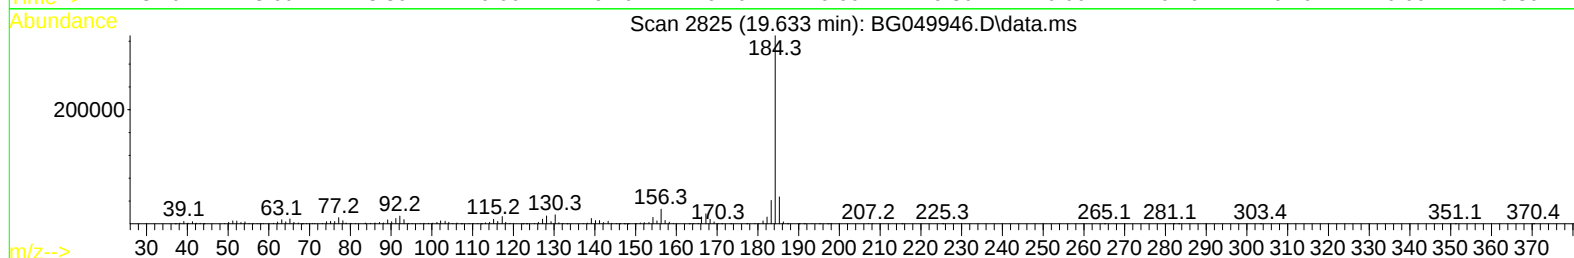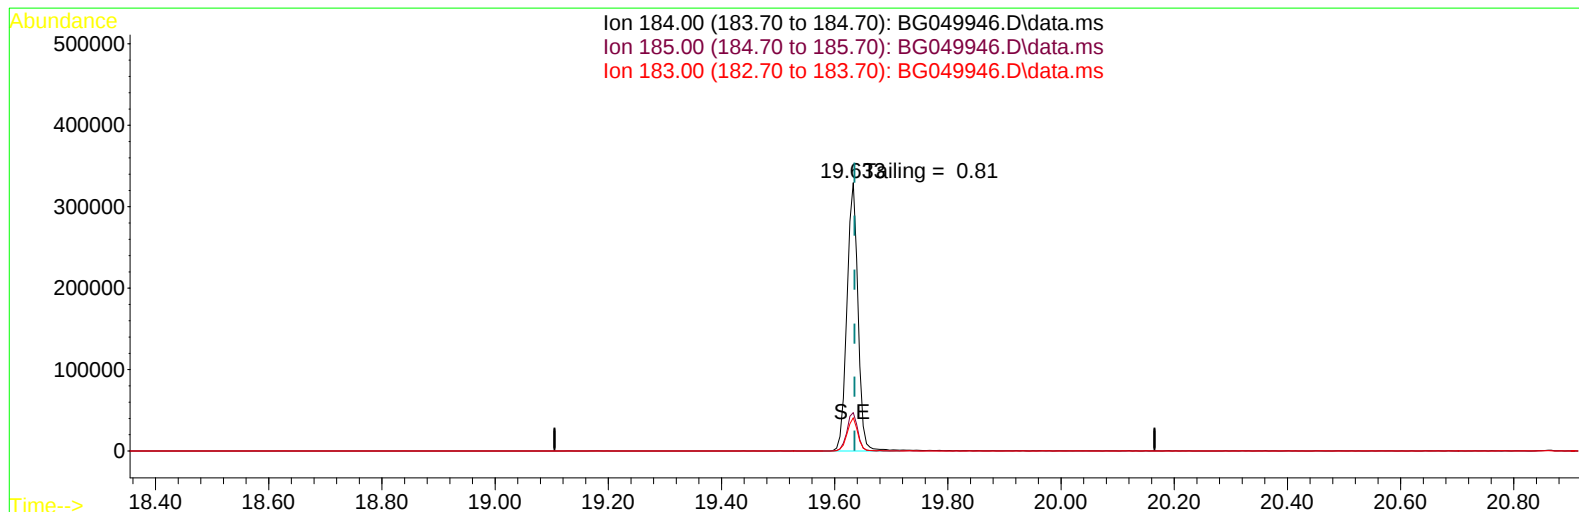

TIC: BG049946.D\data.ms

(77) Benzidine**19.633min (-0.002) 310921.32 ng****response 446122**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.34
183.00	11.70	12.44
0.00	0.00	0.00