

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049950.D
 Acq On : 24 Aug 2021 13:19
 Operator : CG/JU
 Sample : M3463-29
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-25-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.259	371	378	387	rVB	75317	133046	9.09%	1.520%
2	5.529	416	424	434	rBV	407765	696483	47.60%	7.955%
3	7.150	692	700	714	rVB	455175	805907	55.08%	9.205%
4	7.973	834	840	847	rBV	109050	186055	12.71%	2.125%
5	9.148	1033	1040	1051	rVB	287881	512652	35.03%	5.855%
6	10.557	1274	1280	1294	rBV2	64291	131634	9.00%	1.503%
7	10.798	1314	1321	1327	rBV	145748	262254	17.92%	2.995%
8	13.254	1729	1739	1746	rBV	739573	1140690	77.95%	13.028%
9	14.076	1875	1879	1887	rBV2	16410	27832	1.90%	0.318%
10	14.634	1966	1974	1982	rVB	231902	372232	25.44%	4.251%
11	16.132	2223	2229	2237	rBV	740804	1111716	75.97%	12.698%
12	17.389	2438	2443	2449	rBV	279545	441325	30.16%	5.041%
13	17.431	2449	2450	2461	rVB4	16659	22310	1.52%	0.255%
14	18.041	2551	2554	2558	rVB4	14010	16964	1.16%	0.194%
15	18.735	2668	2672	2679	rBV8	24397	36318	2.48%	0.415%
16	19.445	2789	2793	2797	rVB	46978	63315	4.33%	0.723%
17	19.680	2830	2833	2837	rVB5	10632	15312	1.05%	0.175%
18	20.003	2880	2888	2894	rBV	1116355	1463284	100.00%	16.713%
19	20.297	2936	2938	2943	rVB6	20139	22266	1.52%	0.254%
20	20.644	2994	2997	3001	rBV5	15725	21857	1.49%	0.250%
21	21.026	3060	3062	3065	rVB4	15619	15173	1.04%	0.173%
22	21.243	3095	3099	3105	rVB7	30725	47314	3.23%	0.540%
23	21.302	3105	3109	3118	rVB6	41803	97938	6.69%	1.119%
24	21.378	3119	3122	3126	rVB	35917	43580	2.98%	0.498%
25	21.478	3134	3139	3141	rBV6	27164	48946	3.34%	0.559%
26	21.537	3145	3149	3153	rVB	112782	151418	10.35%	1.729%
27	21.666	3165	3171	3178	rBV	250014	409990	28.02%	4.683%
28	22.447	3300	3304	3307	rBV4	22834	38623	2.64%	0.441%
29	24.903	3713	3722	3731	rBV	152987	418924	28.63%	4.785%


Sum of corrected areas: 8755358

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049950.D
Acq On : 24 Aug 2021 13:19
Operator : CG/JU
Sample : M3463-29
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-25-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

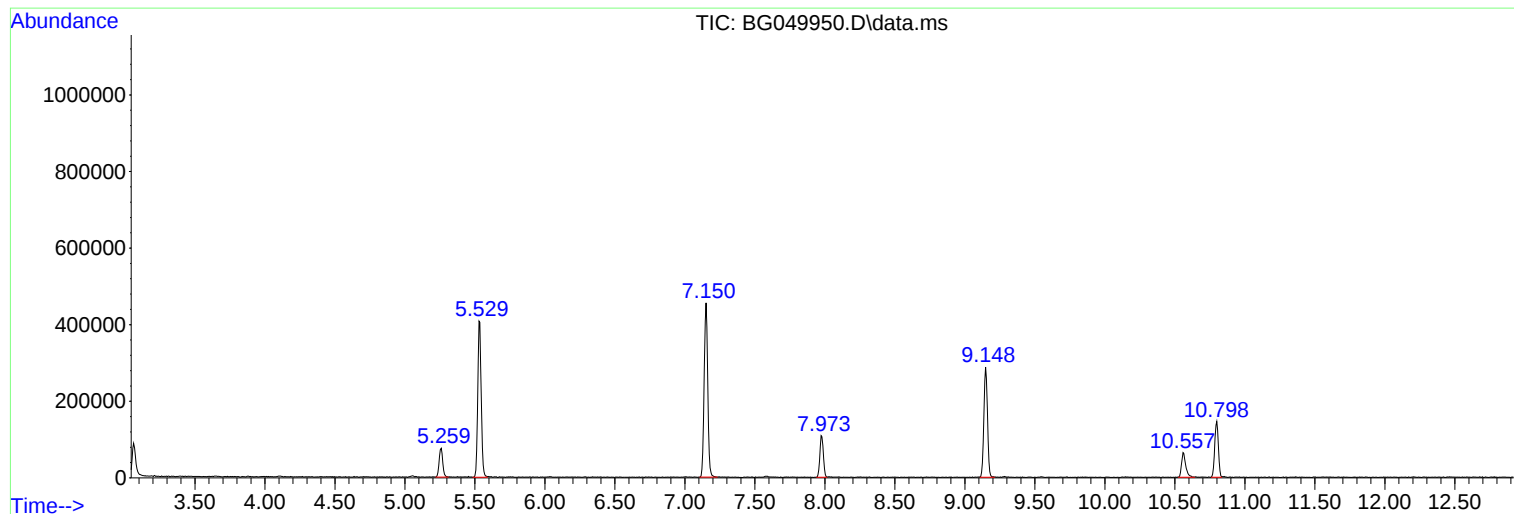

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049950.D
Acq On : 24 Aug 2021 13:19
Operator : CG/JU
Sample : M3463-29
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-25-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049950.D
Acq On : 24 Aug 2021 13:19
Operator : CG/JU
Sample : M3463-29
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-25-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------