

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049952.D
 Acq On : 24 Aug 2021 14:41
 Operator : CG/JU
 Sample : M3463-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-18-0204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.097	175	180	189	rVB2	8072	15313	1.89%	0.151%
2	4.644	267	273	282	rBV3	19933	37869	4.66%	0.374%
3	5.531	417	424	435	rBV	352231	600146	73.92%	5.928%
4	6.641	608	613	618	rVB5	6964	12659	1.56%	0.125%
5	7.146	687	699	710	rBV	373903	683758	84.22%	6.754%
6	7.581	768	773	776	rBV2	5709	9227	1.14%	0.091%
7	7.974	832	840	849	rVB	106051	178334	21.97%	1.762%
8	9.149	1032	1040	1047	rBV	238706	437101	53.84%	4.318%
9	10.559	1273	1280	1297	rBV	110340	222745	27.44%	2.200%
10	10.794	1308	1320	1326	rBV	143283	260807	32.12%	2.576%
11	10.847	1326	1329	1333	rVB4	7815	12409	1.53%	0.123%
12	12.462	1599	1604	1608	rBV3	6615	9983	1.23%	0.099%
13	13.250	1730	1738	1746	rBV	479258	734247	90.44%	7.253%
14	13.514	1779	1783	1788	rBV6	9818	15136	1.86%	0.150%
15	13.955	1854	1858	1865	rBV3	5581	10711	1.32%	0.106%
16	14.084	1875	1880	1887	rVB3	9340	14653	1.80%	0.145%
17	14.366	1923	1928	1932	rBV2	14453	24895	3.07%	0.246%
18	14.636	1968	1974	1981	rVB	240730	362924	44.70%	3.585%
19	15.035	2036	2042	2046	rBV6	5109	9816	1.21%	0.097%
20	15.682	2146	2152	2156	rBV5	4602	9341	1.15%	0.092%
21	16.075	2214	2219	2222	rBV6	8002	12183	1.50%	0.120%
22	16.128	2222	2228	2236	rVV	533542	811882	100.00%	8.020%
23	16.334	2259	2263	2265	rBV2	8210	11344	1.40%	0.112%
24	16.357	2265	2267	2271	rVB5	10538	12909	1.59%	0.128%
25	16.516	2290	2294	2299	rVB5	6233	10212	1.26%	0.101%
26	16.845	2346	2350	2354	rBV4	8146	10911	1.34%	0.108%
27	17.039	2380	2383	2387	rBV5	8108	10906	1.34%	0.108%
28	17.121	2393	2397	2402	rBV5	8114	11985	1.48%	0.118%
29	17.174	2402	2406	2409	rVV5	6064	8868	1.09%	0.088%
30	17.209	2409	2412	2417	rVB3	7489	11513	1.42%	0.114%
31	17.385	2436	2442	2447	rBV	276361	444023	54.69%	4.386%
32	17.432	2447	2450	2457	rVV	89141	124972	15.39%	1.235%
33	17.520	2460	2465	2470	rVV2	16265	24428	3.01%	0.241%
34	17.585	2474	2476	2481	rVB5	7485	9680	1.19%	0.096%
35	17.796	2508	2512	2519	rVV4	11131	21400	2.64%	0.211%
36	17.867	2520	2524	2527	rVV4	12780	15103	1.86%	0.149%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049952.D
 Acq On : 24 Aug 2021 14:41
 Operator : CG/JU
 Sample : M3463-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-18-0204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.967	2537	2541	2548	rVB7	8689	15838	1.95%	0.156%
38	18.037	2550	2553	2558	rBV3	21415	25163	3.10%	0.249%
39	18.266	2588	2592	2596	rBV2	25218	34119	4.20%	0.337%
40	18.313	2596	2600	2605	rVB2	35168	46775	5.76%	0.462%
41	18.396	2611	2614	2619	rVB6	8797	11411	1.41%	0.113%
42	18.454	2619	2624	2629	rBV3	34260	68832	8.48%	0.680%
43	18.495	2629	2631	2637	rVB	20138	27574	3.40%	0.272%
44	18.589	2639	2647	2654	rBV	26143	57011	7.02%	0.563%
45	18.766	2670	2677	2680	rBV	20538	36243	4.46%	0.358%
46	18.813	2681	2685	2690	rVB4	18752	33410	4.12%	0.330%
47	19.007	2714	2718	2724	rBV9	9691	14749	1.82%	0.146%
48	19.059	2724	2727	2731	rVB5	13989	18844	2.32%	0.186%
49	19.095	2731	2733	2737	rBV4	10054	12119	1.49%	0.120%
50	19.183	2743	2748	2750	rBV2	36167	52564	6.47%	0.519%
51	19.212	2750	2753	2760	rVB7	41644	65233	8.03%	0.644%
52	19.318	2767	2771	2772	rBV4	18699	18077	2.23%	0.179%
53	19.447	2786	2793	2798	rBV	221139	330337	40.69%	3.263%
54	19.594	2814	2818	2824	rBV2	17337	31678	3.90%	0.313%
55	19.682	2829	2833	2836	rBV3	33182	44647	5.50%	0.441%
56	19.776	2844	2849	2850	rBV2	25274	37735	4.65%	0.373%
57	19.805	2850	2854	2862	rVB	213168	329520	40.59%	3.255%
58	19.876	2863	2866	2872	rVB5	19527	25849	3.18%	0.255%
59	19.999	2881	2887	2892	rVB	555274	724743	89.27%	7.159%
60	20.134	2903	2910	2916	rBV6	24065	63002	7.76%	0.622%
61	20.211	2922	2923	2926	rVB3	11831	9386	1.16%	0.093%
62	20.299	2934	2938	2943	rVB	53854	85404	10.52%	0.844%
63	20.393	2952	2954	2959	rVB	24815	30786	3.79%	0.304%
64	20.458	2963	2965	2969	rVB2	26340	30380	3.74%	0.300%
65	20.599	2985	2989	2993	rBV	23798	38485	4.74%	0.380%
66	20.640	2993	2996	2999	rVV3	28865	37612	4.63%	0.372%
67	21.298	3104	3108	3112	rBV7	38681	68165	8.40%	0.673%
68	21.533	3145	3148	3154	rVB2	39705	62352	7.68%	0.616%
69	21.662	3163	3170	3175	rBV2	274783	588634	72.50%	5.815%
70	21.709	3175	3178	3186	rVB	100379	154811	19.07%	1.529%
71	23.871	3540	3546	3553	rBV2	61576	190988	23.52%	1.887%
72	23.935	3553	3557	3564	rVB4	84444	186275	22.94%	1.840%
73	24.746	3689	3695	3707	rVB2	69497	190770	23.50%	1.884%
74	24.899	3713	3721	3729	rBV2	135952	367292	45.24%	3.628%
75	25.410	3803	3808	3810	rBV6	25857	48324	5.95%	0.477%
76	30.379	4645	4654	4672	rVB6	145204	693693	85.44%	6.852%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049952.D
Acq On : 24 Aug 2021 14:41
Operator : CG/JU
Sample : M3463-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-18-0204

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 10123223

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049952.D
Acq On : 24 Aug 2021 14:41
Operator : CG/JU
Sample : M3463-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-18-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

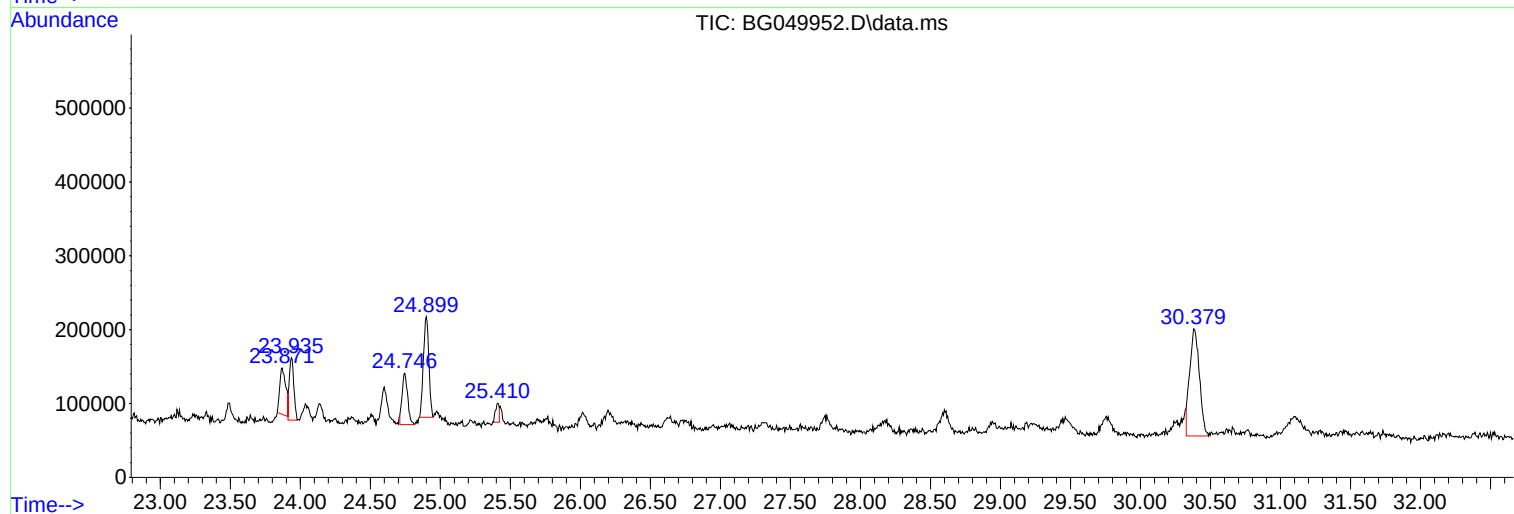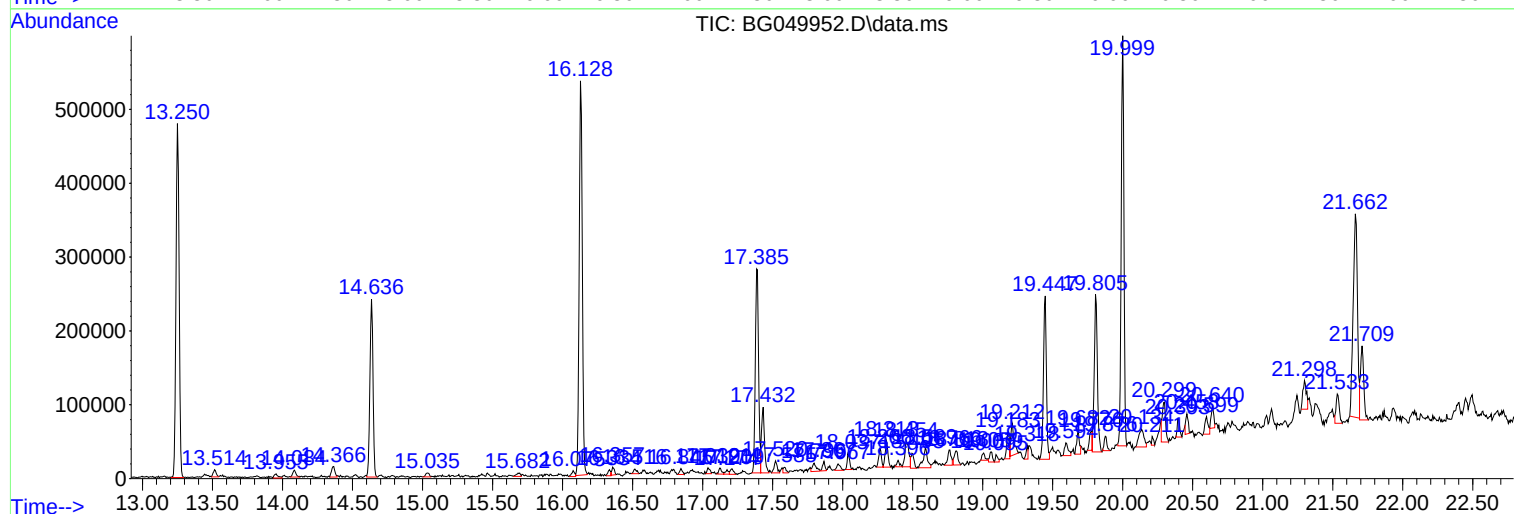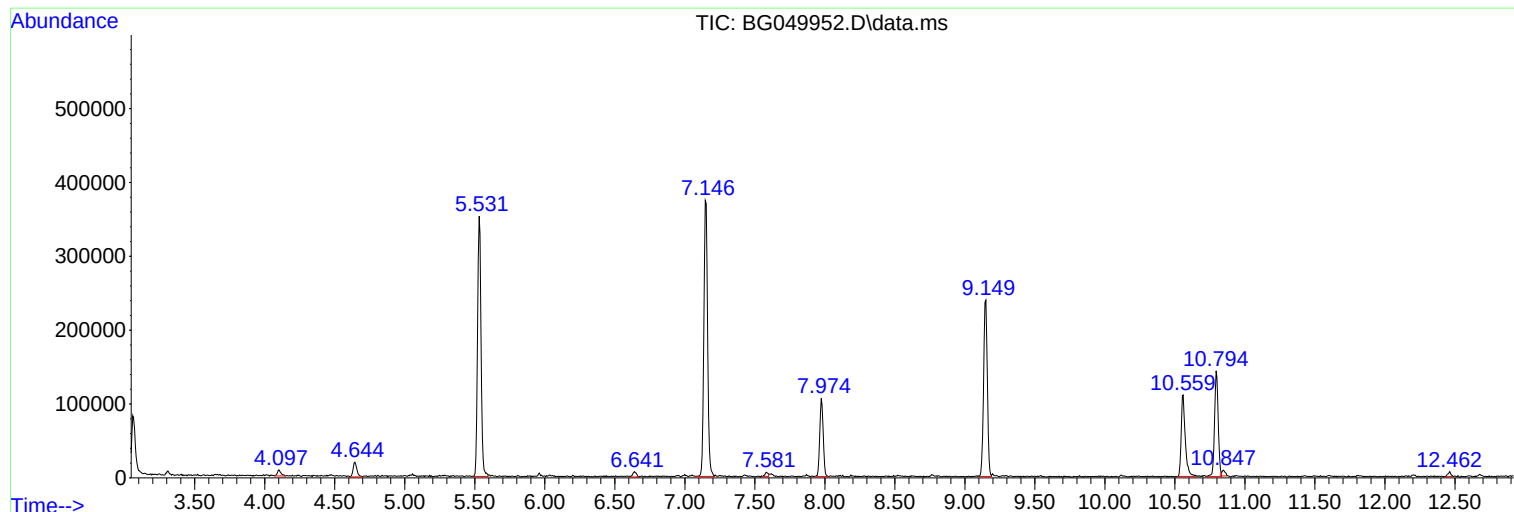

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049952.D
Acq On : 24 Aug 2021 14:41
Operator : CG/JU
Sample : M3463-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-18-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049952.D
Acq On : 24 Aug 2021 14:41
Operator : CG/JU
Sample : M3463-19
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-18-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------