

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049953.D
 Acq On : 24 Aug 2021 15:22
 Operator : CG/JU
 Sample : M3463-21
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-19-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.535	418	425	435	rBV	575996	962252	51.70%	6.319%
2	7.150	691	700	711	rBV	614910	1088854	58.50%	7.151%
3	7.979	830	841	847	rBV	110418	187072	10.05%	1.229%
4	9.148	1030	1040	1048	rBV	388968	704564	37.85%	4.627%
5	10.557	1274	1280	1296	rBV	168320	316794	17.02%	2.080%
6	10.798	1312	1321	1328	rBV	141883	259999	13.97%	1.707%
7	13.254	1731	1739	1749	rBV	832961	1339199	71.95%	8.795%
8	14.634	1968	1974	1982	rVB	241136	375458	20.17%	2.466%
9	16.132	2222	2229	2236	rBV	853389	1317191	70.77%	8.650%
10	16.784	2334	2340	2345	rBV9	11538	25168	1.35%	0.165%
11	17.389	2435	2443	2448	rBV	277631	438105	23.54%	2.877%
12	17.431	2448	2450	2459	rVB2	35837	50041	2.69%	0.329%
13	18.041	2550	2554	2559	rVB2	35271	45292	2.43%	0.297%
14	18.811	2682	2685	2692	rVB8	11189	19768	1.06%	0.130%
15	19.181	2745	2748	2750	rVV4	16948	21459	1.15%	0.141%
16	19.210	2750	2753	2756	rVB3	44075	51268	2.75%	0.337%
17	19.445	2787	2793	2797	rBV	112237	170499	9.16%	1.120%
18	19.492	2798	2801	2805	rVB6	17743	26813	1.44%	0.176%
19	19.680	2829	2833	2838	rVB4	30396	42614	2.29%	0.280%
20	19.774	2845	2849	2851	rBV3	20122	28288	1.52%	0.186%
21	19.810	2851	2855	2860	rVB	91807	137160	7.37%	0.901%
22	19.998	2881	2887	2893	rBV	1091083	1429371	76.79%	9.387%
23	20.280	2931	2935	2936	rBV4	29099	37760	2.03%	0.248%
24	21.302	3104	3109	3118	rVB6	63536	134947	7.25%	0.886%
25	21.472	3133	3138	3144	rVB	348296	506474	27.21%	3.326%
26	21.537	3146	3149	3154	rVB4	51937	78978	4.24%	0.519%
27	21.666	3164	3171	3176	rBV	241887	436784	23.47%	2.868%
28	22.494	3308	3312	3319	rVB5	69515	158700	8.53%	1.042%
29	23.217	3430	3435	3438	rBV7	21175	41169	2.21%	0.270%
30	24.151	3589	3594	3604	rVB4	64022	151121	8.12%	0.992%
31	24.738	3692	3694	3696	rBV3	16443	18880	1.01%	0.124%
32	24.897	3714	3721	3729	rVB2	141653	378112	20.31%	2.483%
33	26.348	3963	3968	3975	rVB5	33945	79907	4.29%	0.525%
34	26.618	4005	4014	4024	rVB4	168529	551976	29.65%	3.625%
35	29.473	4484	4500	4517	rVB5	332660	1556663	83.63%	10.223%
36	30.395	4645	4657	4677	rVB7	370870	1861346	100.00%	12.224%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049953.D
Acq On : 24 Aug 2021 15:22
Operator : CG/JU
Sample : M3463-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	31.088	4766	4775	4777	rBV9	71784	196991	10.58%	1.294%
----	--------	------	------	------	------	-------	--------	--------	--------


Sum of corrected areas: 15227037

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049953.D
Acq On : 24 Aug 2021 15:22
Operator : CG/JU
Sample : M3463-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

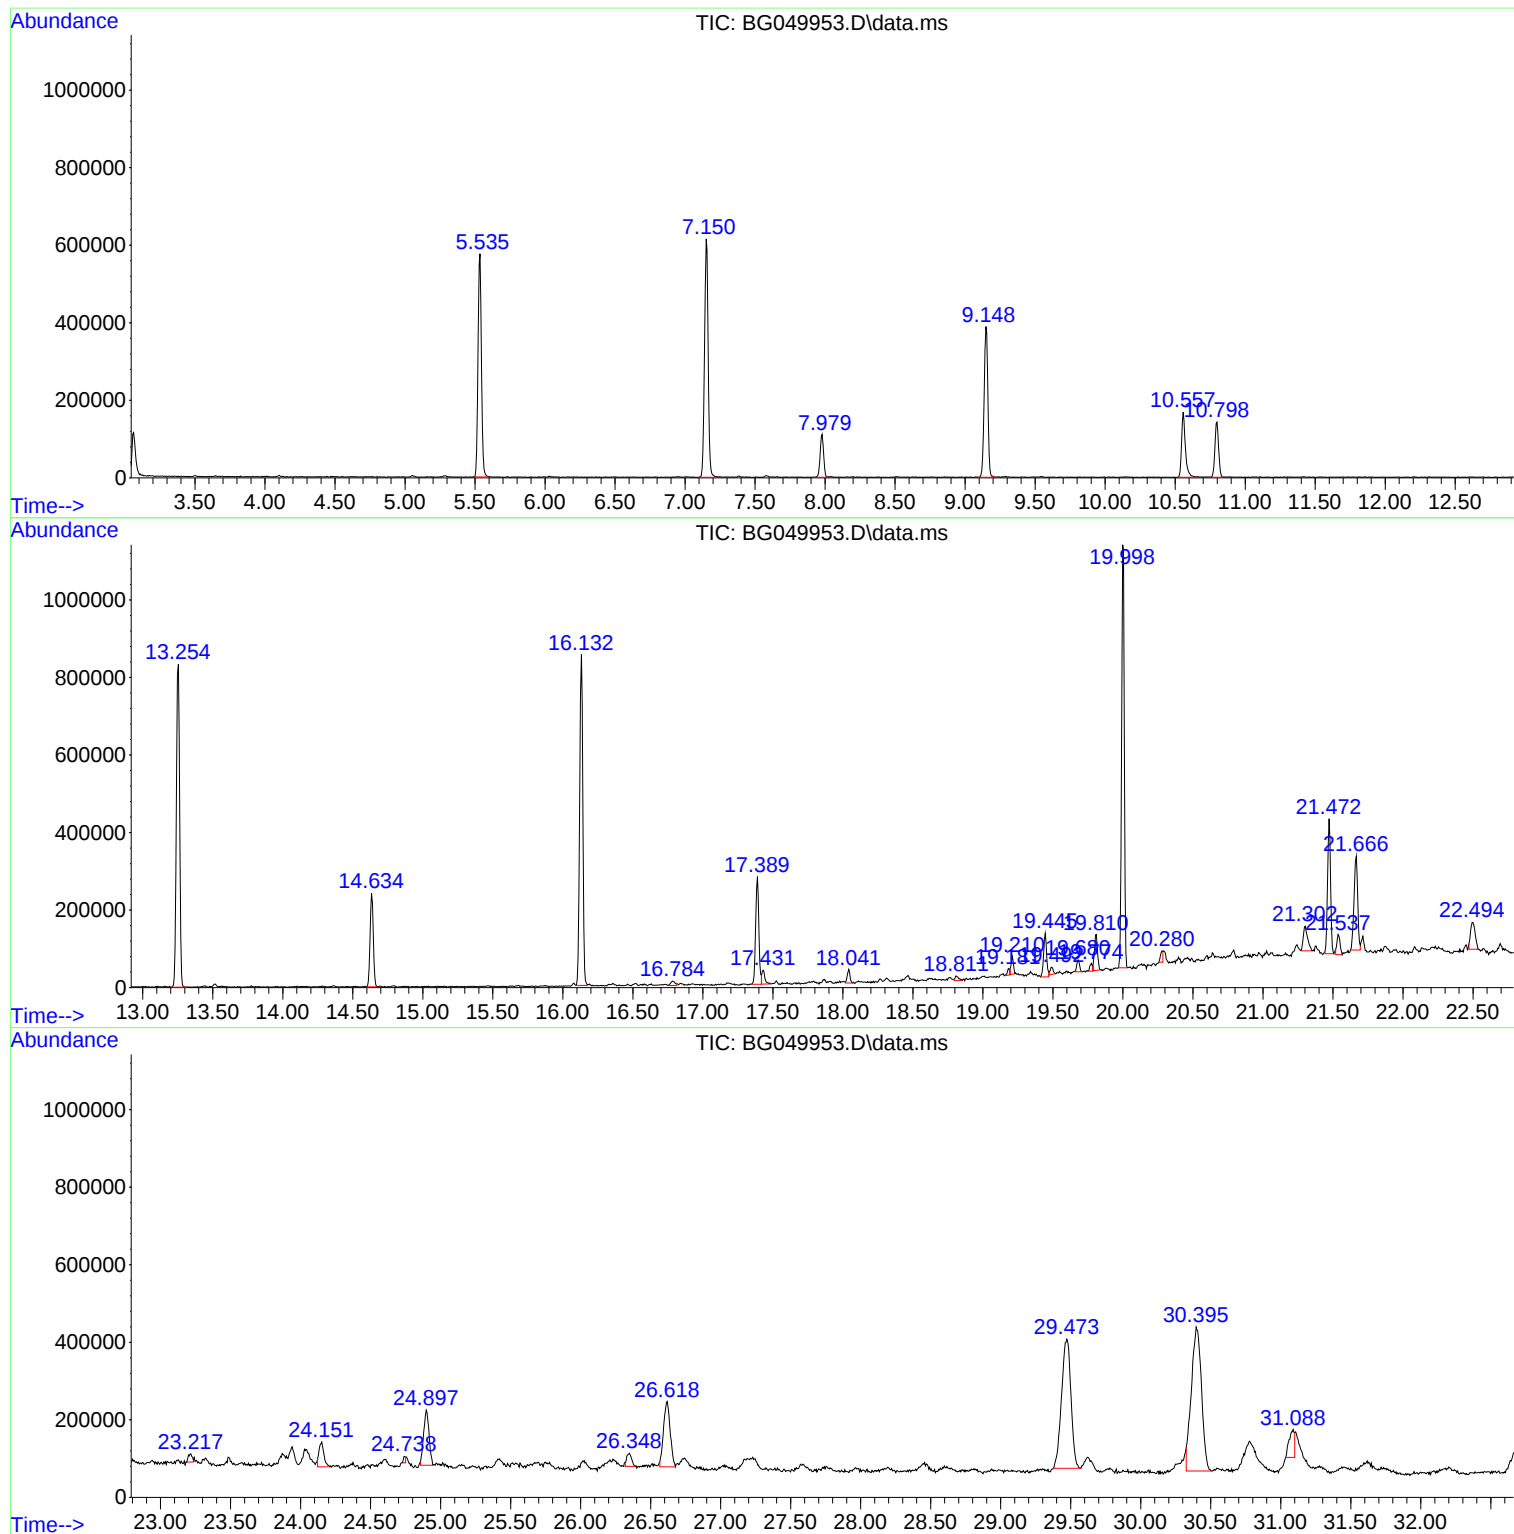

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049953.D
Acq On : 24 Aug 2021 15:22
Operator : CG/JU
Sample : M3463-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049953.D
Acq On : 24 Aug 2021 15:22
Operator : CG/JU
Sample : M3463-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------