

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049954.D
 Acq On : 24 Aug 2021 16:03
 Operator : CG/JU
 Sample : M3463-23
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-19-0204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.535	418	425	436	rBV	549973	894567	61.04%	7.036%
2	7.150	692	700	712	rBV	560912	1020951	69.66%	8.030%
3	7.978	832	841	847	rVB	115296	194722	13.29%	1.532%
4	9.147	1033	1040	1048	rBV	368447	669234	45.66%	5.264%
5	10.557	1273	1280	1294	rBV2	128531	242862	16.57%	1.910%
6	10.798	1312	1321	1329	rBV2	152667	273235	18.64%	2.149%
7	13.254	1731	1739	1746	rBV	858201	1310612	89.42%	10.308%
8	14.634	1968	1974	1981	rVB	256144	385966	26.33%	3.036%
9	16.132	2223	2229	2240	rBV	811337	1230732	83.97%	9.680%
10	16.367	2258	2269	2270	rBV8	8097	20500	1.40%	0.161%
11	17.389	2433	2443	2447	rBV	293403	452535	30.88%	3.559%
12	17.430	2447	2450	2460	rVV	89876	139650	9.53%	1.098%
13	17.524	2460	2466	2471	rVV	18642	31754	2.17%	0.250%
14	18.041	2549	2554	2559	rVB	23376	30632	2.09%	0.241%
15	18.264	2589	2592	2597	rBV3	11496	15062	1.03%	0.118%
16	18.317	2597	2601	2607	rVB5	15904	24354	1.66%	0.192%
17	18.464	2622	2626	2629	rVB2	19452	21967	1.50%	0.173%
18	18.811	2681	2685	2688	rVB5	11618	15903	1.09%	0.125%
19	19.445	2787	2793	2797	rBV	211815	302612	20.65%	2.380%
20	19.492	2797	2801	2805	rVB6	21935	33675	2.30%	0.265%
21	19.680	2829	2833	2837	rBV2	72814	95070	6.49%	0.748%
22	19.774	2845	2849	2850	rBV3	32971	43240	2.95%	0.340%
23	19.809	2851	2855	2861	rVB	163721	244302	16.67%	1.921%
24	20.003	2881	2888	2893	rBV	1065080	1465654	100.00%	11.528%
25	20.127	2905	2909	2910	rBV4	15529	17163	1.17%	0.135%
26	20.297	2934	2938	2942	rVB2	46212	68945	4.70%	0.542%
27	20.397	2953	2955	2958	rVB2	22870	21941	1.50%	0.173%
28	21.025	3058	3062	3065	rBV5	21032	35546	2.43%	0.280%
29	21.296	3104	3108	3118	rVB8	61008	141621	9.66%	1.114%
30	21.472	3133	3138	3144	rBV2	117484	180114	12.29%	1.417%
31	21.660	3163	3170	3175	rBV2	256892	554223	37.81%	4.359%
32	21.713	3175	3179	3187	rVB	86289	163701	11.17%	1.288%
33	22.441	3301	3303	3306	rBV3	22305	31622	2.16%	0.249%
34	22.488	3307	3311	3320	rVB6	83836	201573	13.75%	1.585%
35	23.487	3478	3481	3489	rVB8	49609	89038	6.07%	0.700%
36	23.869	3542	3546	3553	rBV	42288	104672	7.14%	0.823%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049954.D
Acq On : 24 Aug 2021 16:03
Operator : CG/JU
Sample : M3463-23
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0204

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	24.039	3568	3575	3583	rVB7	57274	169456	11.56%	1.333%
38	24.750	3687	3696	3704	rBV2	56168	186675	12.74%	1.468%
39	24.902	3713	3722	3731	rBV2	141021	390694	26.66%	3.073%
40	25.414	3802	3809	3816	rBV6	71818	199687	13.62%	1.571%
41	30.395	4646	4657	4674	rVB10	210485	997736	68.07%	7.847%


Sum of corrected areas: 12714198

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049954.D
Acq On : 24 Aug 2021 16:03
Operator : CG/JU
Sample : M3463-23
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

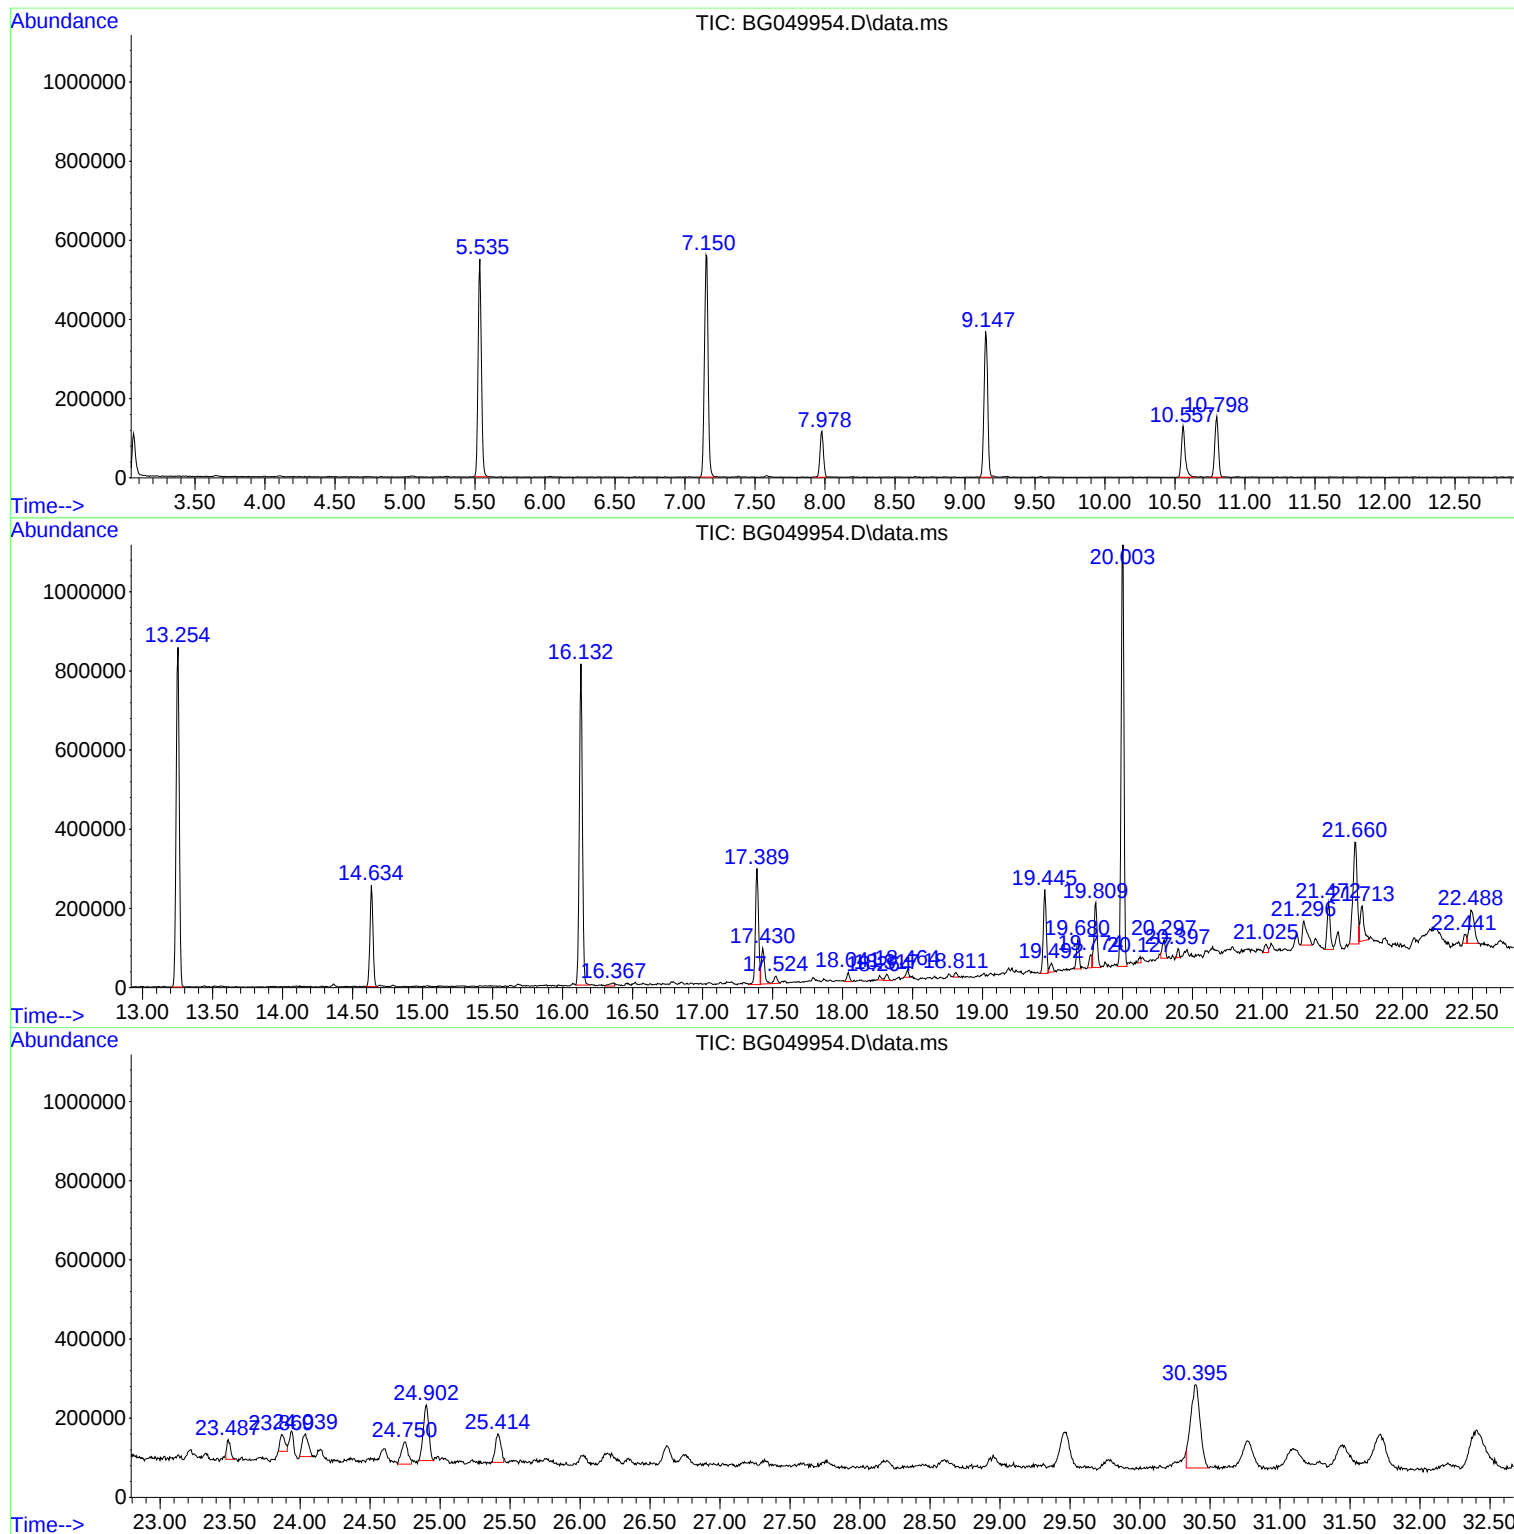

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049954.D
Acq On : 24 Aug 2021 16:03
Operator : CG/JU
Sample : M3463-23
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049954.D
Acq On : 24 Aug 2021 16:03
Operator : CG/JU
Sample : M3463-23
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-19-0204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------