

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049955.D
 Acq On : 24 Aug 2021 16:45
 Operator : CG/JU
 Sample : M3463-37
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-29-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.537	418	425	435	rBV	479214	817435	12.23%	4.912%
2	7.152	690	700	717	rBV	518051	911111	13.63%	5.475%
3	7.975	833	840	848	rVB	117511	193342	2.89%	1.162%
4	9.149	1032	1040	1047	rBV	323219	590051	8.83%	3.546%
5	10.559	1272	1280	1292	rBV	203774	369076	5.52%	2.218%
6	10.800	1313	1321	1327	rVB	148784	270365	4.05%	1.625%
7	13.250	1731	1738	1748	rVB	767959	1213663	18.16%	7.293%
8	13.520	1777	1784	1791	rBV2	108825	179222	2.68%	1.077%
9	14.636	1966	1974	1981	rBV	247881	385984	5.77%	2.319%
10	16.134	2222	2229	2238	rVB	722025	1140253	17.06%	6.852%
11	17.391	2437	2443	2449	rBV	281556	442063	6.61%	2.656%
12	19.212	2749	2753	2757	rVB2	57713	73055	1.09%	0.439%
13	19.441	2788	2792	2797	rBV	48830	73001	1.09%	0.439%
14	20.000	2881	2887	2893	rVB	1056686	1378974	20.63%	8.286%
15	21.233	3093	3097	3104	rBV3	125712	196833	2.94%	1.183%
16	21.298	3104	3108	3118	rVB6	55049	117421	1.76%	0.706%
17	21.492	3136	3141	3145	rBV8	53820	100743	1.51%	0.605%
18	21.533	3145	3148	3153	rVB2	53929	77060	1.15%	0.463%
19	21.662	3165	3170	3176	rBV	237937	417914	6.25%	2.511%
20	22.343	3268	3286	3300	rVB4	1109344	6683883	100.00%	40.164%
21	23.489	3475	3481	3488	rBV4	66697	138615	2.07%	0.833%
22	23.941	3553	3558	3566	rVB3	86115	183556	2.75%	1.103%
23	24.899	3712	3721	3731	rVB	150015	433984	6.49%	2.608%
24	25.416	3802	3809	3821	rVB5	88379	253961	3.80%	1.526%




Sum of corrected areas: 16641565

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049955.D
Acq On : 24 Aug 2021 16:45
Operator : CG/JU
Sample : M3463-37
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-29-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

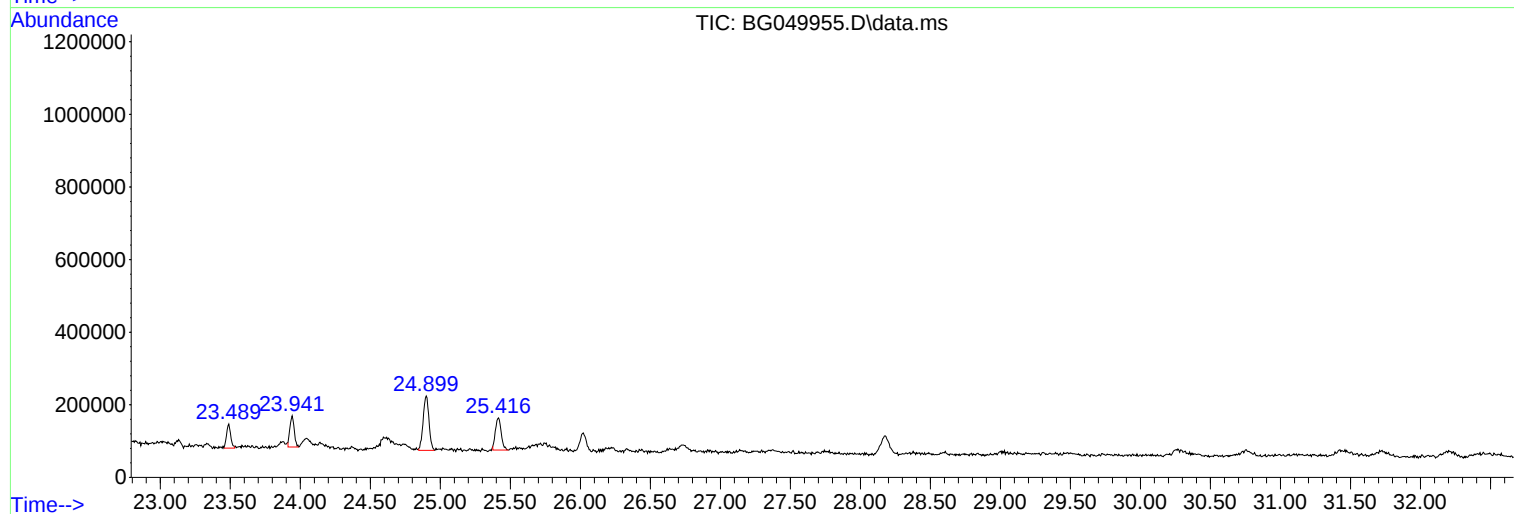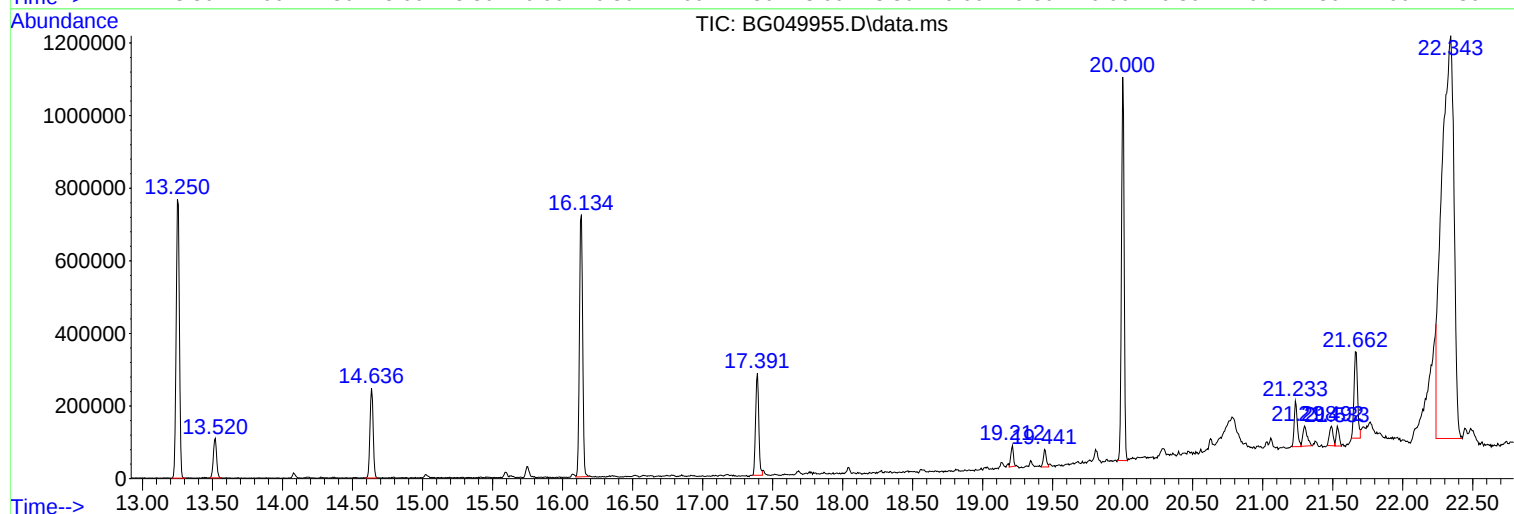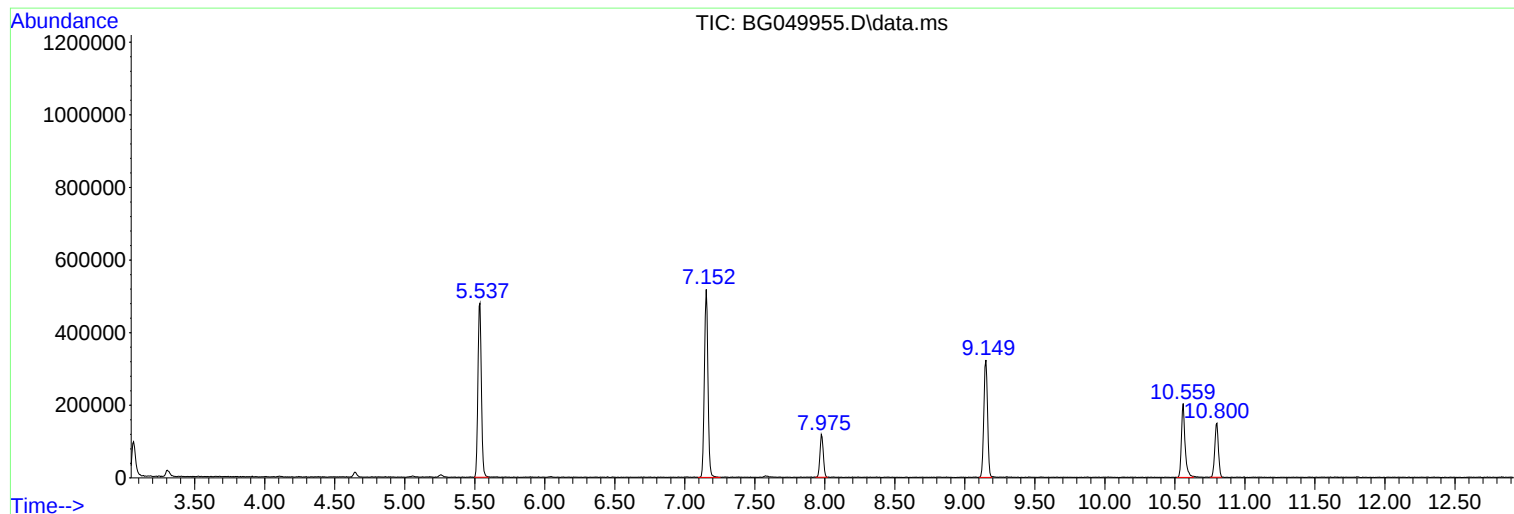

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049955.D
Acq On : 24 Aug 2021 16:45
Operator : CG/JU
Sample : M3463-37
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-29-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049955.D
Acq On : 24 Aug 2021 16:45
Operator : CG/JU
Sample : M3463-37
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-29-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------