

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049957.D
 Acq On : 24 Aug 2021 18:08
 Operator : CG/JU
 Sample : M3419-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-03-0205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049957.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.541	418	426	437	rBV	464411	791358	25.40%	3.105%
2	7.156	691	701	712	rBV	511770	916205	29.40%	3.595%
3	7.978	832	841	850	rBV2	118077	206666	6.63%	0.811%
4	9.153	1033	1041	1052	rBV	332804	618658	19.85%	2.427%
5	10.569	1276	1282	1287	rBV5	19468	38879	1.25%	0.153%
6	10.798	1310	1321	1327	rBV	153625	305449	9.80%	1.198%
7	10.851	1327	1330	1338	rVB2	30553	51529	1.65%	0.202%
8	11.644	1455	1465	1473	rBV8	23190	67588	2.17%	0.265%
9	12.461	1599	1604	1613	rVB2	32896	54994	1.76%	0.216%
10	12.678	1634	1641	1647	rBV	29700	52258	1.68%	0.205%
11	13.254	1732	1739	1748	rVB	887222	1371939	44.03%	5.383%
12	13.800	1827	1832	1834	rBV6	17991	31677	1.02%	0.124%
13	13.959	1853	1859	1863	rBV	41476	76829	2.47%	0.301%
14	14.011	1864	1868	1871	rVV4	23316	37348	1.20%	0.147%
15	14.053	1871	1875	1878	rVV2	31294	43995	1.41%	0.173%
16	14.100	1878	1883	1886	rVB5	18694	34259	1.10%	0.134%
17	14.194	1892	1899	1902	rBV5	21705	38702	1.24%	0.152%
18	14.364	1922	1928	1937	rBV	152879	298005	9.56%	1.169%
19	14.464	1940	1945	1950	rVV3	41089	64914	2.08%	0.255%
20	14.605	1964	1969	1970	rVV5	29283	43075	1.38%	0.169%
21	14.640	1970	1975	1982	rVV2	219948	362850	11.64%	1.424%
22	14.711	1982	1987	1993	rVB6	31597	67504	2.17%	0.265%
23	15.040	2036	2043	2046	rBV4	35106	60633	1.95%	0.238%
24	15.110	2052	2055	2060	rVB3	28838	45234	1.45%	0.177%
25	15.257	2073	2080	2083	rBV5	42101	87916	2.82%	0.345%
26	15.421	2102	2108	2113	rBV6	52634	103922	3.34%	0.408%
27	15.521	2120	2125	2128	rBV3	30348	57417	1.84%	0.225%
28	15.686	2149	2153	2157	rBV2	56741	97816	3.14%	0.384%
29	15.979	2200	2203	2209	rVB4	26774	45591	1.46%	0.179%
30	16.138	2223	2230	2236	rVB	668057	1030860	33.08%	4.044%
31	16.361	2260	2268	2274	rBV7	65548	160021	5.14%	0.628%
32	16.743	2330	2333	2338	rVB4	33485	44017	1.41%	0.173%
33	17.213	2410	2413	2419	rVB	58096	89816	2.88%	0.352%
34	17.395	2439	2444	2447	rBV	217135	341762	10.97%	1.341%
35	17.442	2447	2452	2457	rVB	829799	1256674	40.33%	4.930%
36	17.530	2463	2467	2471	rBV	110804	155018	4.98%	0.608%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049957.D
 Acq On : 24 Aug 2021 18:08
 Operator : CG/JU
 Sample : M3419-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-03-0205

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.977	2540	2543	2549	rVB	82777	117266	3.76%	0.460%
38	18.276	2589	2594	2598	rBV	299695	456231	14.64%	1.790%
39	18.323	2598	2602	2609	rVB	380170	555879	17.84%	2.181%
40	18.464	2621	2626	2631	rBV3	351802	710447	22.80%	2.787%
41	18.505	2631	2633	2639	rVB	256665	313756	10.07%	1.231%
42	18.770	2674	2678	2682	rBV	159022	213337	6.85%	0.837%
43	18.817	2682	2686	2691	rVV2	179042	282616	9.07%	1.109%
44	19.063	2726	2728	2733	rVB	92468	116828	3.75%	0.458%
45	19.187	2745	2749	2754	rBV	324077	555722	17.83%	2.180%
46	19.334	2770	2774	2781	rBV4	170034	388301	12.46%	1.523%
47	19.463	2790	2796	2801	rVB	1749601	2608013	83.70%	10.232%
48	19.827	2848	2858	2864	rVB	1867981	3115938	100.00%	12.225%
49	20.009	2885	2889	2894	rVB	1173936	1580647	50.73%	6.201%
50	20.420	2954	2959	2963	rBV2	542618	867467	27.84%	3.403%
51	20.473	2965	2968	2971	rVB	298972	370313	11.88%	1.453%
52	20.608	2988	2991	2995	rBV	285536	351843	11.29%	1.380%
53	20.655	2996	2999	3009	rVB2	259542	413590	13.27%	1.623%
54	21.666	3166	3171	3177	rBV3	799275	1803412	57.88%	7.075%
55	21.730	3179	3182	3193	rVB	914500	1515446	48.64%	5.946%




Sum of corrected areas: 25488430

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049957.D
Acq On : 24 Aug 2021 18:08
Operator : CG/JU
Sample : M3419-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

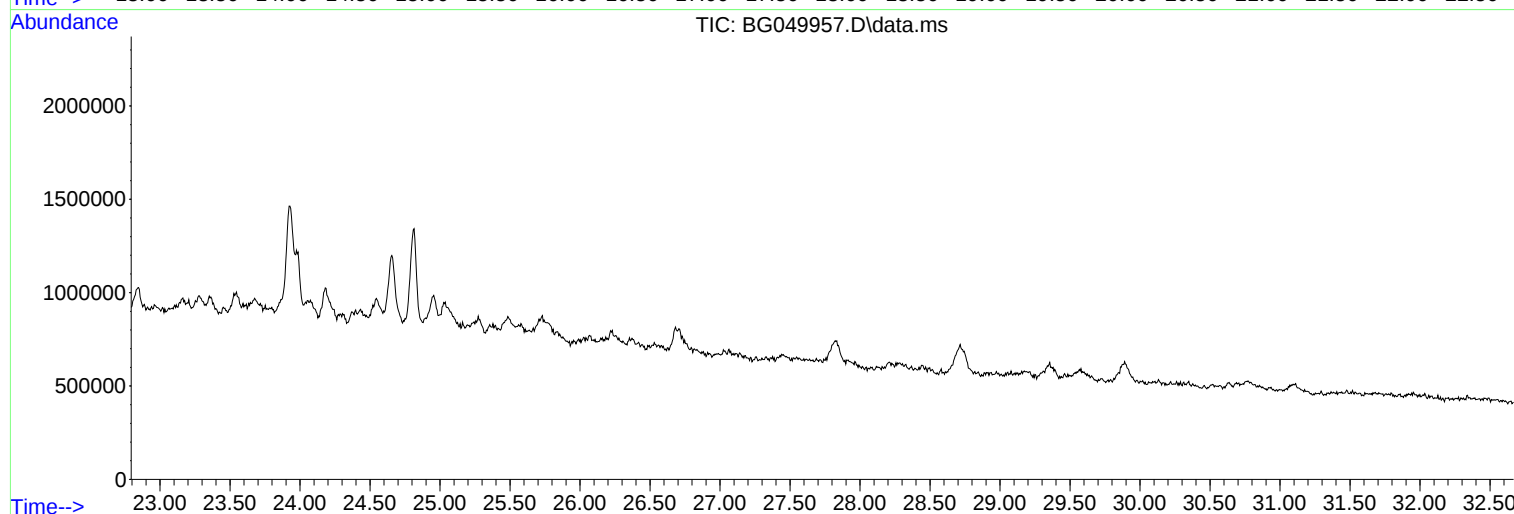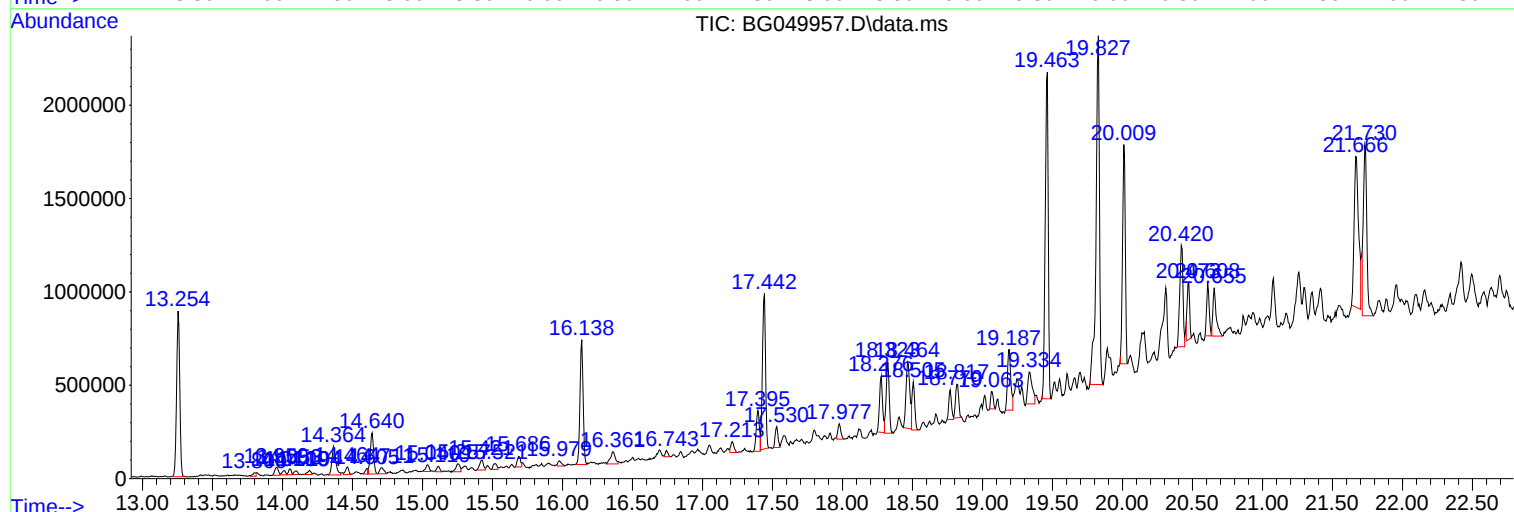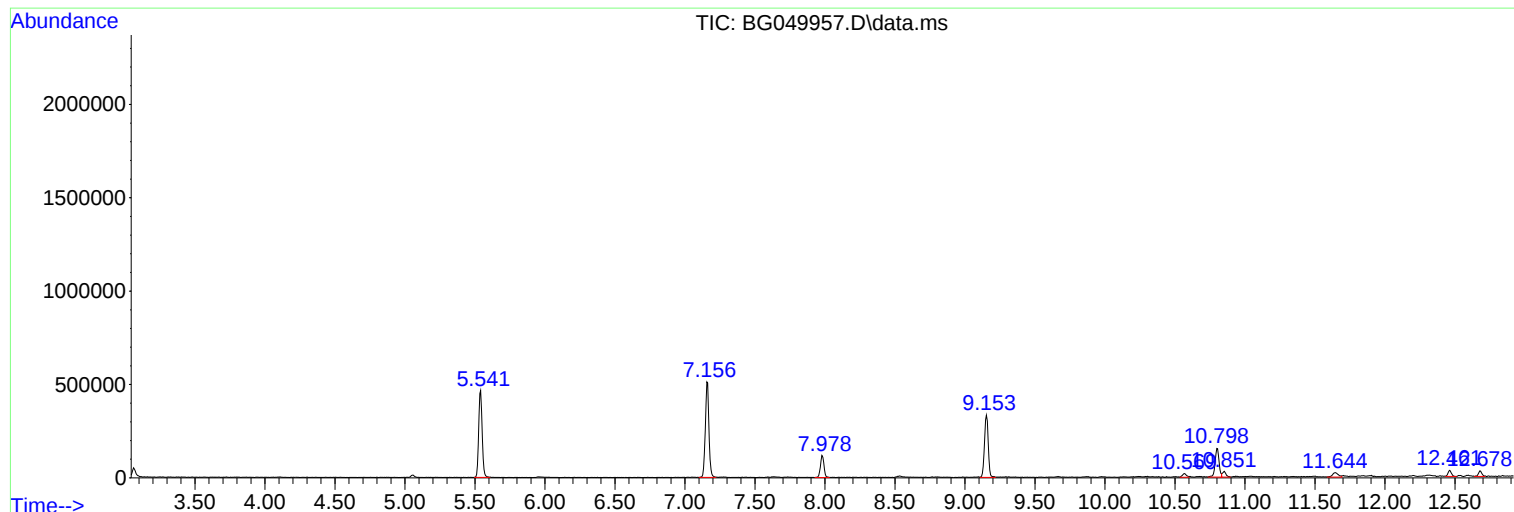

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049957.D
Acq On : 24 Aug 2021 18:08
Operator : CG/JU
Sample : M3419-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049957.D
Acq On : 24 Aug 2021 18:08
Operator : CG/JU
Sample : M3419-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-03-0205

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
