

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049958.D
 Acq On : 24 Aug 2021 18:49
 Operator : CG/JU
 Sample : M3463-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-16-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.068	3	5	14	rVB2	51094	83466	10.48%	1.090%
2	5.266	372	379	386	rBV	25563	48346	6.07%	0.632%
3	5.542	420	426	439	rBV	318435	549133	68.93%	7.174%
4	5.941	490	494	504	rBV2	15219	28317	3.55%	0.370%
5	7.163	689	702	712	rBV	344263	641955	80.58%	8.387%
6	7.398	737	742	748	rVB5	7968	13196	1.66%	0.172%
7	7.985	833	842	848	rBV	126430	214109	26.87%	2.797%
8	8.814	978	983	990	rVB2	19058	33350	4.19%	0.436%
9	9.154	1034	1041	1049	rBV	225729	403663	50.67%	5.274%
10	10.564	1275	1281	1292	rBV2	117709	225144	28.26%	2.941%
11	10.805	1316	1322	1328	rBV	156605	290026	36.40%	3.789%
12	10.940	1342	1345	1353	rVB5	5230	10241	1.29%	0.134%
13	11.810	1491	1493	1497	rVB2	7455	8791	1.10%	0.115%
14	12.150	1544	1551	1554	rBV7	12729	25689	3.22%	0.336%
15	13.161	1719	1723	1726	rBV3	7017	10093	1.27%	0.132%
16	13.261	1731	1740	1748	rVB	502397	796703	100.00%	10.409%
17	13.425	1762	1768	1769	rBV5	5250	9384	1.18%	0.123%
18	13.519	1779	1784	1791	rBV3	21772	37376	4.69%	0.488%
19	13.960	1854	1859	1864	rVB9	9326	16167	2.03%	0.211%
20	14.077	1872	1879	1882	rBV8	18203	42207	5.30%	0.551%
21	14.371	1923	1929	1934	rBV2	13259	26082	3.27%	0.341%
22	14.471	1942	1946	1949	rBV4	8442	11217	1.41%	0.147%
23	14.641	1968	1975	1981	rVB	255991	401024	50.34%	5.239%
24	14.706	1981	1986	1991	rVB2	22944	35299	4.43%	0.461%
25	15.041	2036	2043	2049	rVB5	16038	40023	5.02%	0.523%
26	15.264	2076	2081	2082	rBV4	10560	16312	2.05%	0.213%
27	15.693	2149	2154	2159	rBV	23694	38905	4.88%	0.508%
28	15.986	2199	2204	2207	rBV7	6407	11322	1.42%	0.148%
29	16.139	2224	2230	2239	rVB	455375	659220	82.74%	8.613%
30	16.274	2250	2253	2259	rVB4	21729	27163	3.41%	0.355%
31	16.362	2266	2268	2273	rVB5	16375	23047	2.89%	0.301%
32	16.691	2320	2324	2326	rBV5	10320	16274	2.04%	0.213%
33	16.850	2349	2351	2356	rBV6	10829	13104	1.64%	0.171%
34	17.396	2438	2444	2448	rBV	248773	382275	47.98%	4.994%
35	17.437	2448	2451	2458	rVB	135895	199030	24.98%	2.600%
36	17.531	2465	2467	2471	rVB	28297	31222	3.92%	0.408%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049958.D
Acq On : 24 Aug 2021 18:49
Operator : CG/JU
Sample : M3463-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-16-0002

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.766	2503	2507	2511	rBV2	52615	100203	12.58%	1.309%
38	18.436	2618	2621	2624	rBV2	58813	66487	8.35%	0.869%
39	18.536	2635	2638	2641	rBV	50635	68331	8.58%	0.893%
40	19.458	2790	2795	2800	rBV	269636	373468	46.88%	4.879%
41	19.822	2852	2857	2866	rBV2	291848	568975	71.42%	7.434%
42	20.010	2884	2889	2893	rBV	557958	740039	92.89%	9.669%
43	21.479	3136	3139	3146	rBV	193042	317696	39.88%	4.151%


Sum of corrected areas: 7654074

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049958.D
Acq On : 24 Aug 2021 18:49
Operator : CG/JU
Sample : M3463-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-16-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

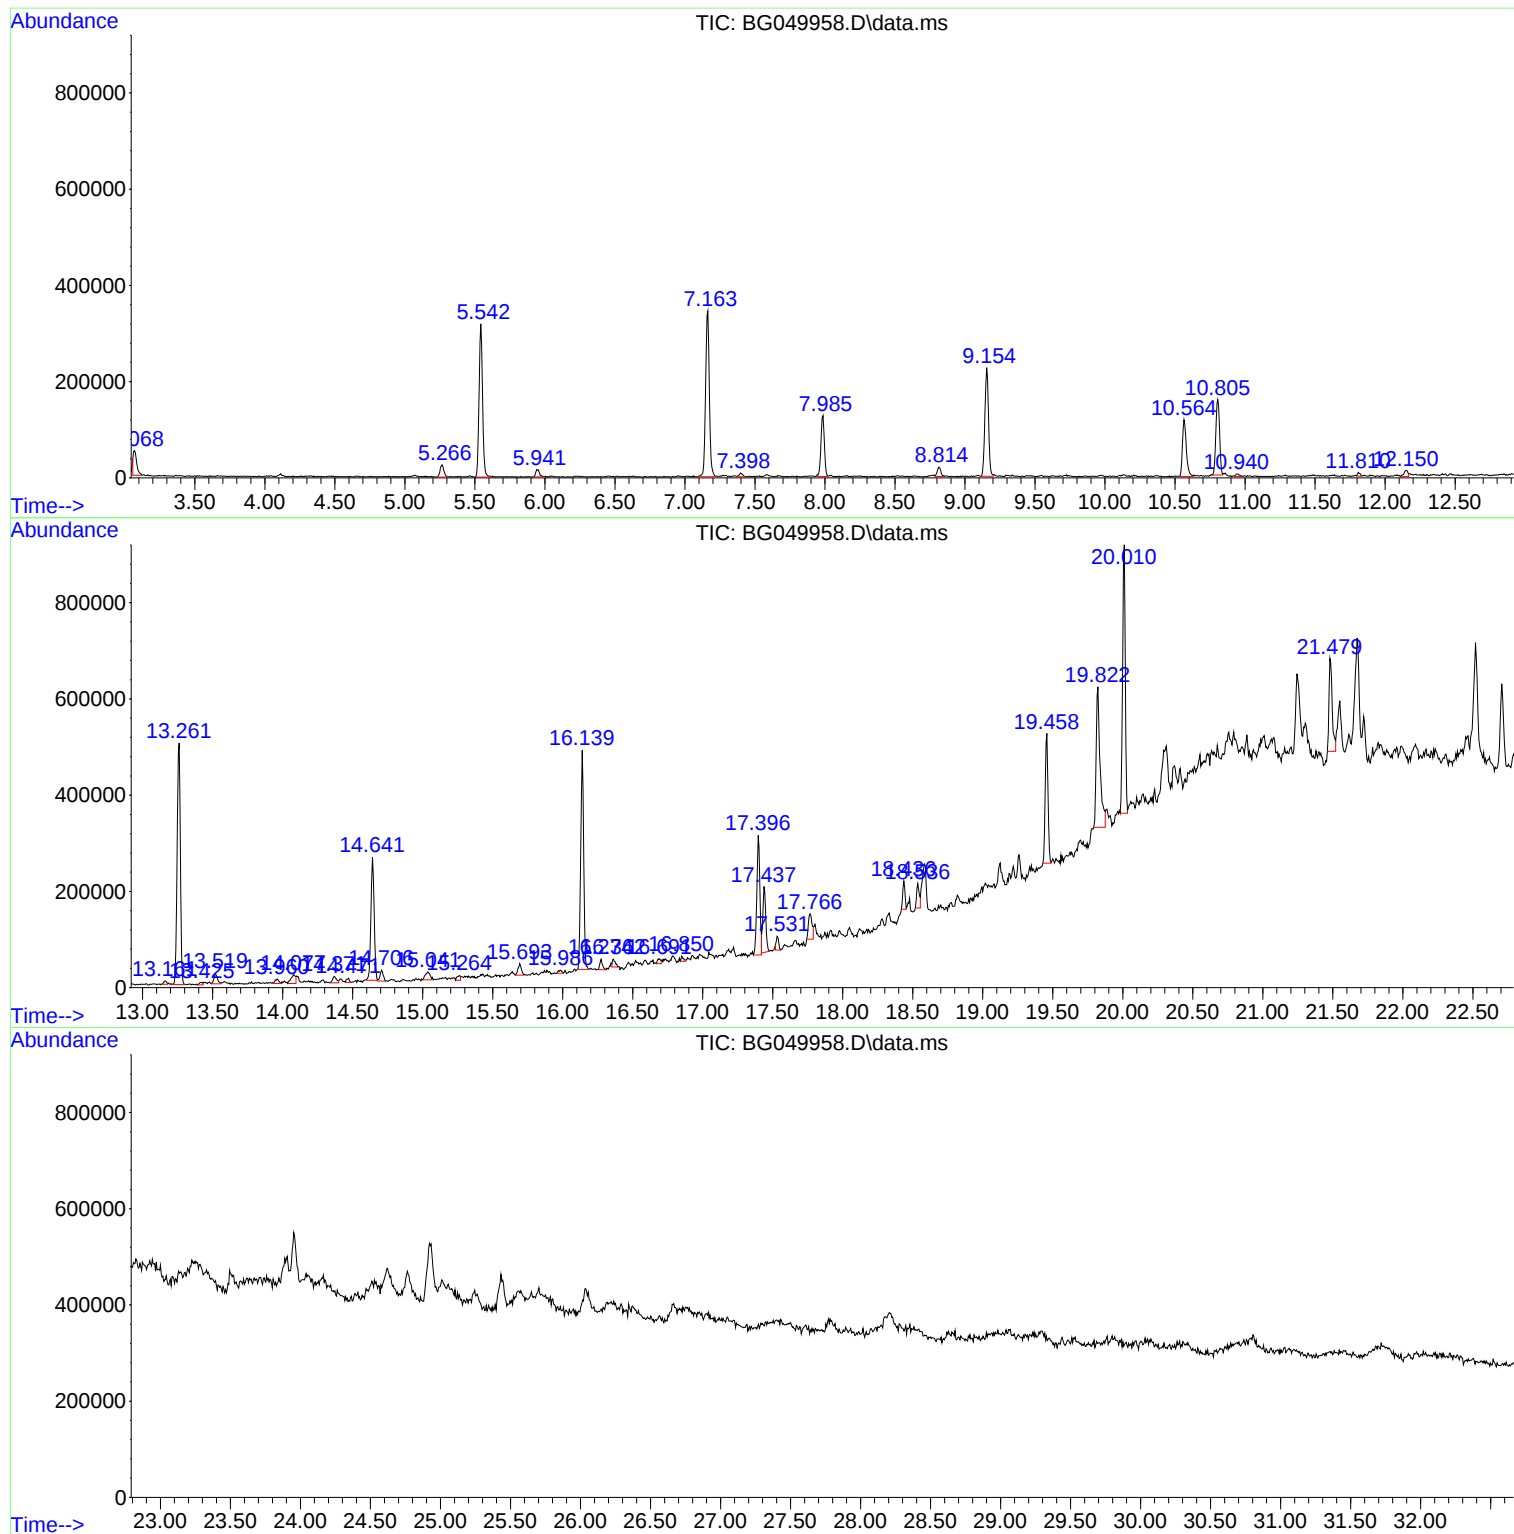

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049958.D
Acq On : 24 Aug 2021 18:49
Operator : CG/JU
Sample : M3463-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-16-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049958.D
Acq On : 24 Aug 2021 18:49
Operator : CG/JU
Sample : M3463-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-16-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------