

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049959.D
 Acq On : 24 Aug 2021 19:31
 Operator : CG/JU
 Sample : M3394-13 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-02-0002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.541	419	426	436	rVB	78901	137101	5.14%	1.641%
2	7.157	691	701	714	rBV	83465	161478	6.05%	1.932%
3	7.985	835	842	849	rVB	132264	225569	8.46%	2.699%
4	9.154	1034	1041	1050	rBV2	55354	103188	3.87%	1.235%
5	10.805	1313	1322	1329	rBV	180516	323034	12.11%	3.866%
6	13.254	1733	1739	1746	rVB	155937	240043	9.00%	2.873%
7	14.370	1923	1929	1936	rBV	42590	81021	3.04%	0.970%
8	14.641	1966	1975	1983	rBV	264754	422740	15.85%	5.059%
9	15.034	2036	2042	2048	rBV4	13644	27665	1.04%	0.331%
10	15.692	2149	2154	2157	rBV4	18784	28666	1.07%	0.343%
11	16.139	2223	2230	2236	rBV2	114812	185683	6.96%	2.222%
12	16.368	2266	2269	2274	rVB6	20081	28120	1.05%	0.337%
13	17.049	2382	2385	2390	rVB4	18097	28326	1.06%	0.339%
14	17.214	2409	2413	2419	rVB2	27133	47436	1.78%	0.568%
15	17.396	2438	2444	2448	rBV	268539	433040	16.23%	5.182%
16	17.437	2448	2451	2460	rVB	306831	447568	16.78%	5.356%
17	17.531	2464	2467	2471	rVB	25552	33077	1.24%	0.396%
18	18.271	2589	2593	2598	rBV	77052	118494	4.44%	1.418%
19	18.324	2598	2602	2608	rVB	98333	141385	5.30%	1.692%
20	18.465	2621	2626	2630	rBV4	96687	189798	7.12%	2.271%
21	18.506	2631	2633	2638	rVB2	67212	84596	3.17%	1.012%
22	18.770	2674	2678	2681	rBV	43547	58807	2.20%	0.704%
23	18.817	2682	2686	2692	rVB3	74708	111912	4.20%	1.339%
24	19.193	2745	2750	2753	rBV3	67214	113870	4.27%	1.363%
25	19.334	2771	2774	2779	rBV3	37292	53736	2.01%	0.643%
26	19.458	2789	2795	2800	rBV	492091	722586	27.09%	8.647%
27	19.822	2851	2857	2866	rVB2	1523035	2667534	100.00%	31.923%
28	20.004	2884	2888	2893	rVB	182801	242432	9.09%	2.901%
29	21.672	3166	3172	3177	rBV3	243999	585992	21.97%	7.013%
30	21.719	3178	3180	3188	rVB	213649	311219	11.67%	3.724%




Sum of corrected areas: 8356116

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049959.D
Acq On : 24 Aug 2021 19:31
Operator : CG/JU
Sample : M3394-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-02-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

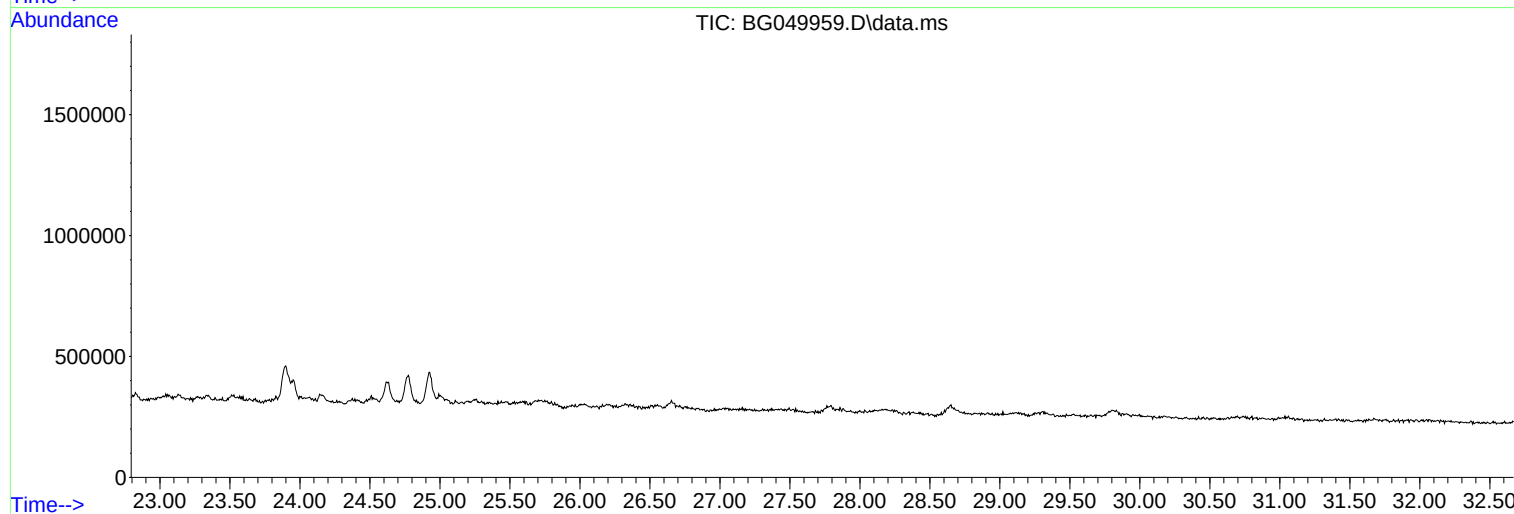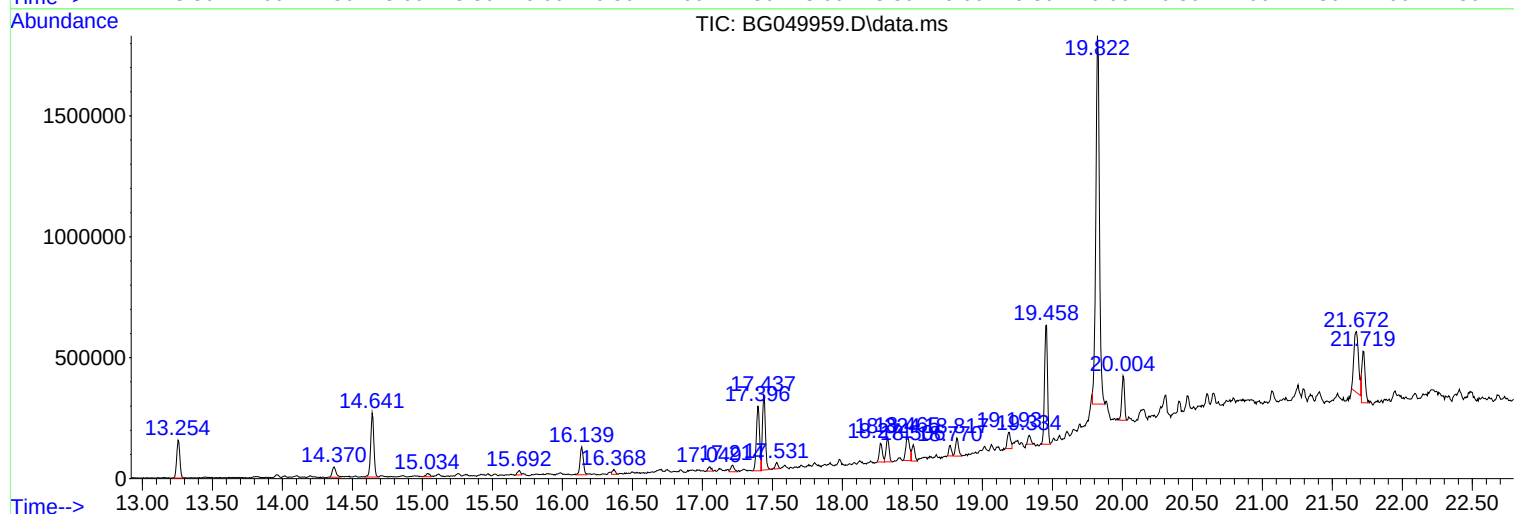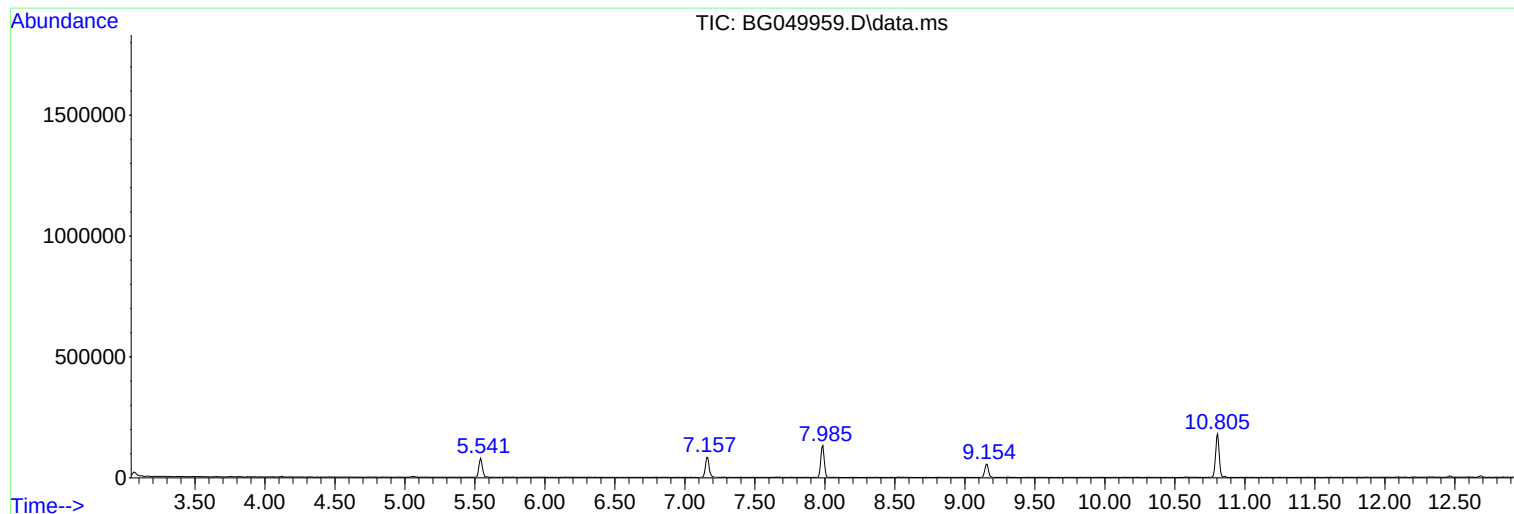

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049959.D
Acq On : 24 Aug 2021 19:31
Operator : CG/JU
Sample : M3394-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-02-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049959.D
Acq On : 24 Aug 2021 19:31
Operator : CG/JU
Sample : M3394-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-02-0002

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
