


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
 Data File : BG049946.D
 Acq On : 24 Aug 2021 10:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 23 16:13:24 2021

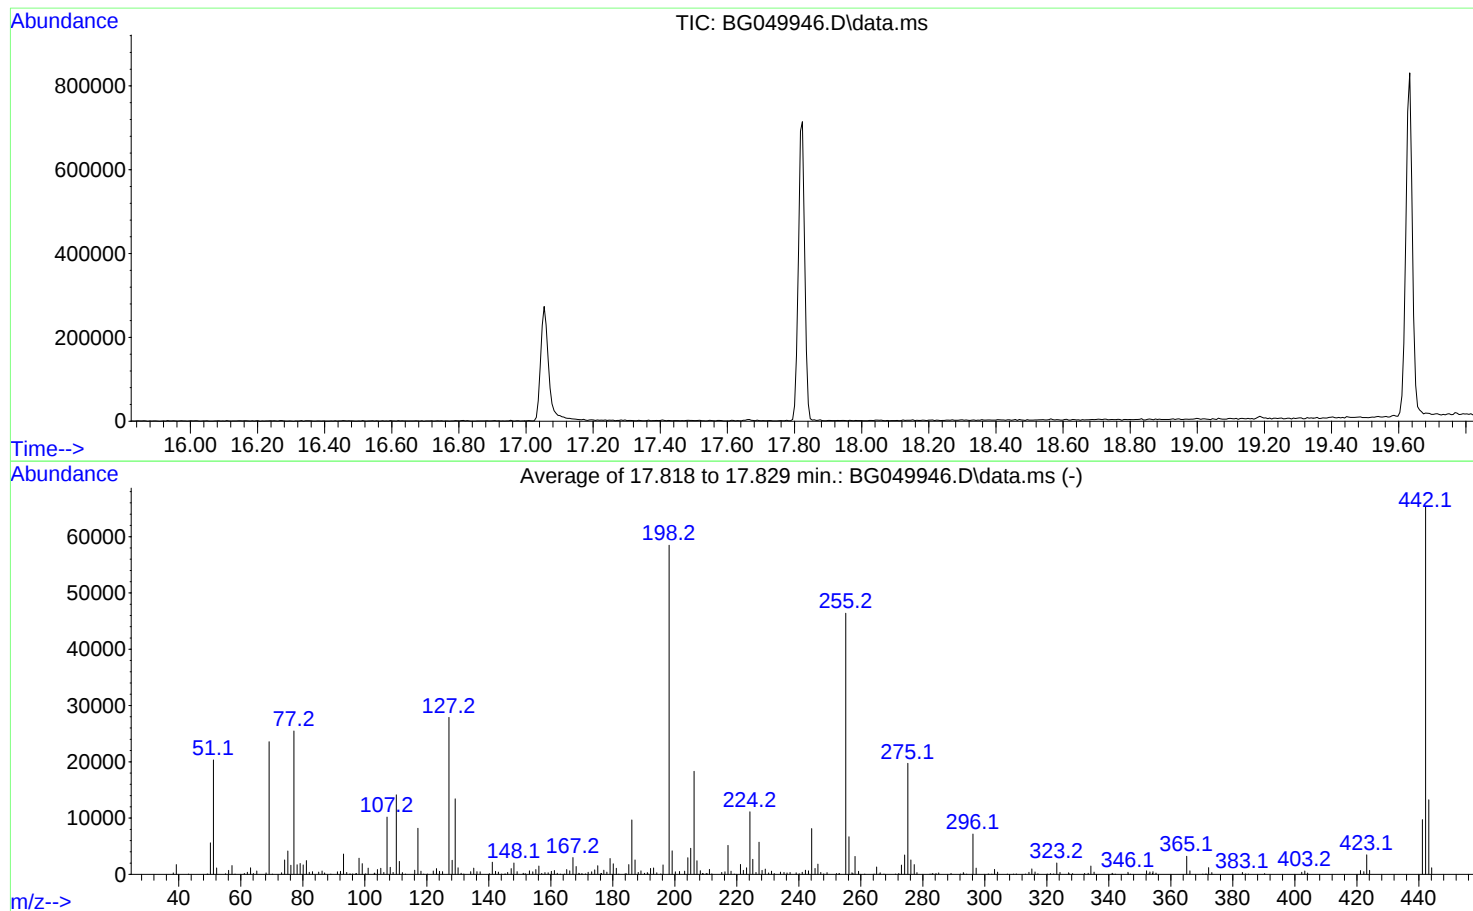




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	20328	PASS
68	69	0.00	2	1.1	270	PASS
69	198	0.00	100	40.3	23570	PASS
70	69	0.00	2	0.2	54	PASS
127	198	10	80	47.7	27885	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58472	PASS
199	198	5	9	7.1	4174	PASS
275	198	10	60	33.7	19724	PASS
365	198	1	100	5.5	3202	PASS
441	198	0.01	100	16.7	9736	PASS
442	442	50	100	100.0	65363	PASS
443	442	15	24	20.3	13238	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049946.D
Acq On : 24 Aug 2021 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 24 11:13:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 16:13:24 2021
Response via : Initial Calibration

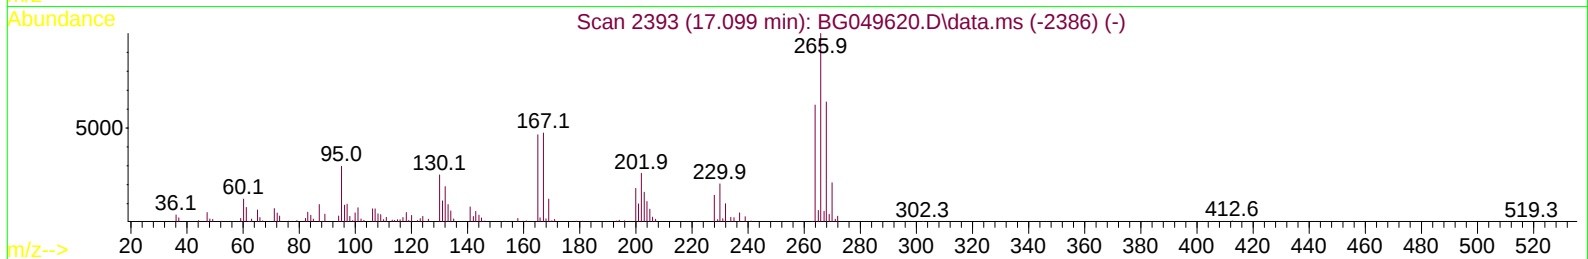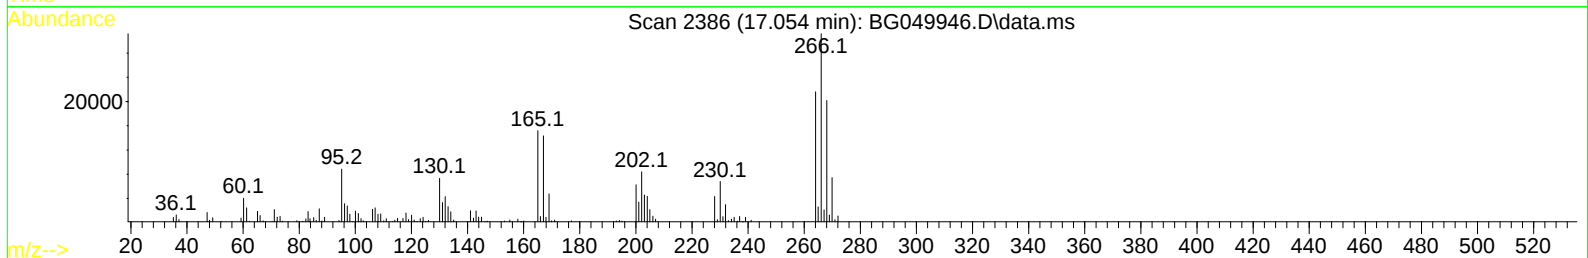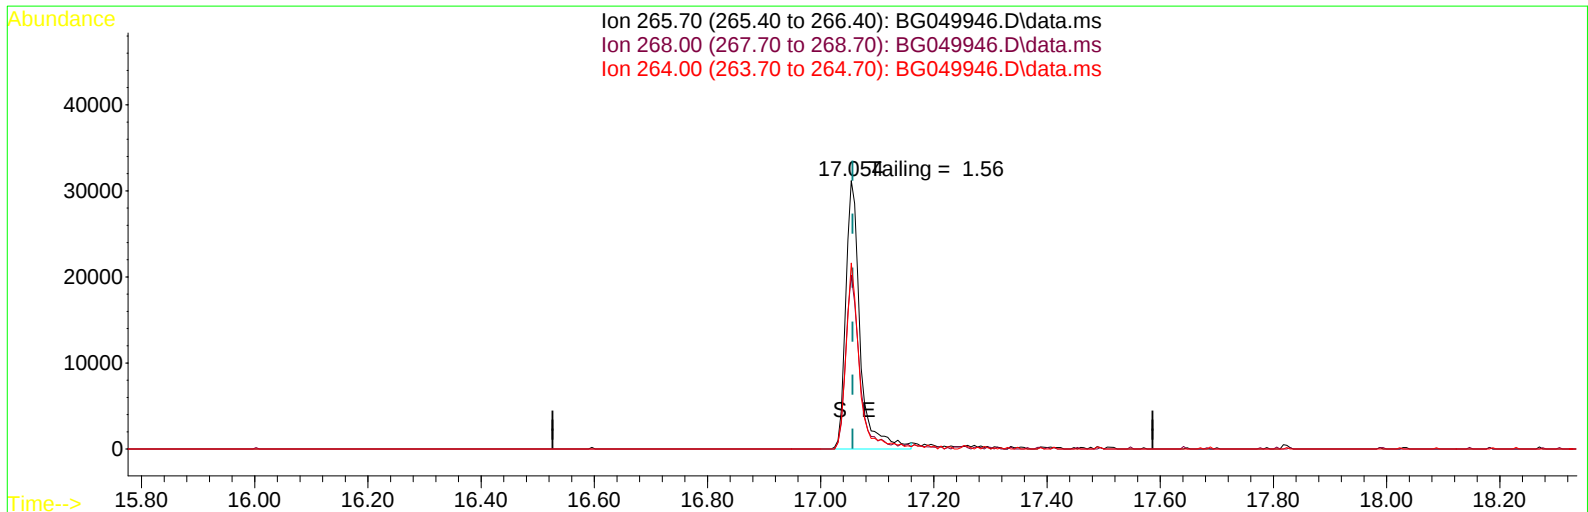

TIC: BG049946.D\data.ms

(70) Pentachlorophenol (C)

17.054min (-0.002) 17628.98 ng




response 54794

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.71
264.00	61.30	69.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082421\
Data File : BG049946.D
Acq On : 24 Aug 2021 10:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 24 11:13:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 16:13:24 2021
Response via : Initial Calibration

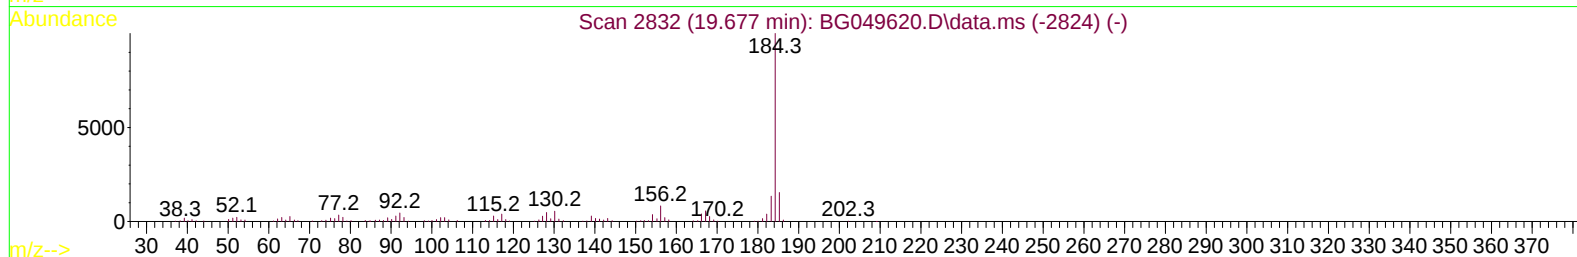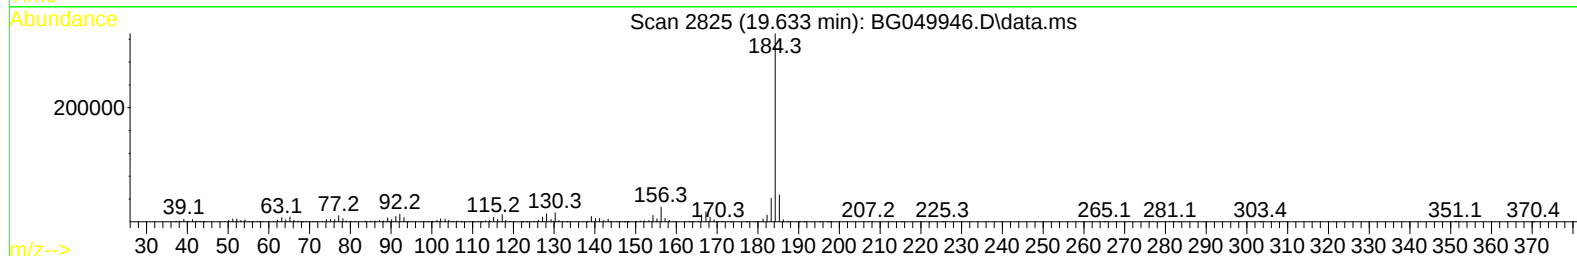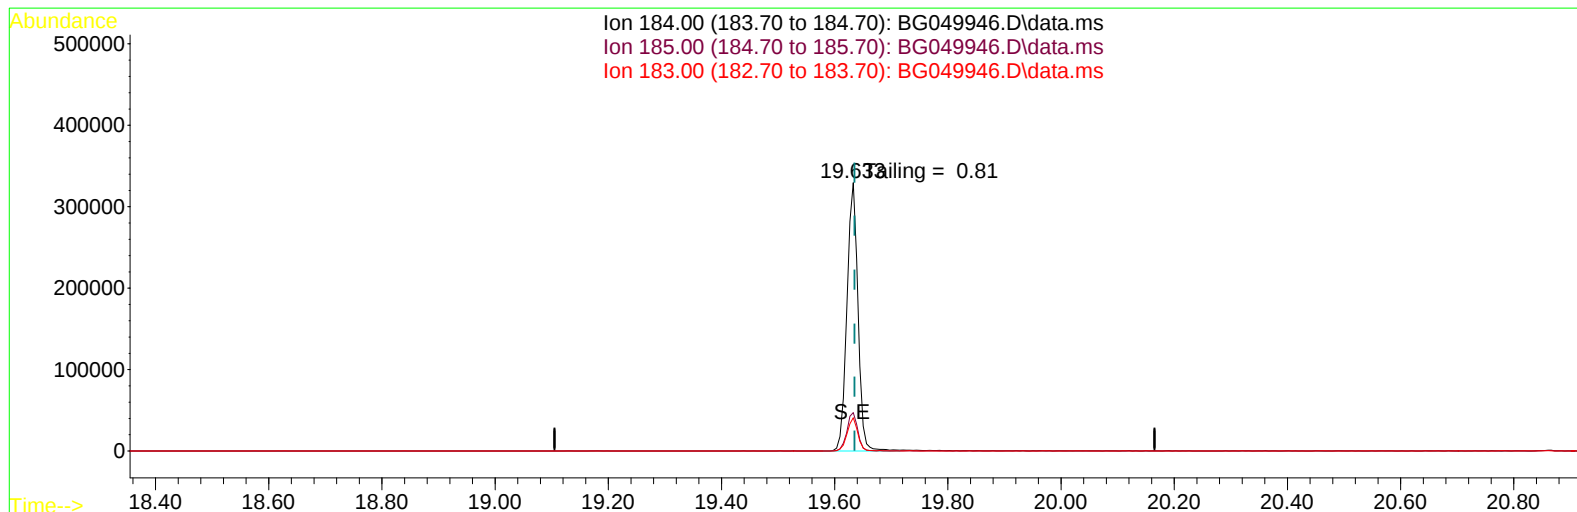

TIC: BG049946.D\data.ms

(77) Benzidine

19.633min (-0.002) 310921.32 ng

response 446122

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.34
183.00	11.70	12.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2021	BNA_G	BG049946.D
Compound Name	Response	Retention Time
DDT	207026	20.86
DDD	7932	20.42
DDE	609	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8541	215567	3.96

Instrument :
BNA_G
ClientSampleId :
DFTPP