
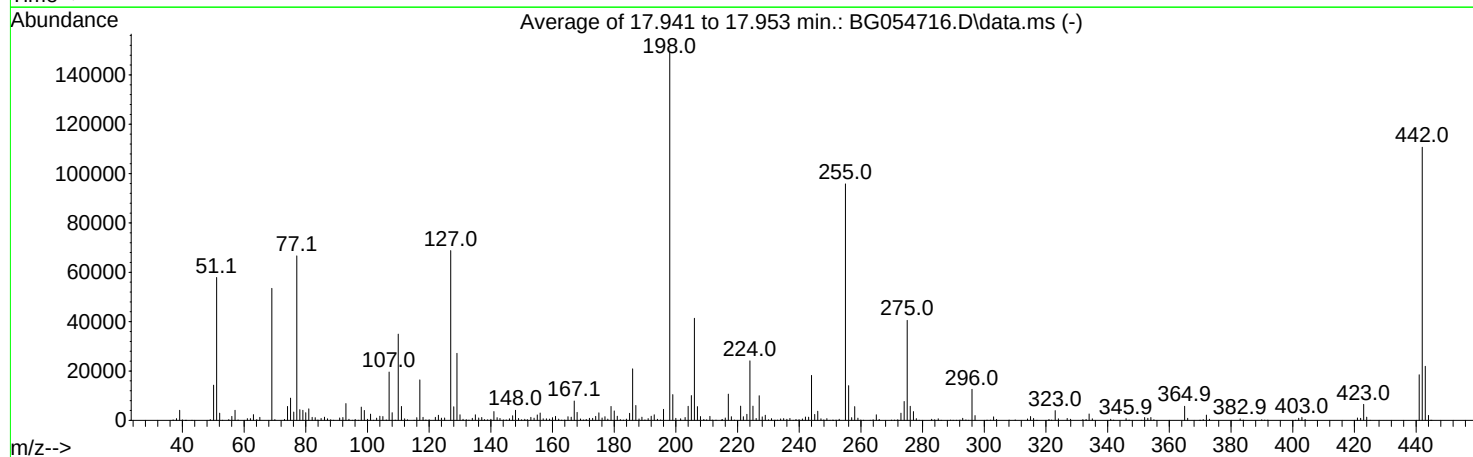


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082422\
 Data File : BG054716.D
 Acq On : 24 Aug 2022 11:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 23 03:09:46 2022

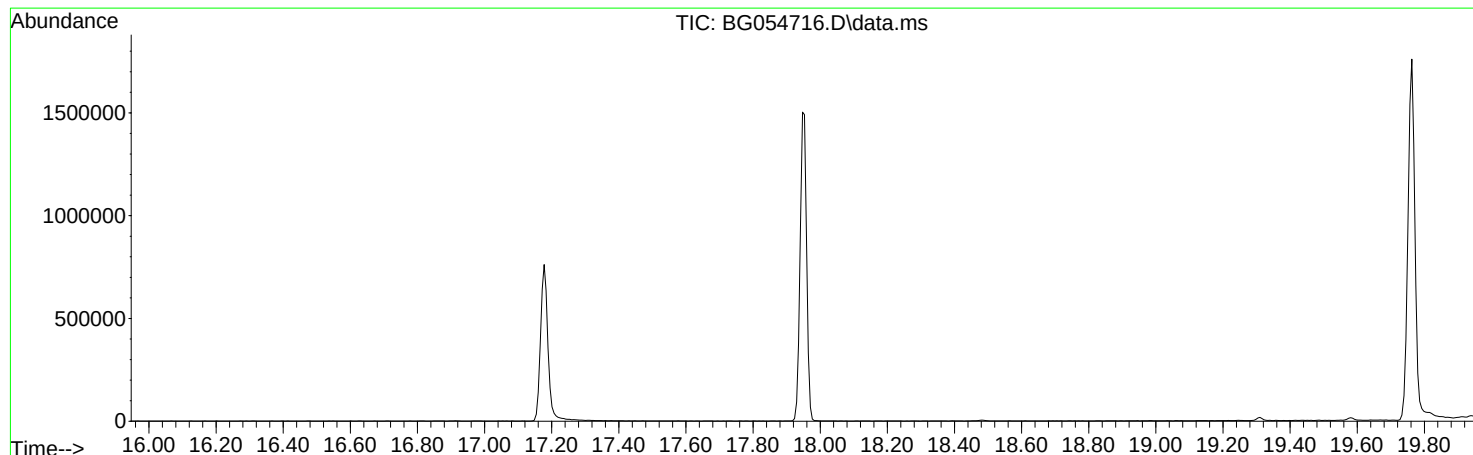




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	57907	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.9	53475	PASS
70	69	0.00	2	0.6	326	PASS
127	198	10	80	46.1	68787	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149085	PASS
199	198	5	9	7.0	10461	PASS
275	198	10	60	27.2	40552	PASS
365	198	1	100	3.8	5707	PASS
441	198	0.01	100	12.4	18480	PASS
442	442	50	100	100.0	110667	PASS
443	442	15	24	19.8	21958	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082422\
 Data File : BG054716.D
 Acq On : 24 Aug 2022 11:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 24 12:08:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 23 03:09:46 2022
 Response via : Initial Calibration

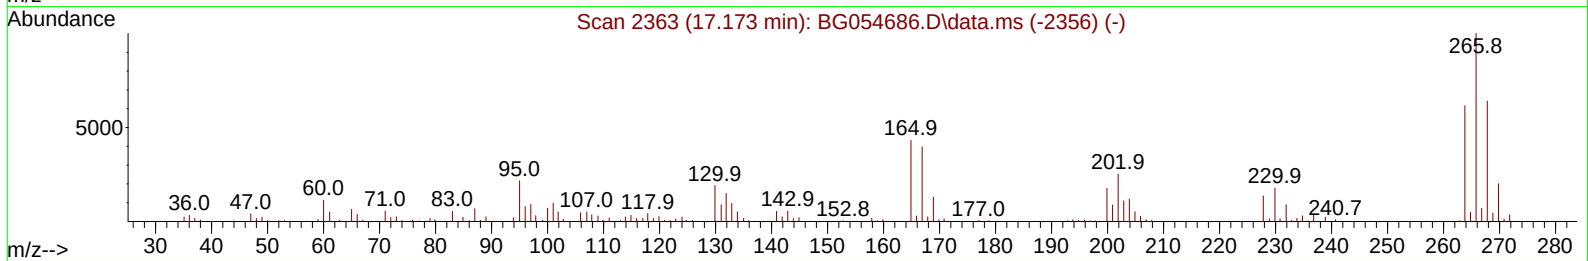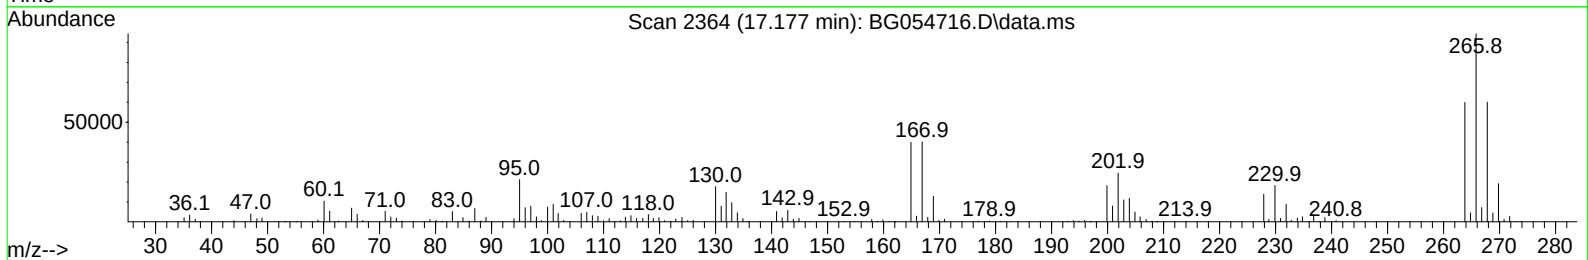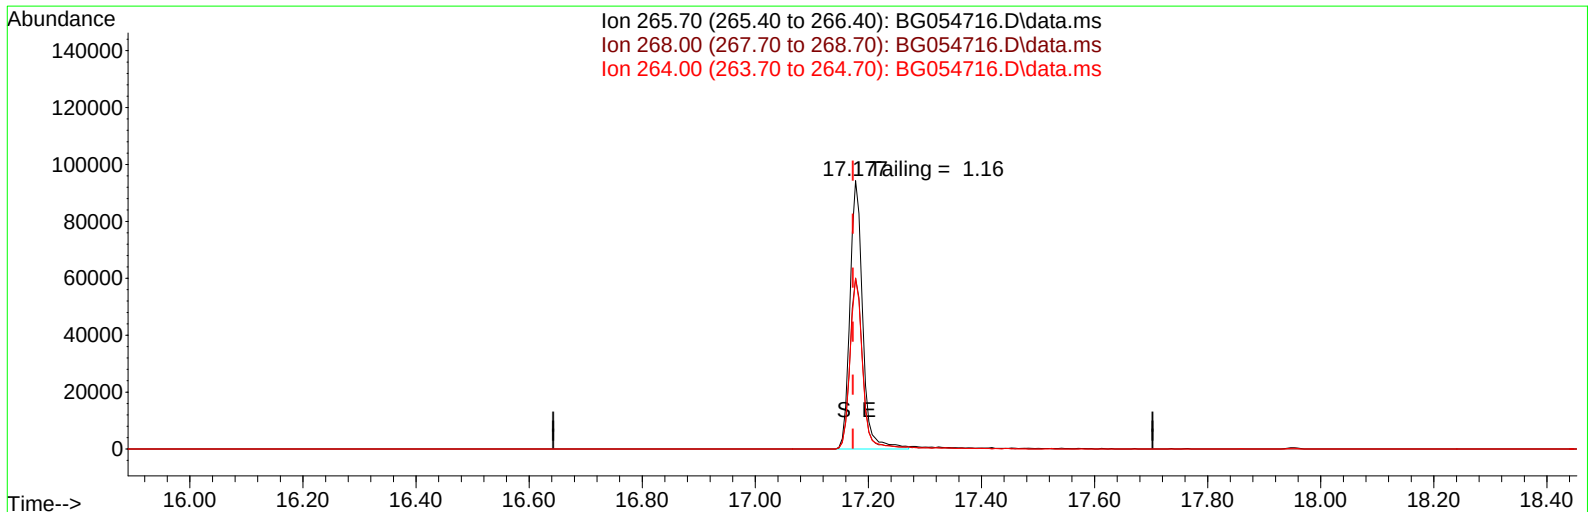

TIC: BG054716.D\data.ms

(70) Pentachlorophenol (C)

17.177min (+ 0.004) 59890.41 ng




response 149989

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.74
264.00	61.70	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082422\
Data File : BG054716.D
Acq On : 24 Aug 2022 11:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 24 12:08:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

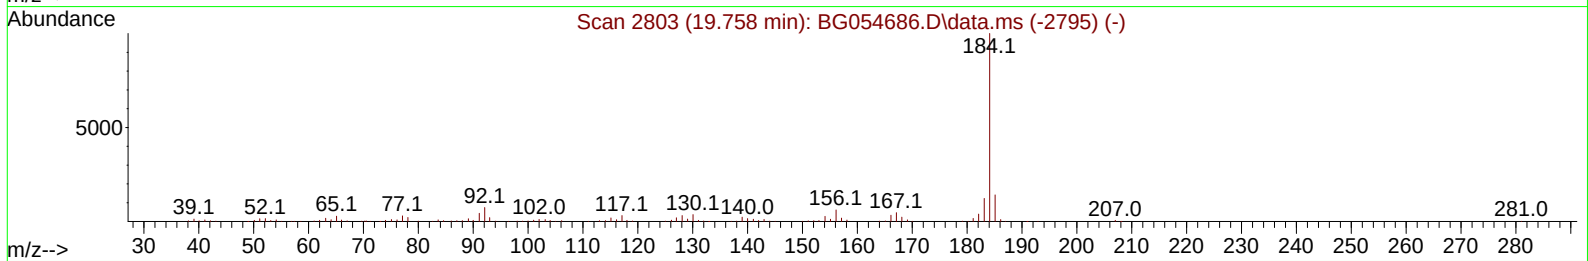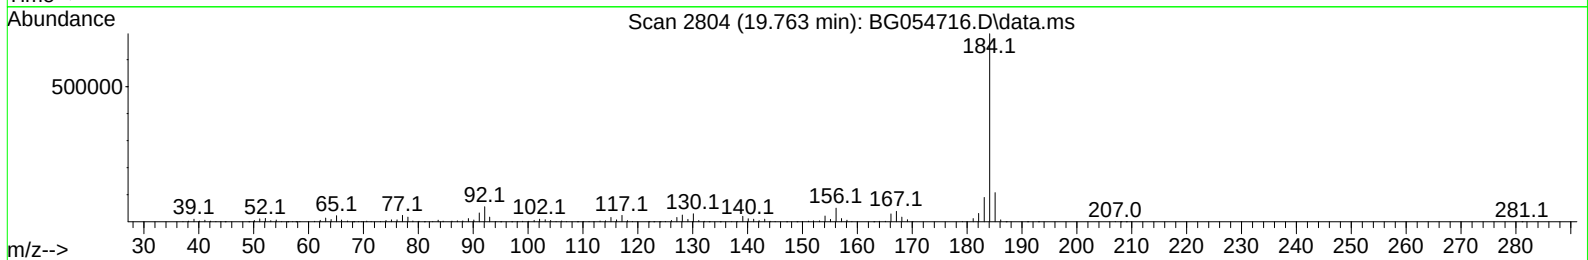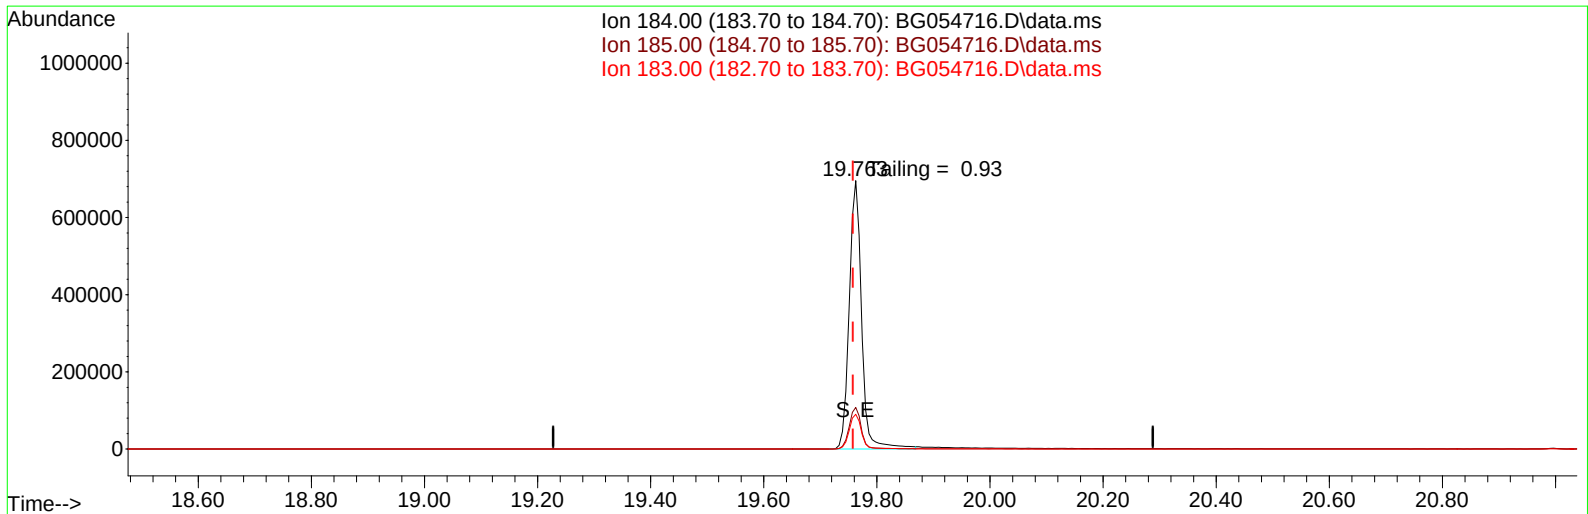

TIC: BG054716.D\data.ms

(77) Benzidine

19.763min (+ 0.005) 25022.58 ng

response 1074641

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.53
183.00	12.30	12.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2022	BNA_G	BG054716.D
Compound Name	Response	Retention Time
DDT	472313	20.996
DDD	16570	20.544
DDE	1979	20.045
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18549	490862	3.78

Instrument :
BNA_G
ClientSampleId :
DFTPP