

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082515\
 Data File : BG018494.D
 Acq On : 25 Aug 2015 17:45
 Operator : UM/MA
 Sample : G3395-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0577

Quant Time: Aug 26 07:07:35 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 26 07:00:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	69628	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	309028	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	211382	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	560984	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	580364	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	568936	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	577	0.37	ng/uL	0.00
5) Phenol-d5	7.17	99	29586	4.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	67187	17.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	67209	13.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	51093	9.62	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	44999	18.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.90	143	44395	18.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	85522	16.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	8545	1.45	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	345766	19.44	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	433454	19.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	14580	4.56	ng/ul	0.00
58) Fluorene-d10	15.63	176	312880	20.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	37104	13.45	ng/ul	0.00
71) Anthracene-d10	17.48	188	526408	19.62	ng/ul	0.00
79) Pyrene-d10	19.76	212	596085	19.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	530804	17.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.09	163	45296	2.58	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082515\
Data File : BG018494.D
Acq On : 25 Aug 2015 17:45
Operator : UM/MA
Sample : G3395-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0577

Quant Time: Aug 26 07:07:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 26 07:00:42 2015
Response via : Initial Calibration

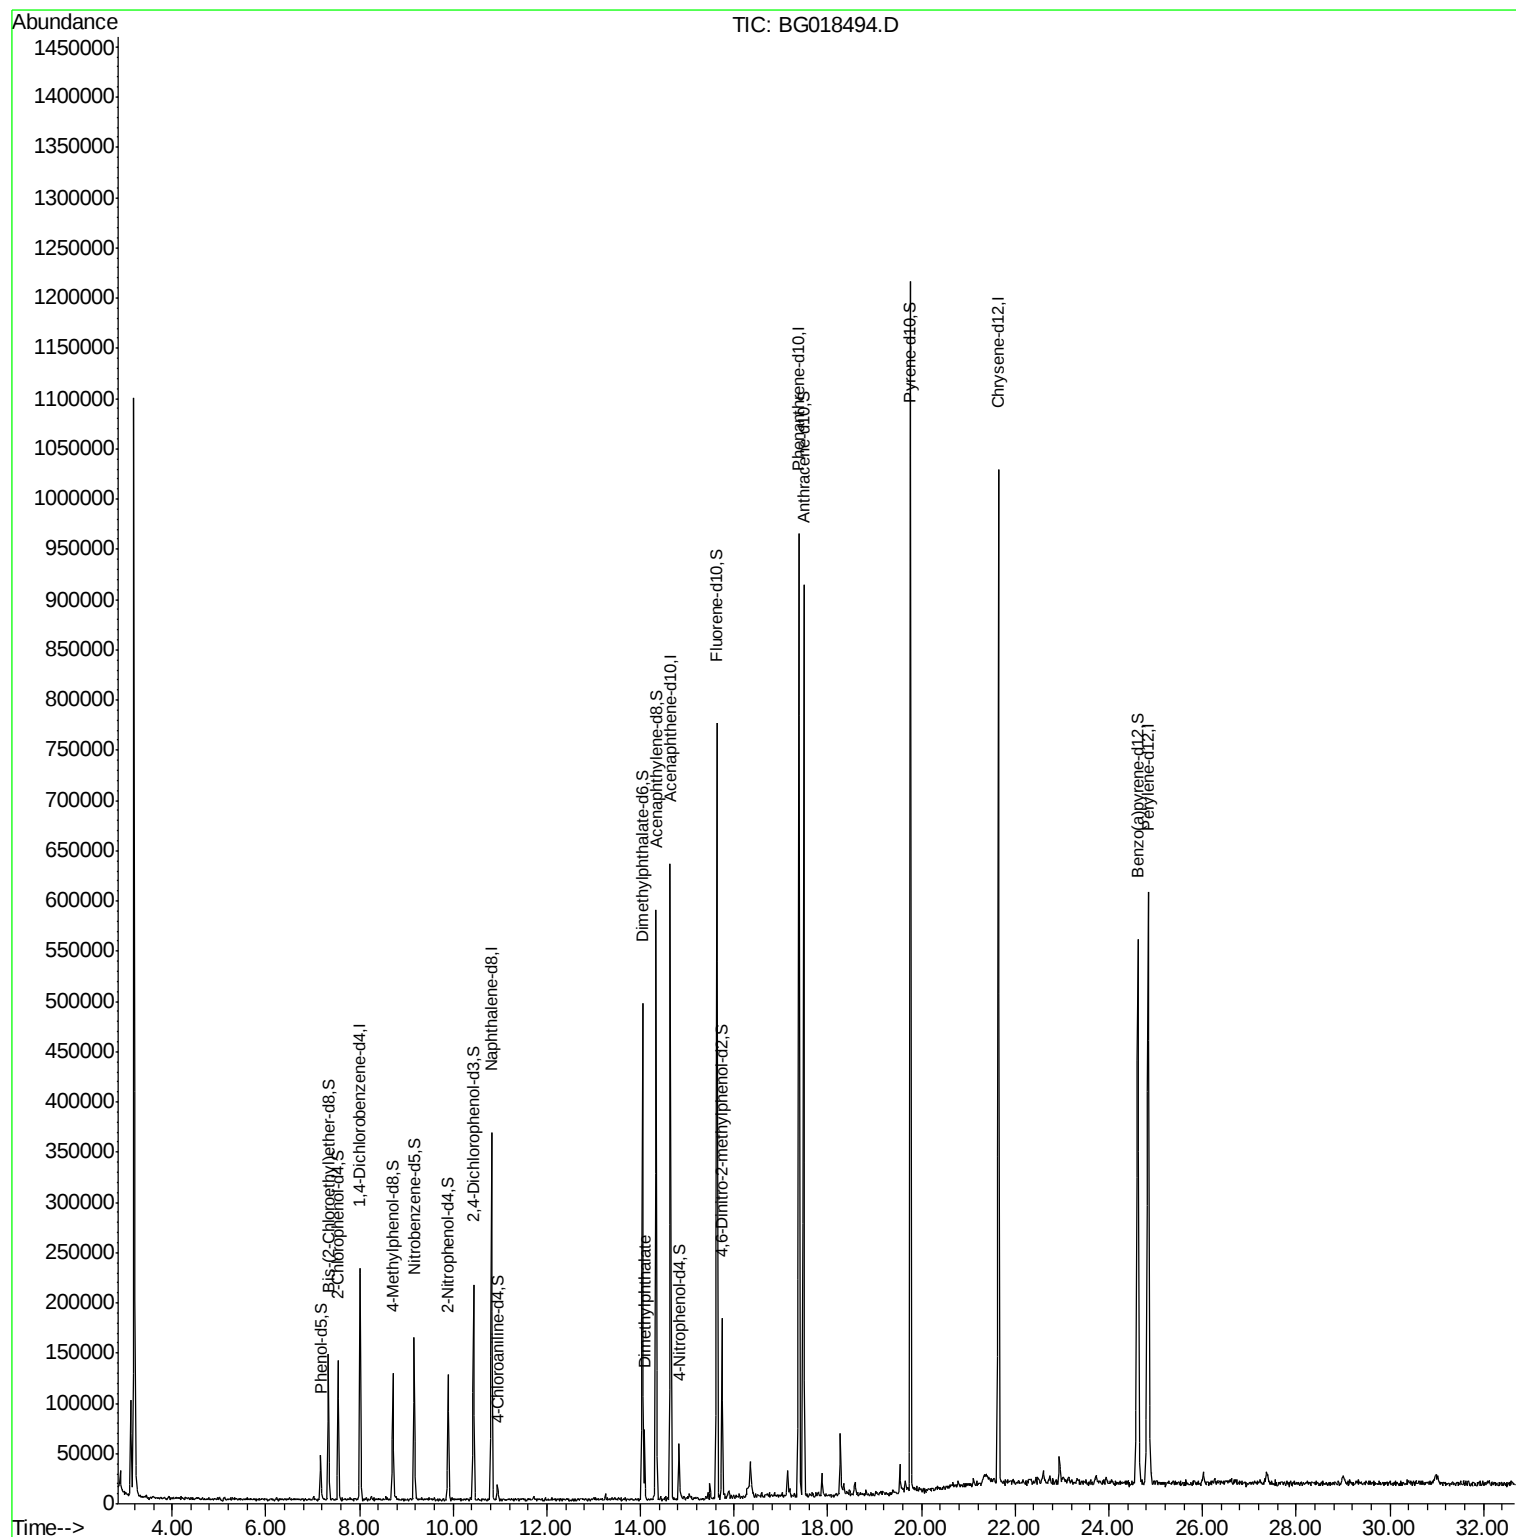

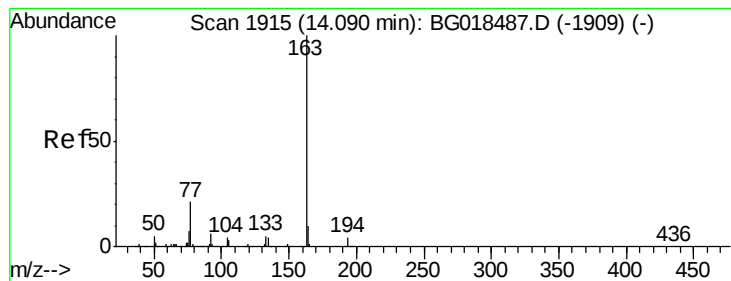

#45

Dimethylphthalate

Concen: 2.58 ng/ul

RT: 14.09 min Scan# 1914

Delta R.T. -0.00 min

Lab File: BG018494.D

Acq: 25 Aug 2015 17:45

Instrument :

BNA_G

ClientSampleId :

C0577

Tgt Ion:163 Resp: 45296

Ion Ratio Lower Upper

163 100

194 4.8 2.9 4.3#

164 10.8 7.7 11.5

