


Data Path : Z:\HPCHEM1\BNA_G\Data\BG082515\
Data File : BG018486.D
Acq On : 25 Aug 2015 12:20
Operator : UM/MA
Sample : DFTPP38
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP38

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Title : SVOA CALIBRATION
Last Update : Thu Aug 20 04:10:50 2015

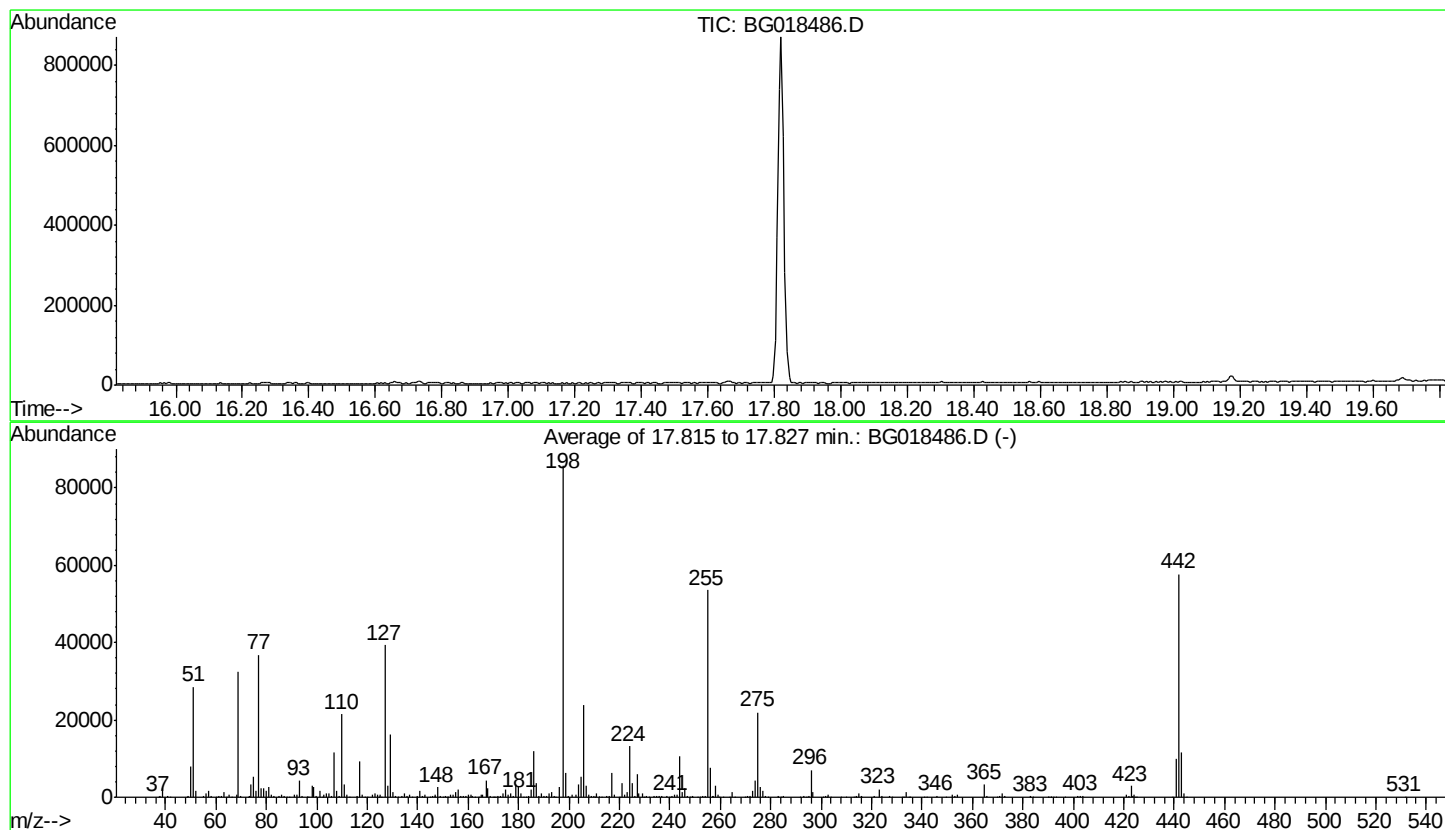

AutoFind: Scans 2549, 2550, 2551; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	28634	PASS
68	69	0.00	2	1.6	511	PASS
69	198	0.00	100	37.8	32398	PASS
70	69	0.00	2	0.8	262	PASS
127	198	10	80	45.9	39338	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	85792	PASS
199	198	5	9	7.3	6286	PASS
275	198	10	60	25.6	21973	PASS
365	198	1	100	3.8	3265	PASS
441	442	0.01	24	17.1	9840	PASS
442	198	50	100	67.2	57680	PASS
443	442	15	24	20.1	11617	PASS