

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082515\
 Data File : BG018493.D
 Acq On : 25 Aug 2015 17:07
 Operator : UM/MA
 Sample : G3395-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0576

Quant Time: Aug 26 07:07:29 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 26 07:00:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	70111	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	310541	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	205941	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	548754	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	583343	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	568760	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.44	96	1688	1.06	ng/uL	0.00
5) Phenol-d5	7.17	99	65521	10.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	89135	22.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	99237	20.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	92299	17.26	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	57360	23.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	57611	23.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	115555	22.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	4434	0.75	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	424769	24.51	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	527384	24.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.88	143	655	0.21	ng/ul	0.05
58) Fluorene-d10	15.63	176	378620	25.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	49113	18.20	ng/ul	0.00
71) Anthracene-d10	17.48	188	627120	23.89	ng/ul	0.00
79) Pyrene-d10	19.77	212	702404	23.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.62	264	676003	22.39	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.08	163	61026	3.57	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082515\
Data File : BG018493.D
Acq On : 25 Aug 2015 17:07
Operator : UM/MA
Sample : G3395-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0576

Quant Time: Aug 26 07:07:29 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 26 07:00:42 2015
Response via : Initial Calibration

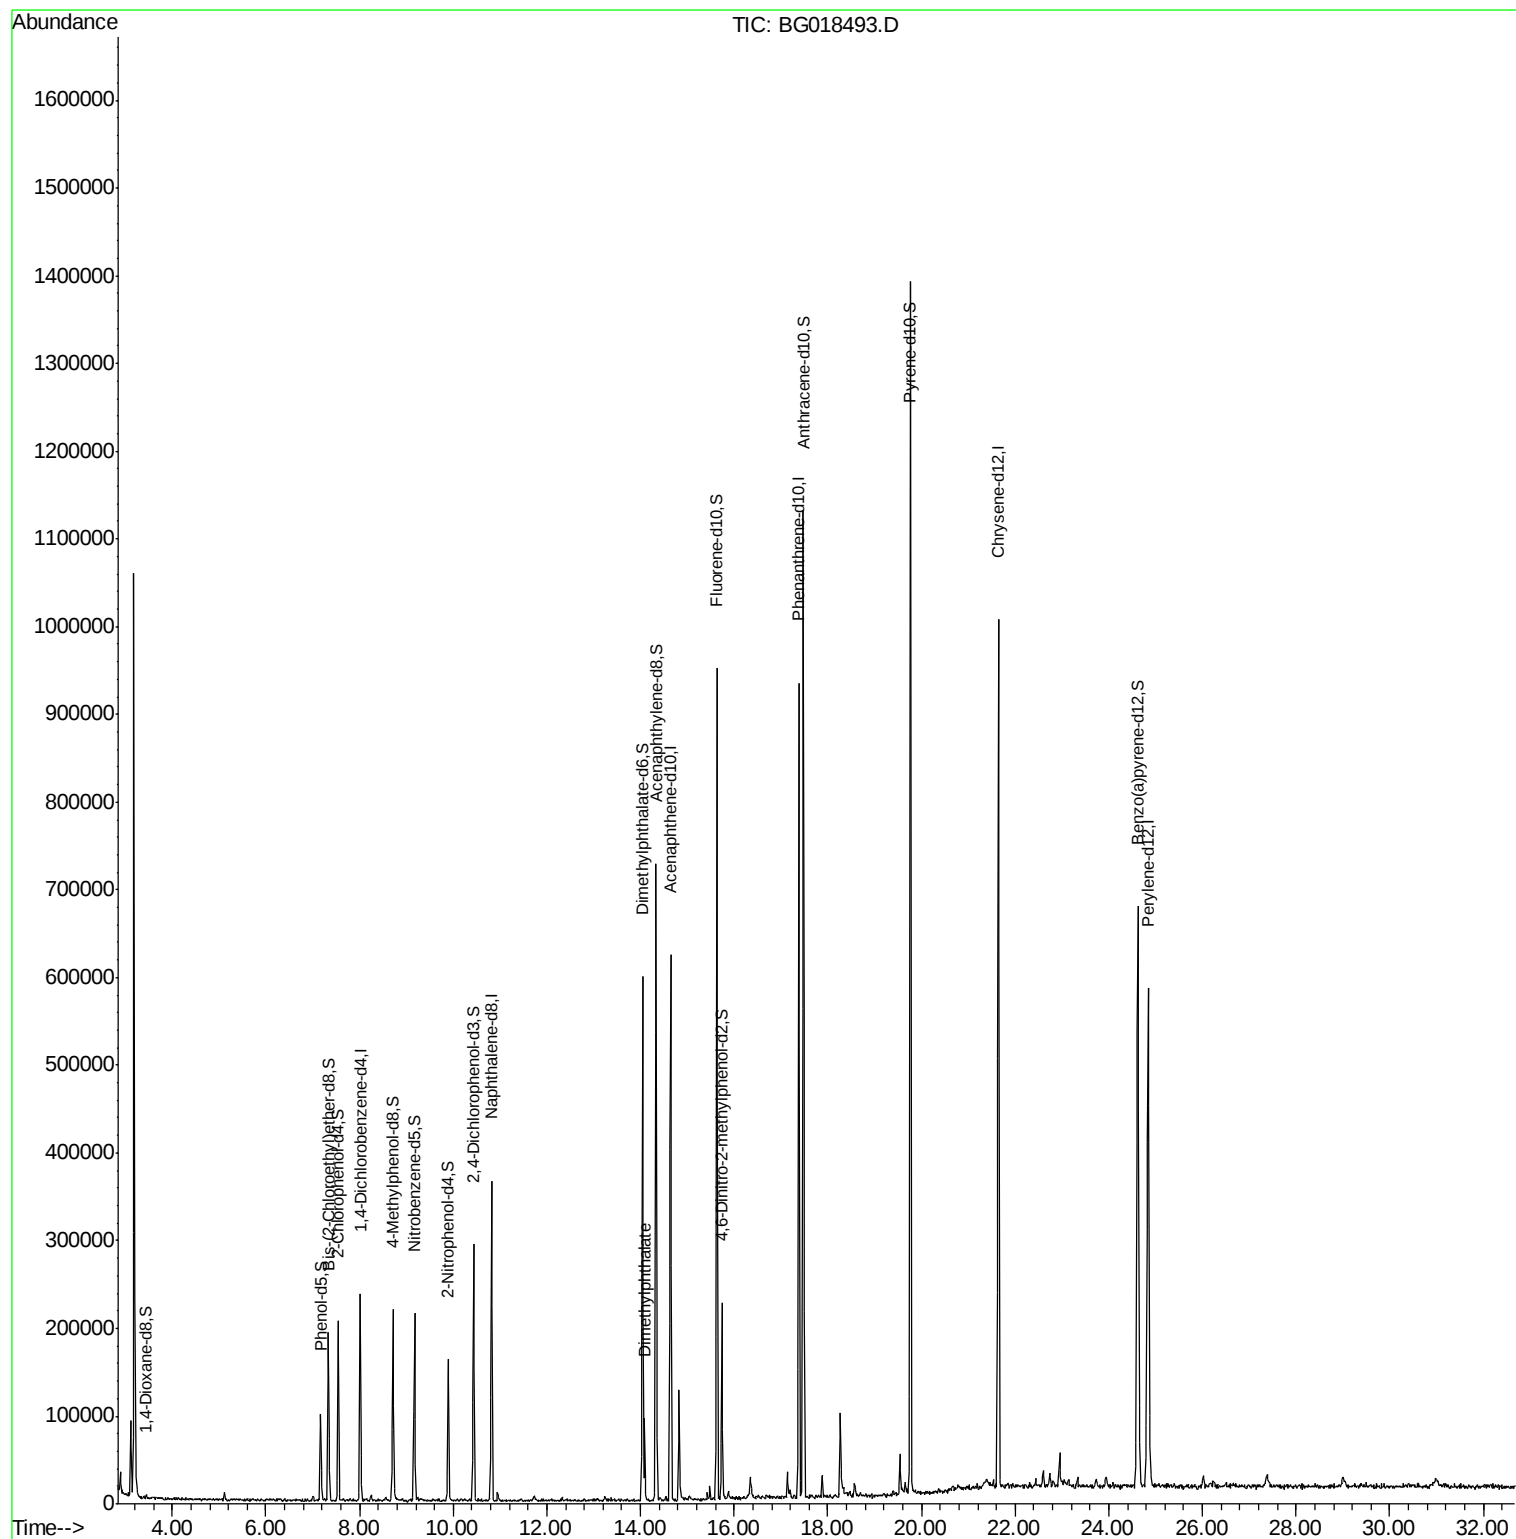

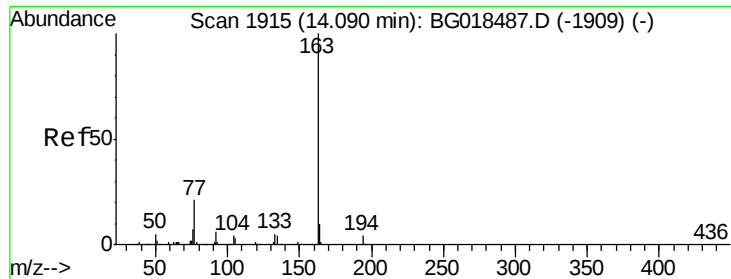

#45
 Dimethylphthalate
 Concen: 3.57 ng/ul
 RT: 14.08 min Scan# 1914
 Delta R.T. -0.01 min
 Lab File: BG018493.D
 Acq: 25 Aug 2015 17:07

Instrument :
 BNA_G
 ClientSampleId :
 C0576

Tgt Ion:163 Resp: 61026
 Ion Ratio Lower Upper
 163 100
 194 4.3 2.9 4.3
 164 11.0 7.7 11.5

