

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
 Data File : BG023906.D
 Acq On : 25 Aug 2016 22:58
 Operator : UM/SJ
 Sample : H4588-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-04

Quant Time: Aug 26 01:06:54 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 24 17:42:04 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	123854	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	542247	20.00	ng	0.00
38) Acenaphthene-d10	14.76	164	343463	20.00	ng	0.00
63) Phenanthrene-d10	17.53	188	759780	20.00	ng	0.00
75) Chrysene-d12	21.85	240	795028	20.00	ng	0.00
86) Perylene-d12	25.24	264	793561	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	386368	52.51	ng	0.00
7) Phenol-d6	7.25	99	368765	32.18	ng	0.00
23) Nitrobenzene-d5	9.27	82	839618	76.98	ng	0.00
41) 2,4,6-Tribromophenol	16.27	330	441041	87.79	ng	0.00
44) 2-Fluorobiphenyl	13.38	172	1565524	76.88	ng	0.00
78) Terphenyl-d14	20.14	244	1955359	74.63	ng	0.00
Target Compounds						
9) Benzaldehyde	7.23	77	546	Below Cal	#	8
32) Benzoic acid	10.26	122	200	6.46 ng	#	1
49) Dimethylphthalate	14.20	163	211218	8.02 ng		99
73) Di-n-butylphthalate	18.46	149	2119	Below Cal	#	38
74) Fluoranthene	19.59	202	2078	Below Cal	#	1
77) Pyrene	19.97	202	2709	Below Cal	#	36

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023906.D
Acq On : 25 Aug 2016 22:58
Operator : UM/SJ
Sample : H4588-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-04

Quant Time: Aug 26 01:06:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

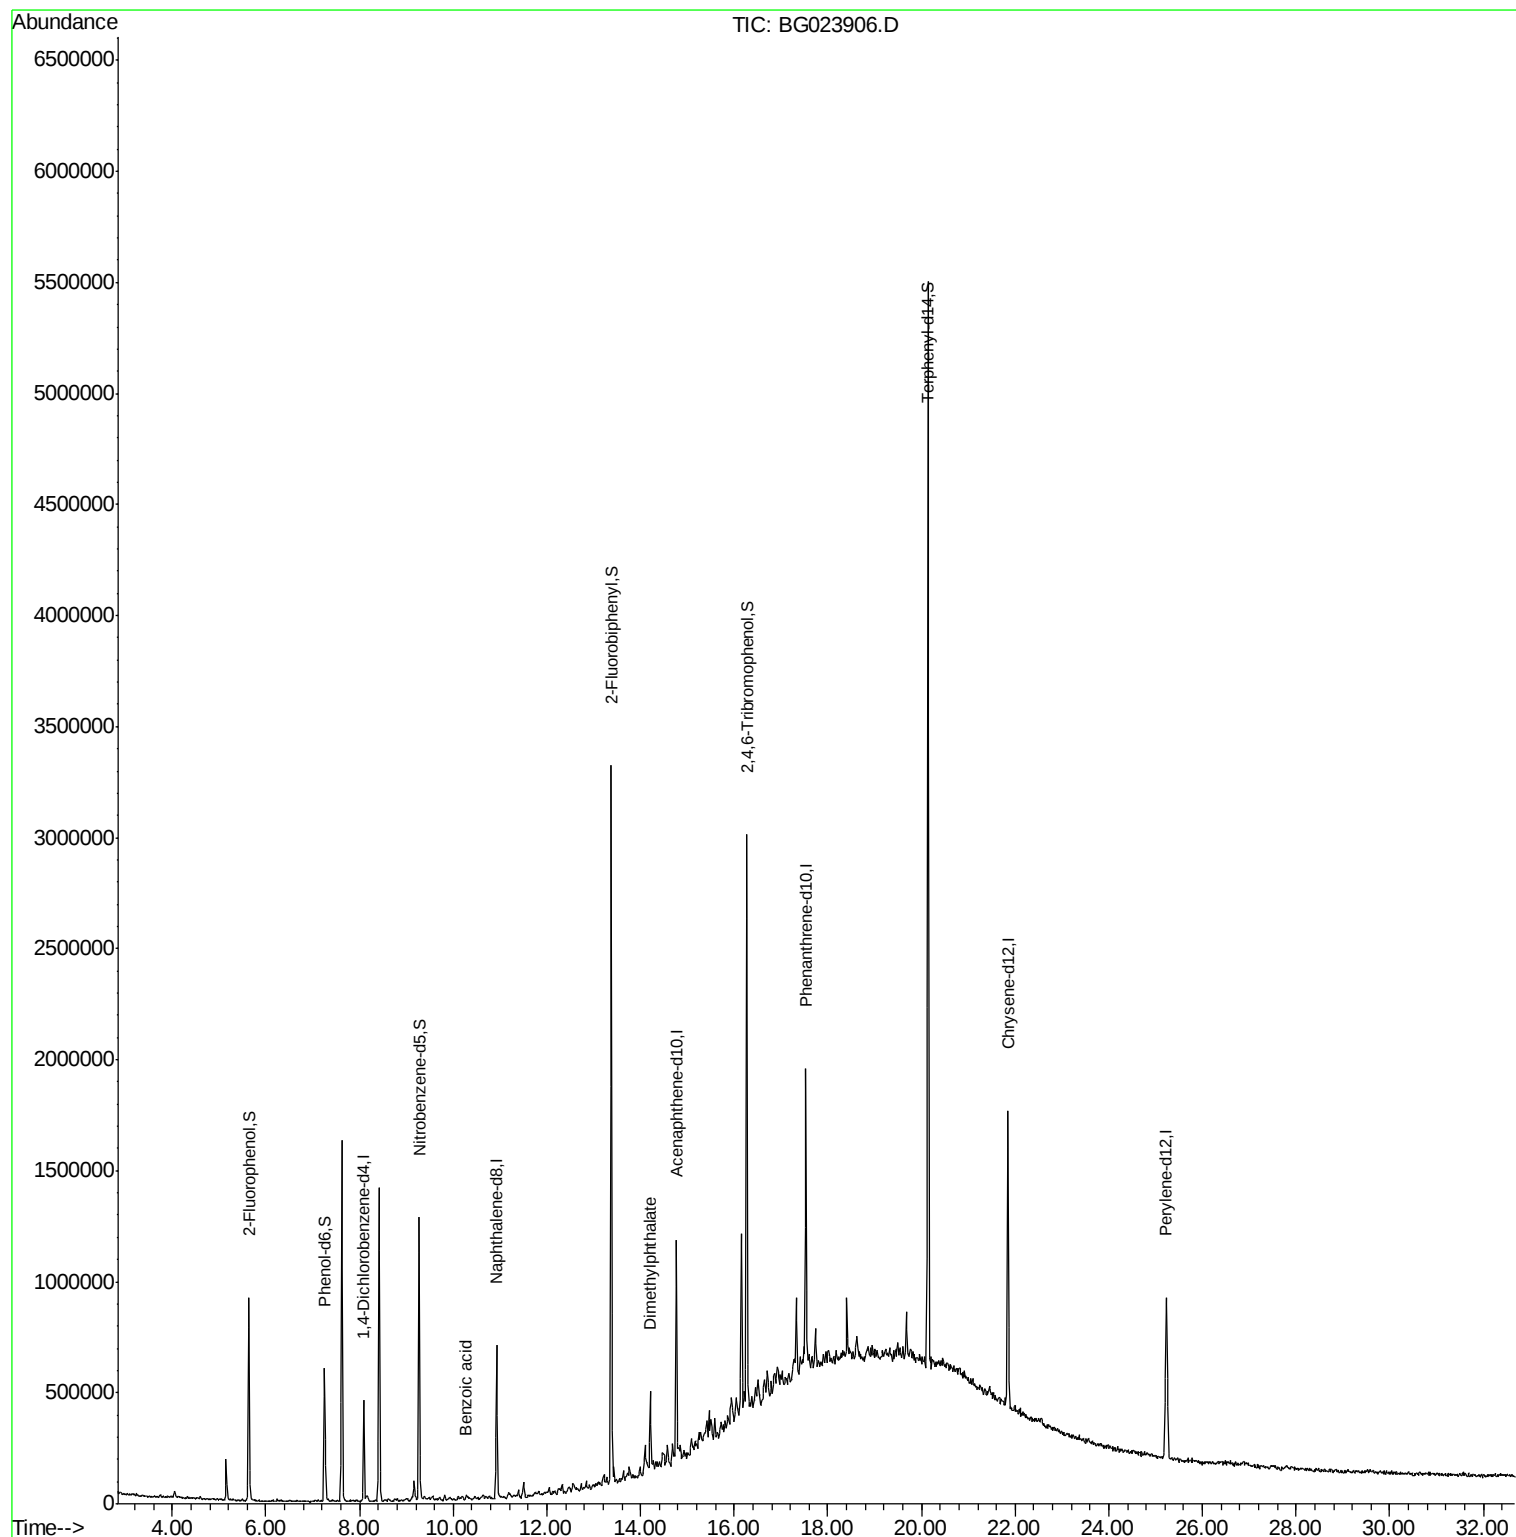



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.09 min Scan# 894

Delta R.T. -0.01 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58





Instrument :

BNA_G

ClientSampleId :

MW-04

Tgt Ion:	152	Resp:	123854
Ion	Ratio	Lower	Upper
152	100		
150	158.7	144.7	217.1
115	58.7	64.0	96.0#

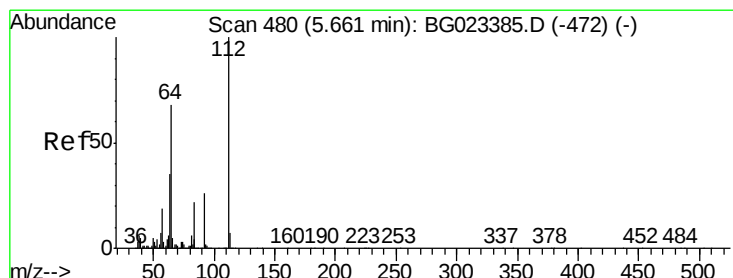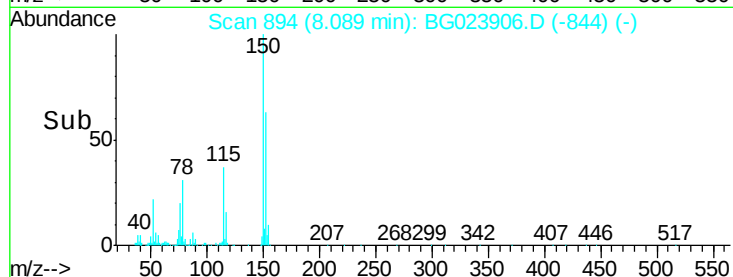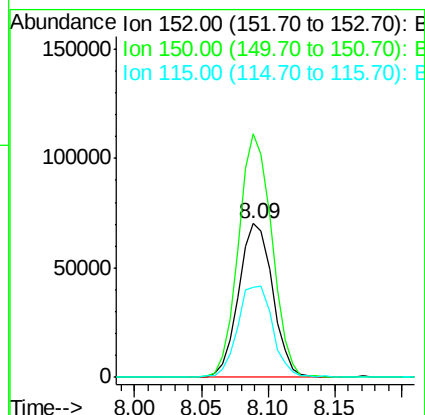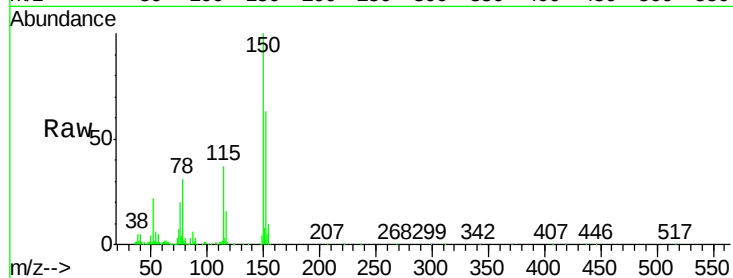

#5

2-Fluorophenol

Concen: 52.51 ng




RT: 5.63 min Scan# 476


Delta R.T. -0.01 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58

Tgt Ion:	112	Resp:	386368
Ion	Ratio	Lower	Upper
112	100		
64	68.5	59.0	88.4
63	38.0	37.8	56.8

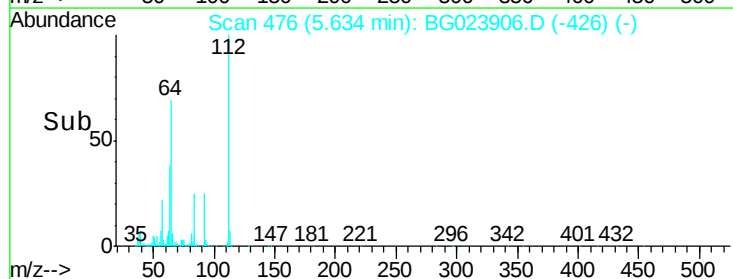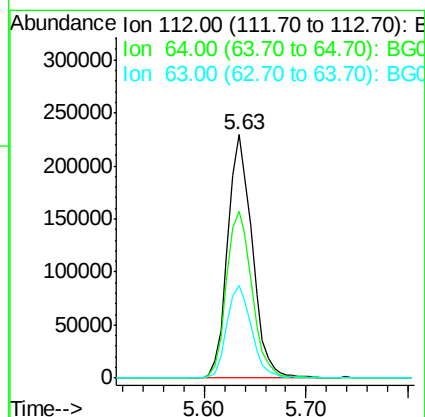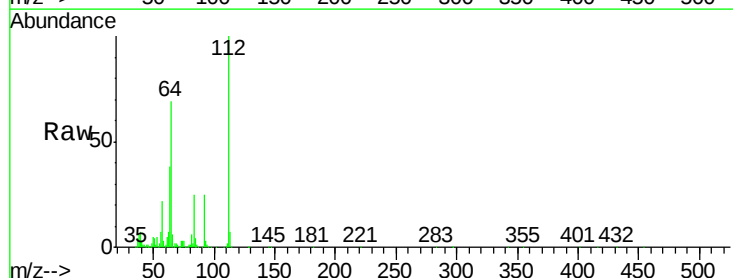

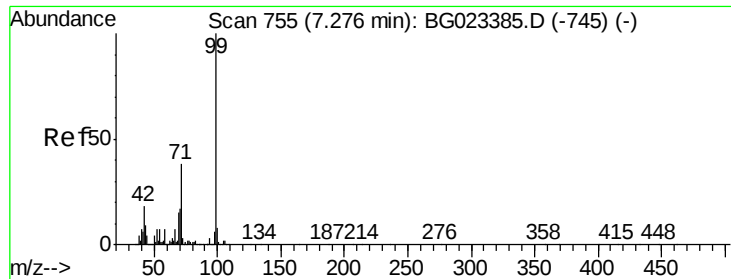

#7

Phenol-d6

Concen: 32.18 ng

RT: 7.25 min Scan# 751

Delta R.T. -0.01 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58

Instrument :

BNA_G

ClientSampled :

MW-04


Tgt Ion: 99 Resp: 368765

Ion Ratio Lower Upper




99 100

42 17.8 17.8 26.6

71 40.9 41.5 62.3#

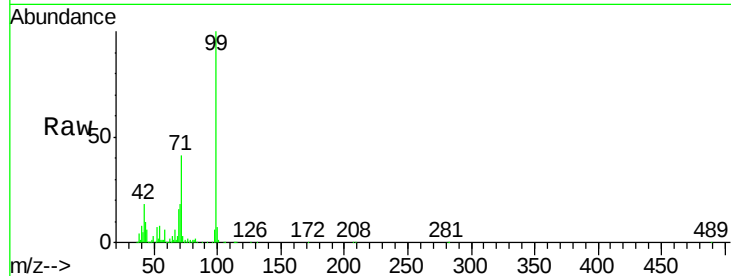

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

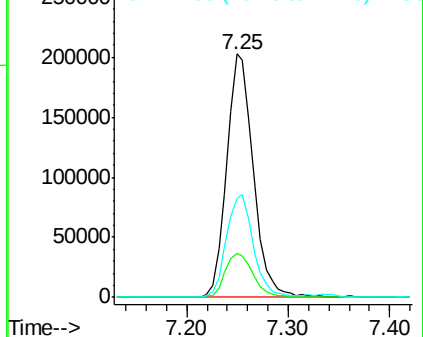

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1377

Delta R.T. -0.01 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58

Tgt Ion: 136 Resp: 542247


Ion Ratio Lower Upper

136 100



137 11.3 9.6 14.4

54 10.0 7.3 10.9

68 7.0 5.3 7.9



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




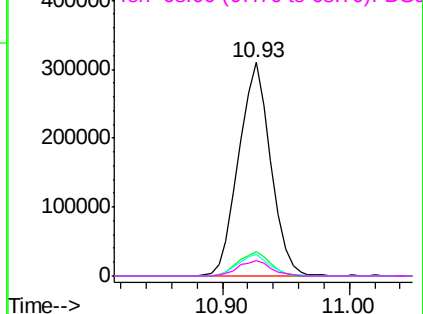




#23
 Nitrobenzene-d5
 Concen: 76.98 ng
 RT: 9.27 min Scan# 1095
 Delta R.T. -0.01 min
 Lab File: BG023906.D
 Acq: 25 Aug 2016 22:58




Instrument :
 BNA_G
 ClientSampleId :
 MW-04


Tgt Ion	Ratio	Lower	Upper
82	100		
128	36.6	24.4	36.6
54	49.7	41.4	62.0

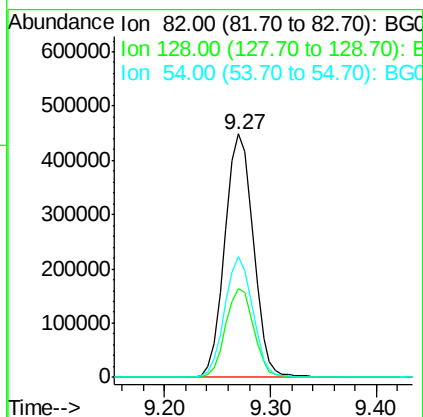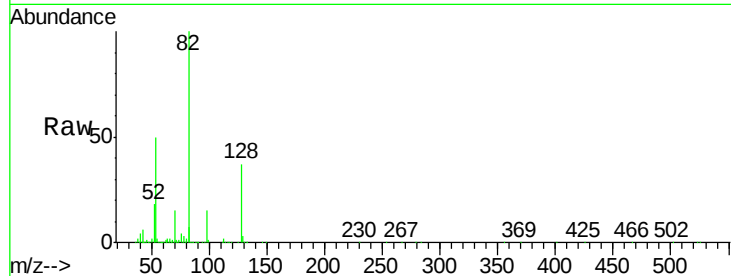

#32
 Benzoic acid
 Concen: 6.46 ng
 RT: 10.26 min Scan# 1263
 Delta R.T. -0.01 min
 Lab File: BG023906.D
 Acq: 25 Aug 2016 22:58

Tgt Ion	Ratio	Lower	Upper
122	100		
105	0.0	117.2	157.2#
77	0.0	109.2	149.2#


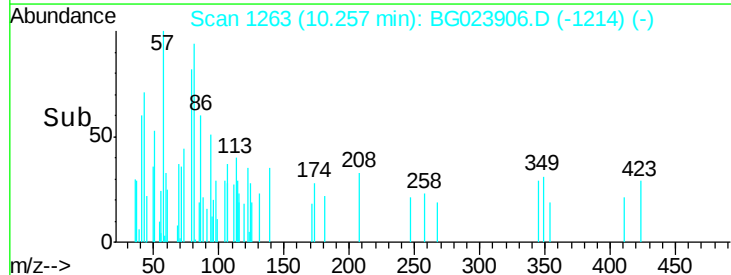
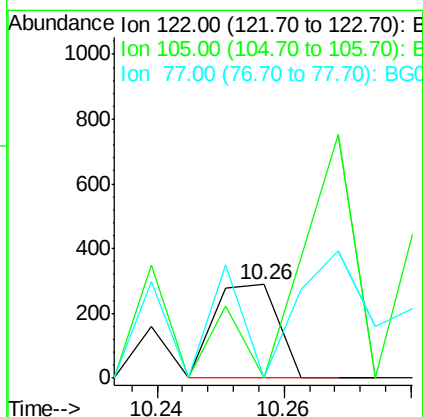



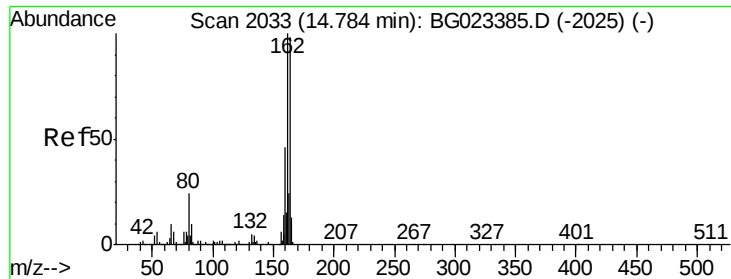

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.76 min Scan# 2030
Delta R.T. -0.01 min
Lab File: BG023906.D
Acq: 25 Aug 2016 22:58




Instrument :
BNA_G
ClientSampleId :
MW-04


Tgt Ion	Ratio	Lower	Upper
164	100		
162	100.9	87.7	131.5
160	47.0	37.2	55.8

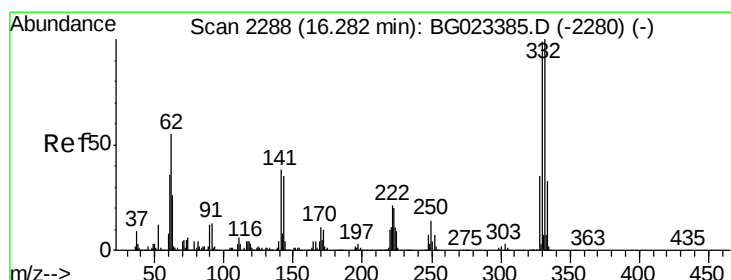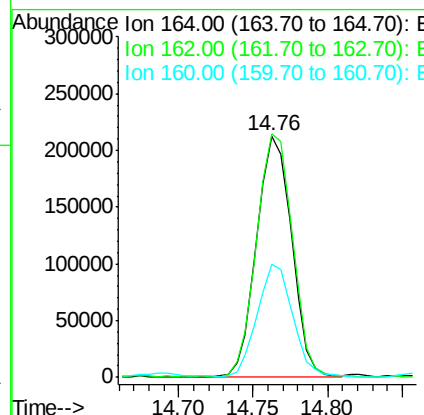

#41
2,4,6-Tribromophenol
Concen: 87.79 ng
RT: 16.27 min Scan# 2287
Delta R.T. 0.01 min
Lab File: BG023906.D
Acq: 25 Aug 2016 22:58

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.2	77.4	116.2
141	44.3	31.7	47.5



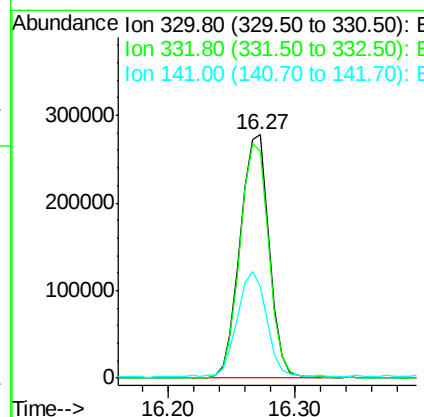
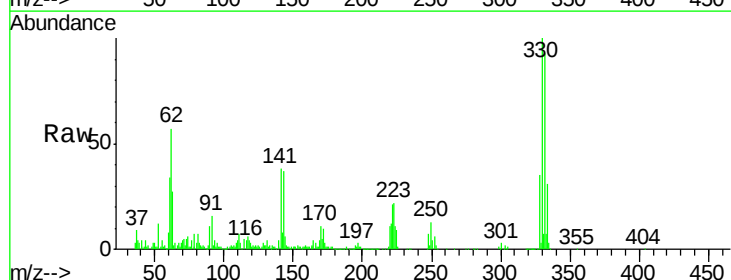


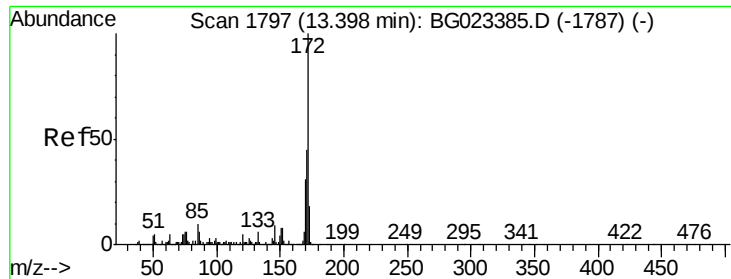

#44
2-Fluorobiphenyl
Concen: 76.88 ng
RT: 13.38 min Scan# 1794
Delta R.T. -0.01 min
Lab File: BG023906.D
Acq: 25 Aug 2016 22:58




Instrument :
BNA_G
ClientSampleId :
MW-04


Tgt Ion:172 Resp: 1565524
Ion Ratio Lower Upper
172 100
171 39.3 31.6 47.4
170 28.0 21.3 31.9

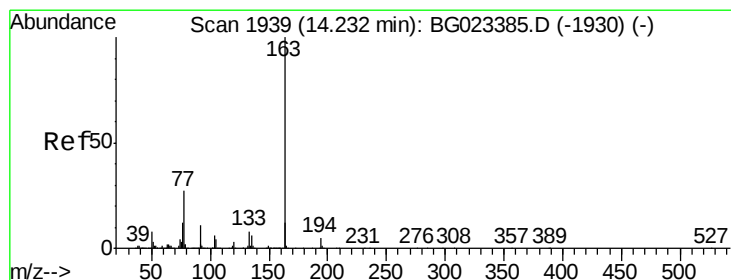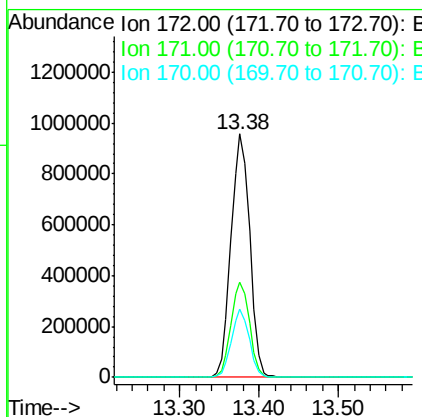

#49
Dimethylphthalate
Concen: 8.02 ng
RT: 14.20 min Scan# 1935
Delta R.T. -0.01 min
Lab File: BG023906.D
Acq: 25 Aug 2016 22:58

Tgt Ion:163 Resp: 211218
Ion Ratio Lower Upper
163 100
194 3.9 3.6 5.4
164 10.4 8.1 12.1

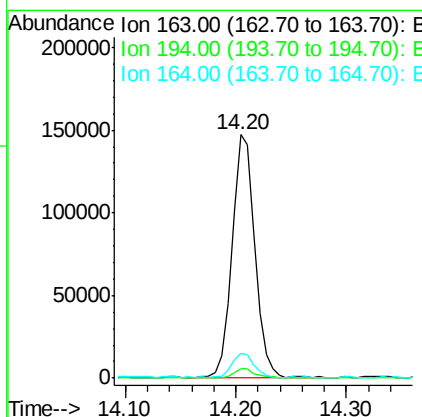

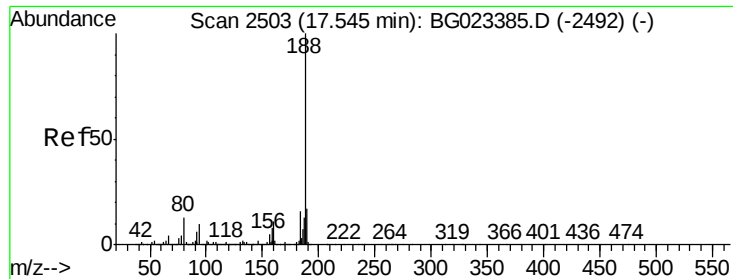

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.53 min Scan# 2501

Delta R.T. 0.00 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58

Instrument :

BNA_G

ClientSampleId :

MW-04


Tgt Ion:188 Resp: 759780

Ion Ratio Lower Upper

188 100

94 10.3 5.2 7.8#




80 12.5 7.2 10.8#

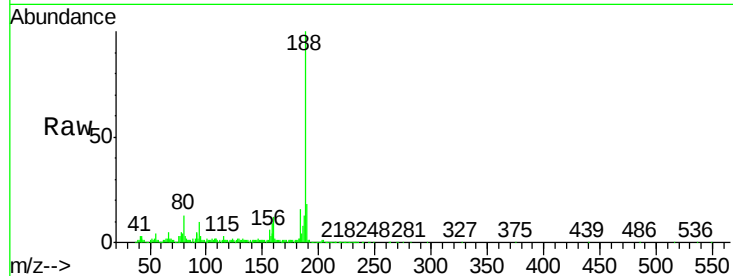

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

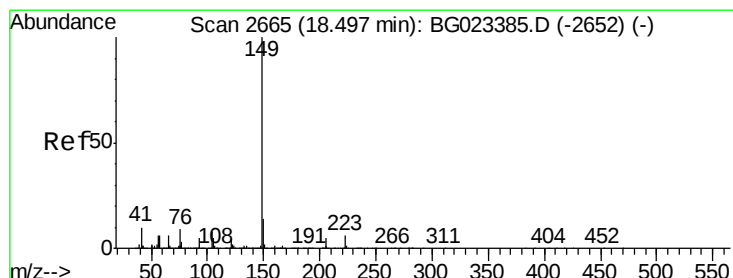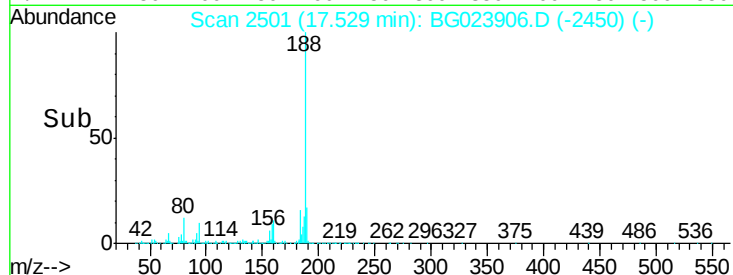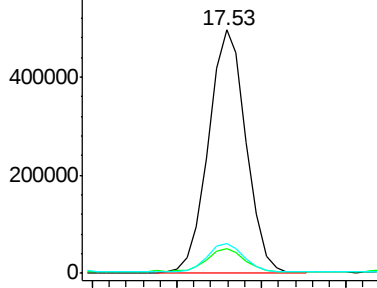

#73

Di-n-butylphthalate

Concen: Below Cal

RT: 18.46 min Scan# 2660

Delta R.T. -0.01 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58


Tgt Ion:149 Resp: 2119

Ion Ratio Lower Upper

149 100

150 39.2 9.1 13.7#



104 25.7 6.9 10.3#

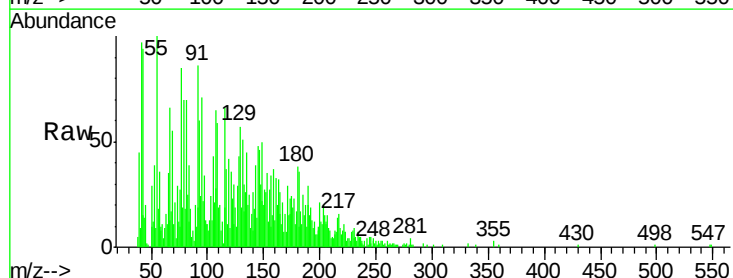


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

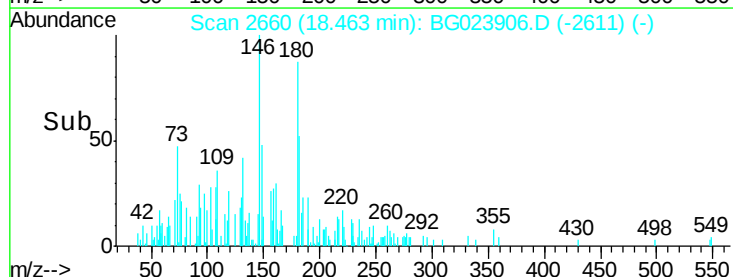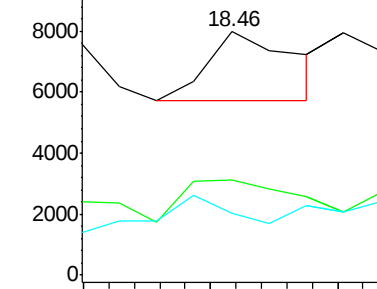



#74

Fluoranthene

Concen: Below Cal

RT: 19.59 min Scan# 2851

Delta R.T. 0.00 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58

Instrument :

BNA_G

ClientSampleId :

MW-04


Tgt Ion:202 Resp: 2078

Ion Ratio Lower Upper

202 100

101 31.2 0.0 27.4#




203 81.6 1.7 41.7#

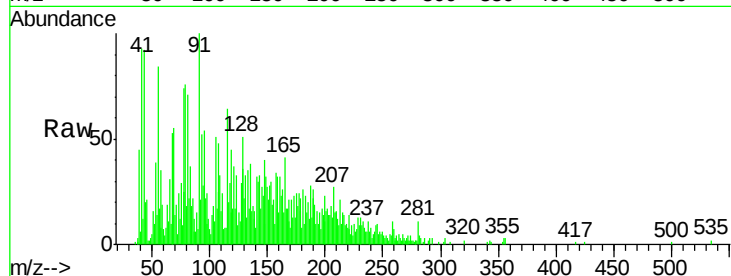

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

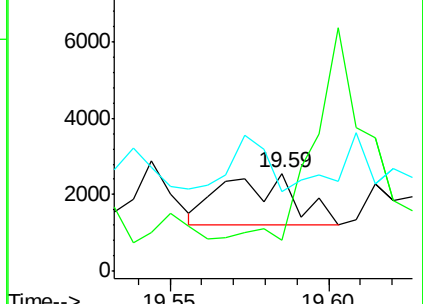

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.85 min Scan# 3236

Delta R.T. 0.00 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58


Tgt Ion:240 Resp: 795028

Ion Ratio Lower Upper

240 100

120 9.3 4.1 6.1#



236 25.2 21.1 31.7




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

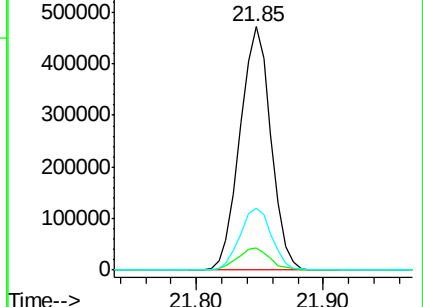



#77

Pyrene

Concen: Below Cal

RT: 19.97 min Scan# 2916

Delta R.T. 0.02 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58

Instrument :

BNA_G

ClientSampled :

MW-04


Tgt Ion:202 Resp: 2709

Ion Ratio Lower Upper

202 100

200 52.7 21.2 31.8#




203 58.5 16.8 25.2#

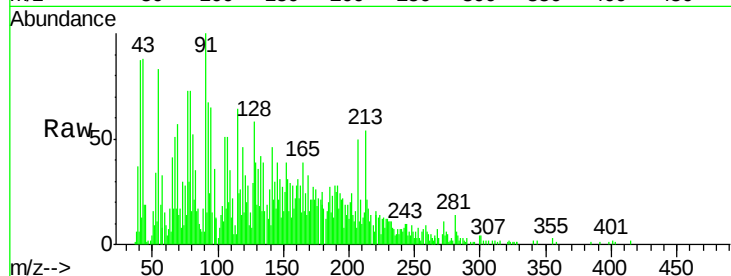

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

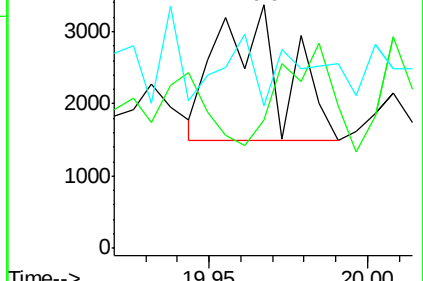

#78

Terphenyl-d14

Concen: 74.63 ng

RT: 20.14 min Scan# 2945

Delta R.T. 0.00 min

Lab File: BG023906.D

Acq: 25 Aug 2016 22:58


Tgt Ion:244 Resp: 1955359

Ion Ratio Lower Upper

244 100

212 11.4 10.8 16.2



122 11.2 8.0 12.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

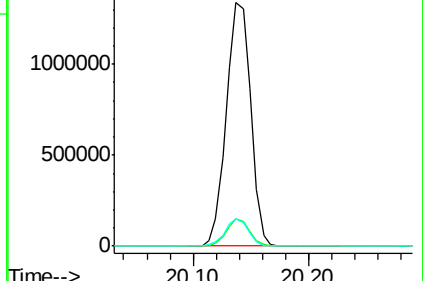

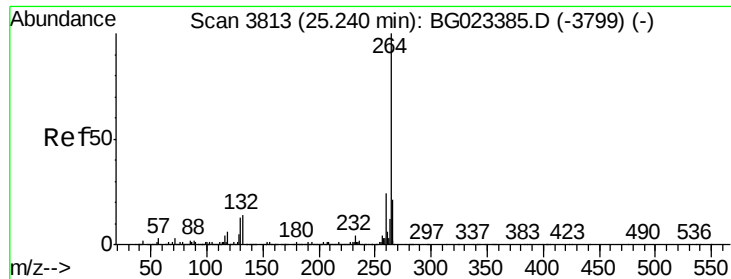

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.24 min Scan# 3813
Delta R.T. 0.01 min
Lab File: BG023906.D
Acq: 25 Aug 2016 22:58

Instrument :
BNA_G
ClientSampleId :
MW-04

Tgt Ion:	264	Resp:	793561
Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.4	27.6
265	22.8	18.9	28.3

