
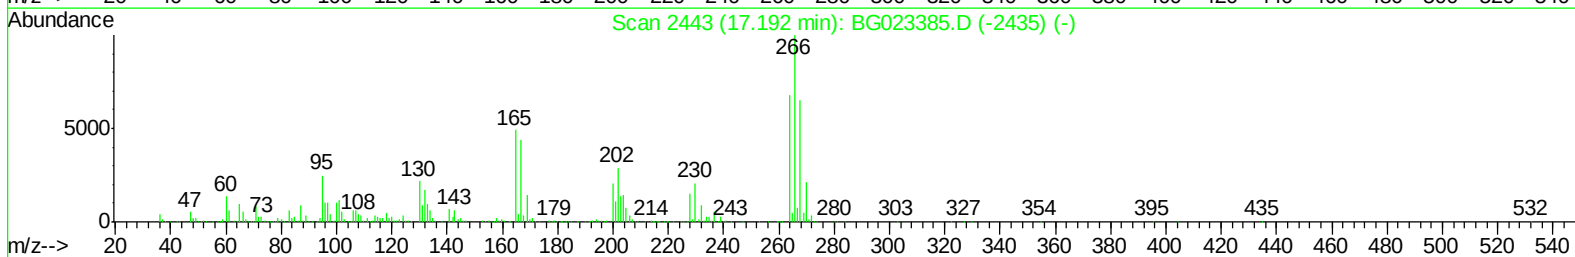
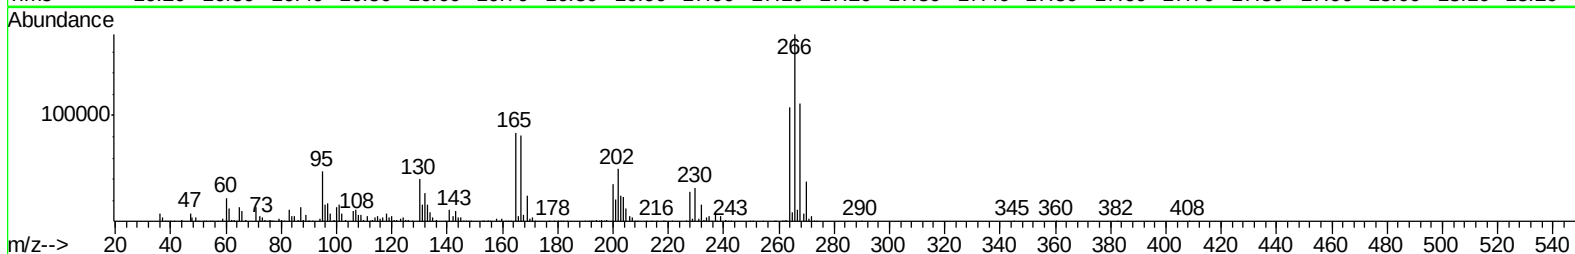


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023892.D
Acq On : 25 Aug 2016 8:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:43:32 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

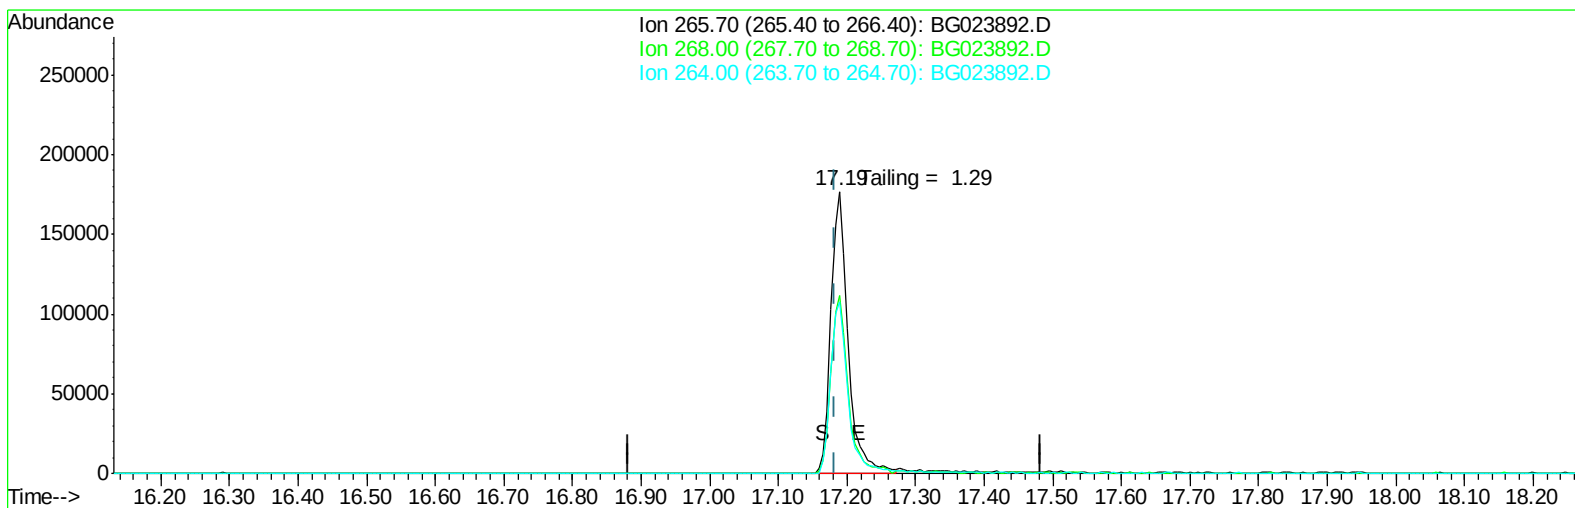

TIC: BG023892.D

(69) Pentachlorophenol (C)




17.189min (+0.006) 42581.03ng

response 302616

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	63.08
264.00	63.20	60.95
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023892.D
Acq On : 25 Aug 2016 8:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:43:32 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

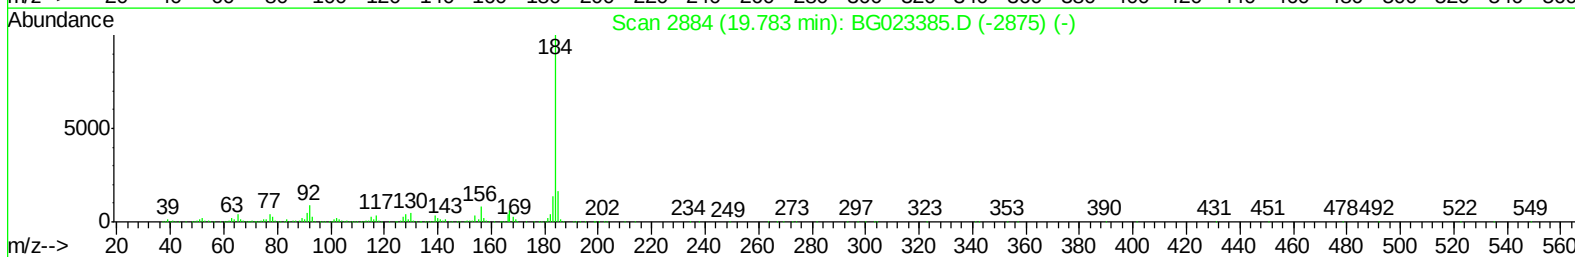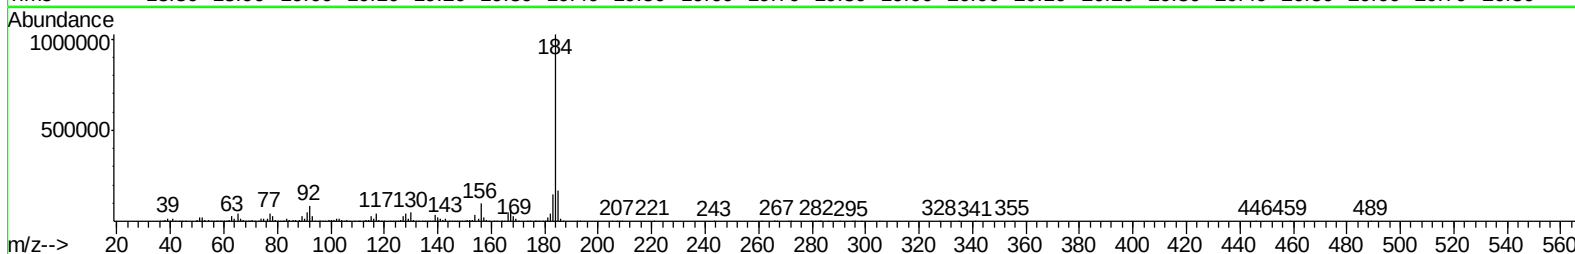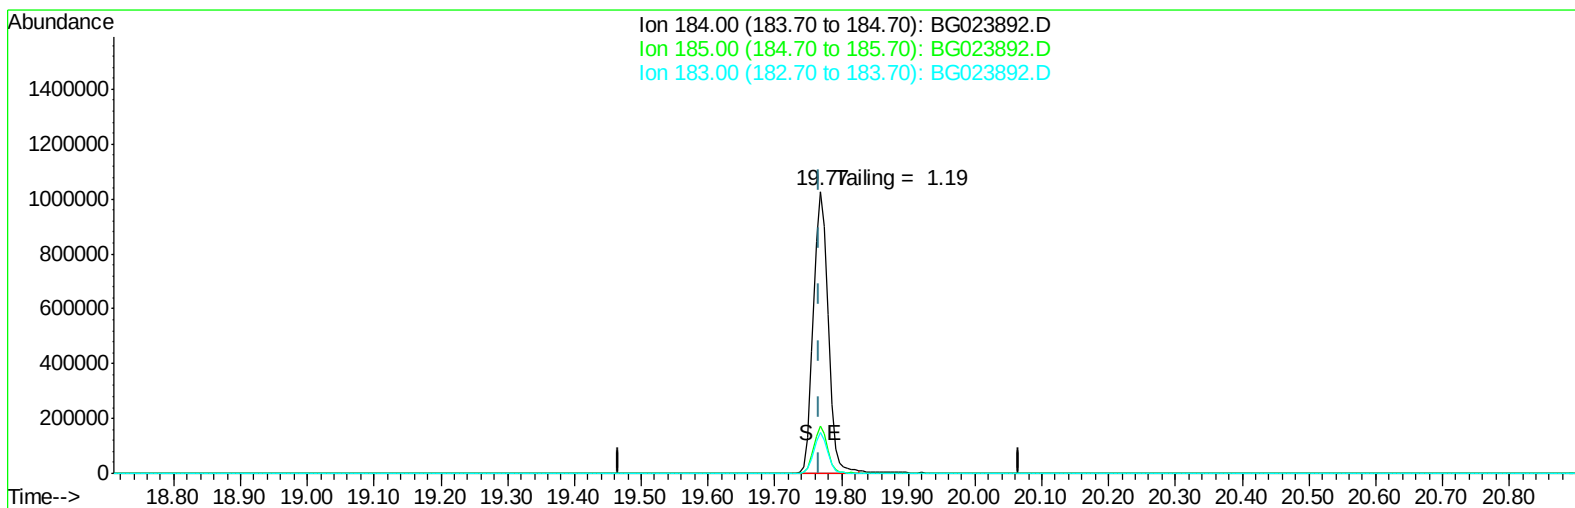

TIC: BG023892.D

(76) Benzidine

19.768min (+0.000) 22408.89ng

response 1571043

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.70
183.00	13.40	14.47
0.00	0.00	0.00