
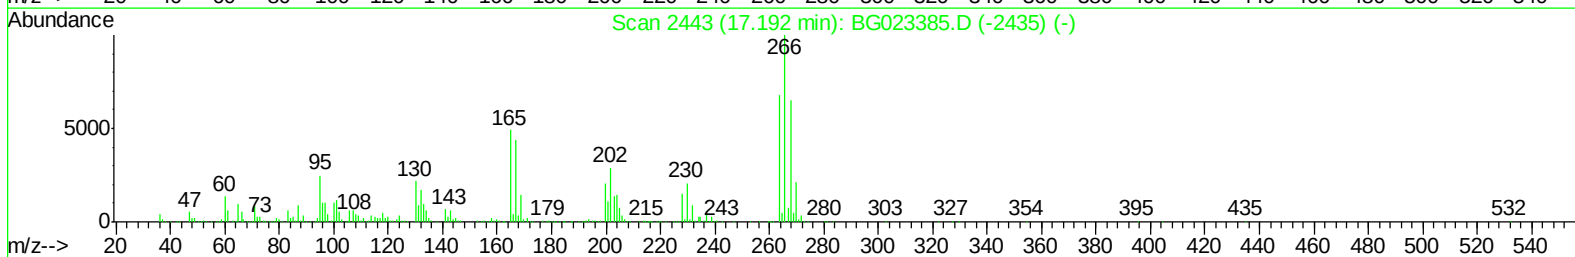
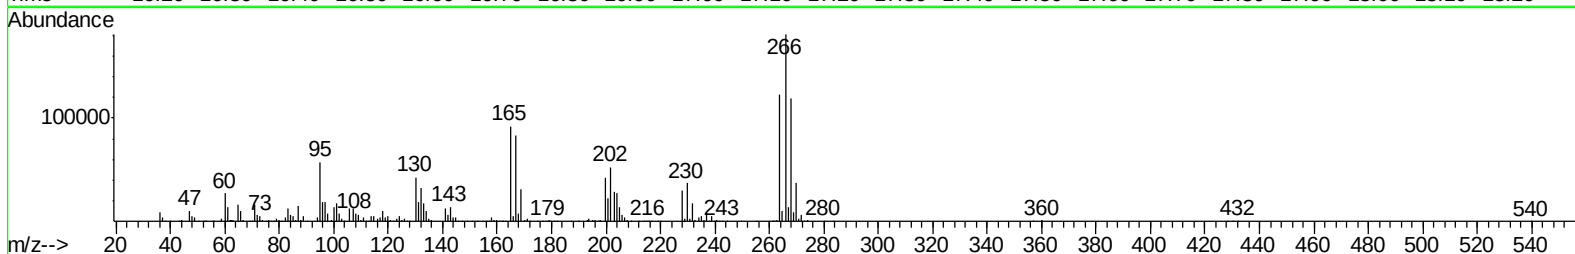


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023895.D
Acq On : 25 Aug 2016 15:04
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:44:06 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

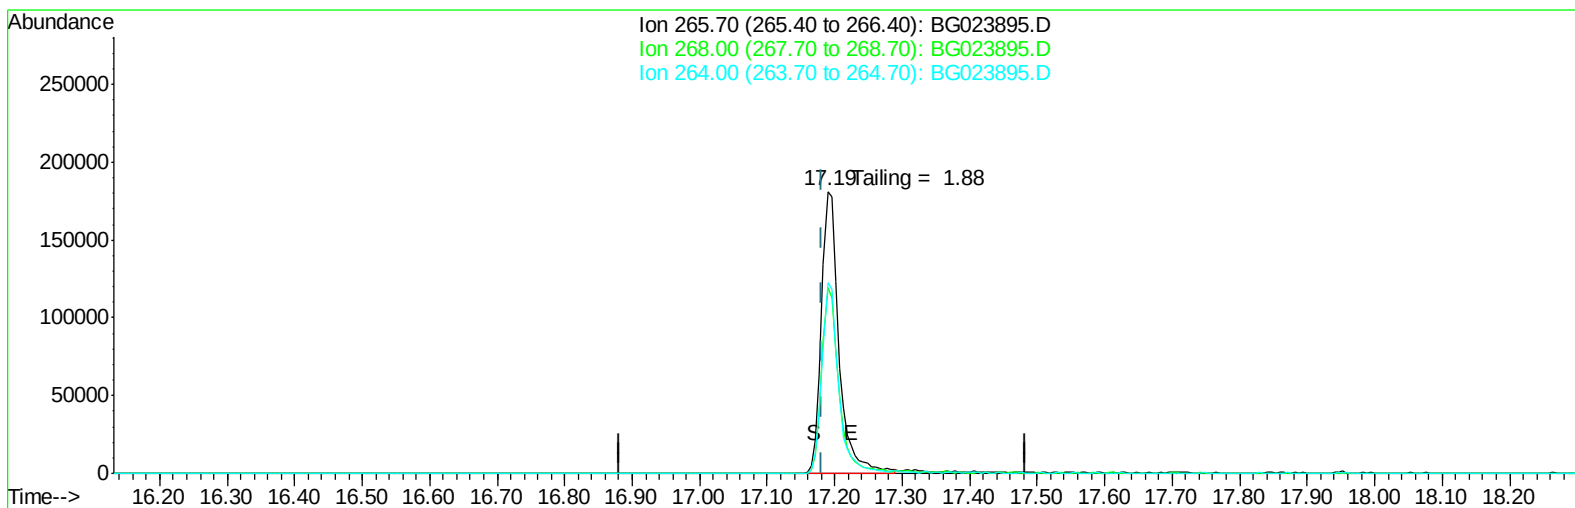

TIC: BG023895.D

(69) Pentachlorophenol (C)




17.189min (+0.007) 62934.27ng

response 323751

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.76
264.00	63.20	67.80
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023895.D
Acq On : 25 Aug 2016 15:04
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:44:06 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

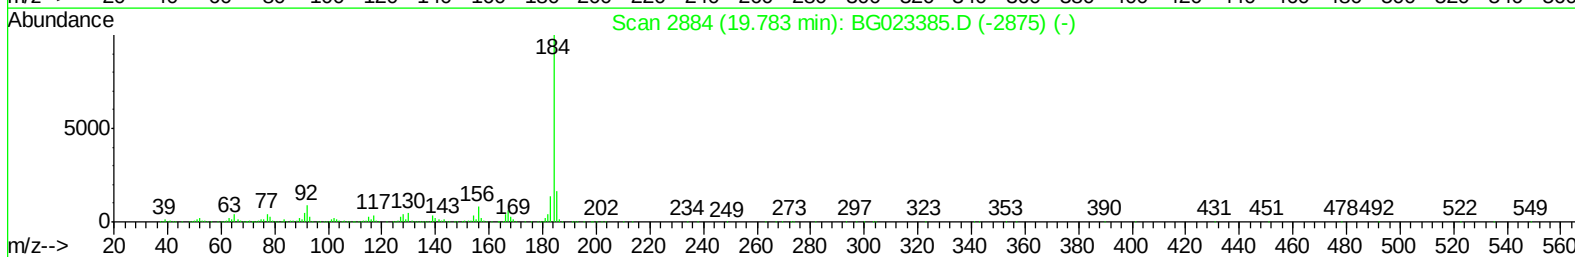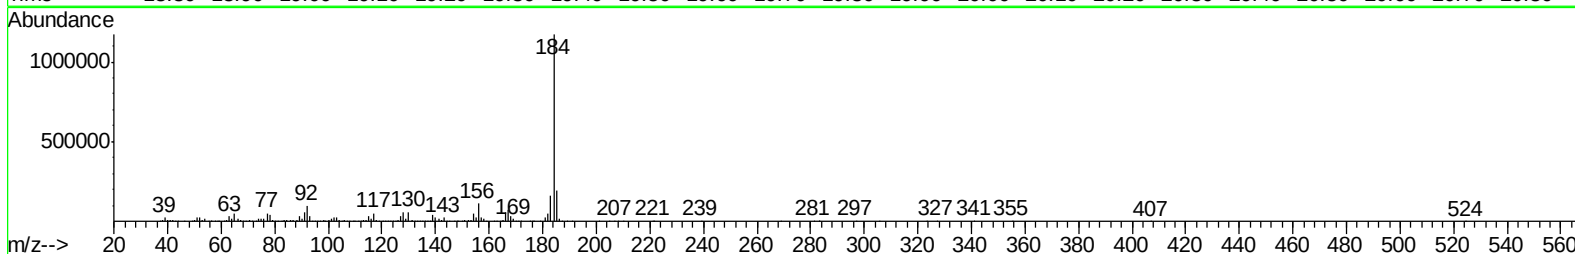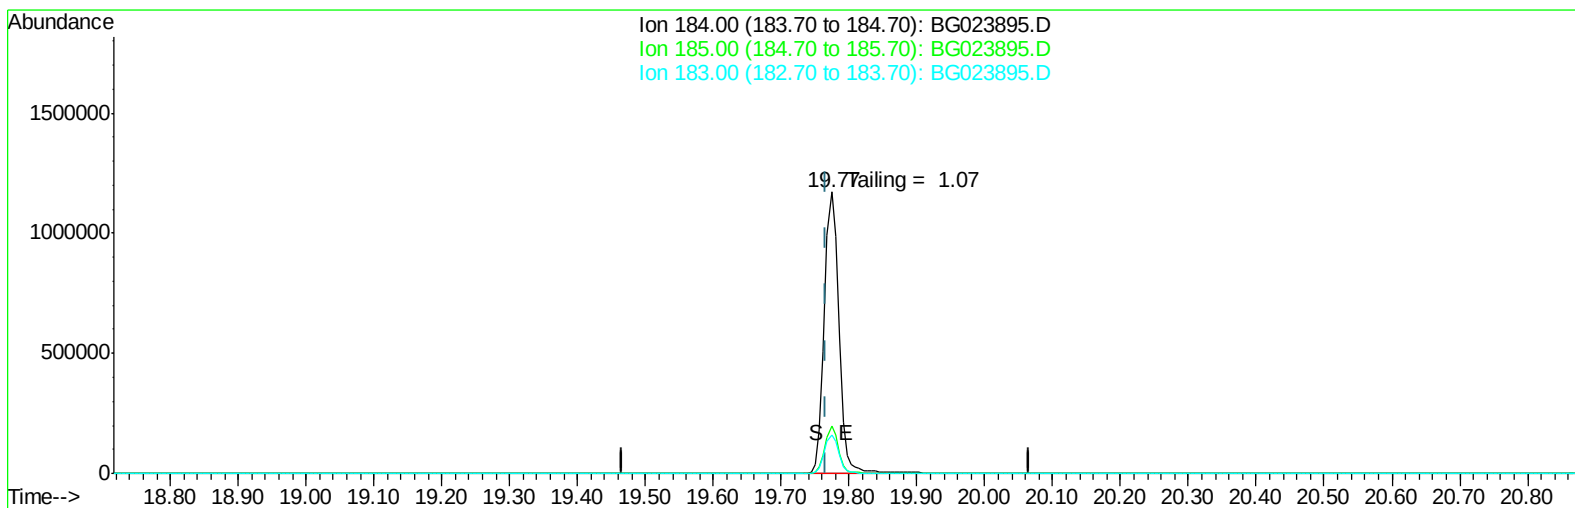

TIC: BG023895.D

(76) Benzidine

19.774min (+0.007) 40659.22ng

response 1719139

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.68
183.00	13.40	13.82
0.00	0.00	0.00