
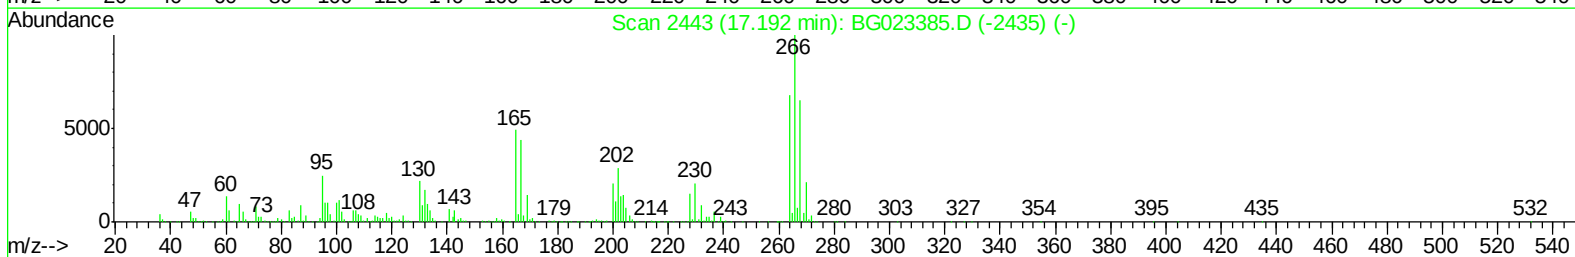
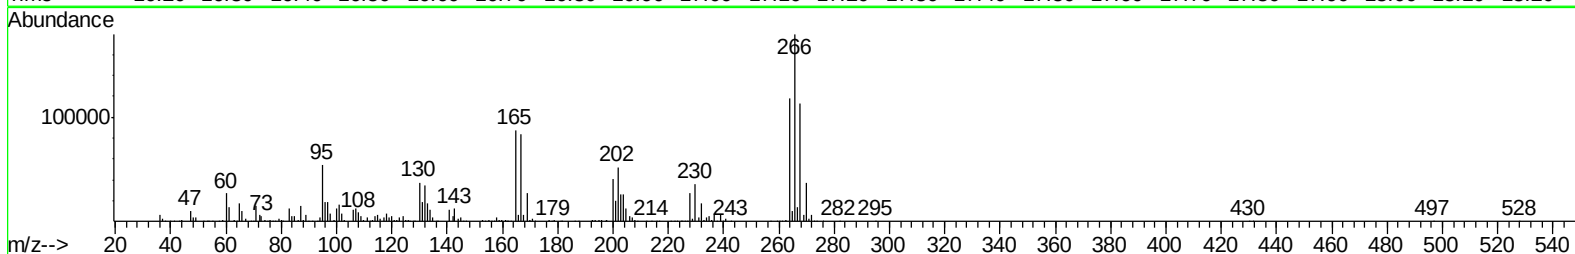


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023910.D
Acq On : 26 Aug 2016 1:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:44:52 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

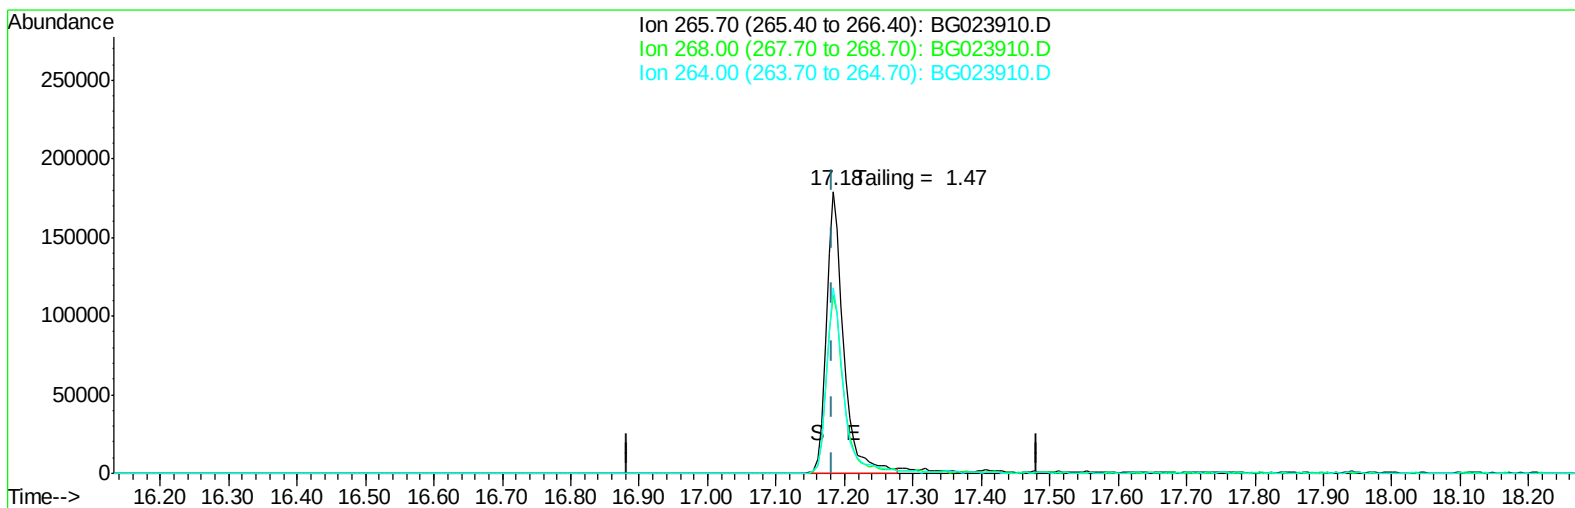

TIC: BG023910.D

(69) Pentachlorophenol (C)




17.184min (+0.001) 494548.76ng

response 312497

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	63.04
264.00	63.20	65.74
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023910.D
Acq On : 26 Aug 2016 1:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 07:44:52 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

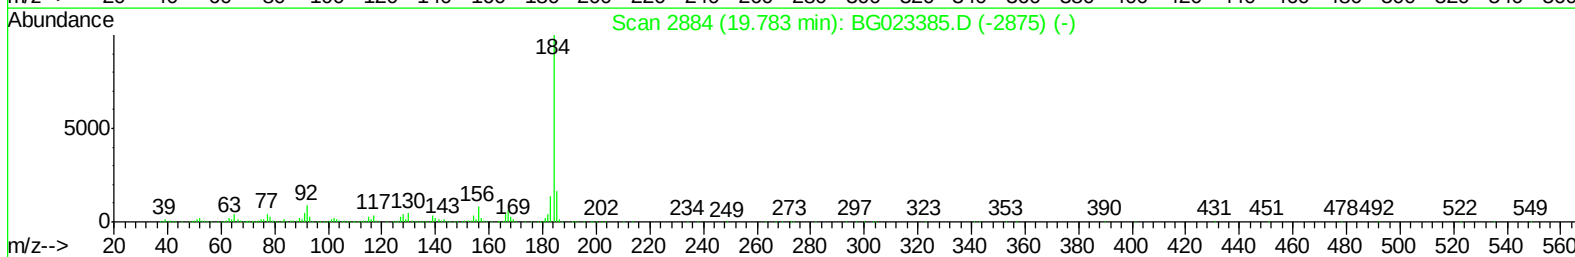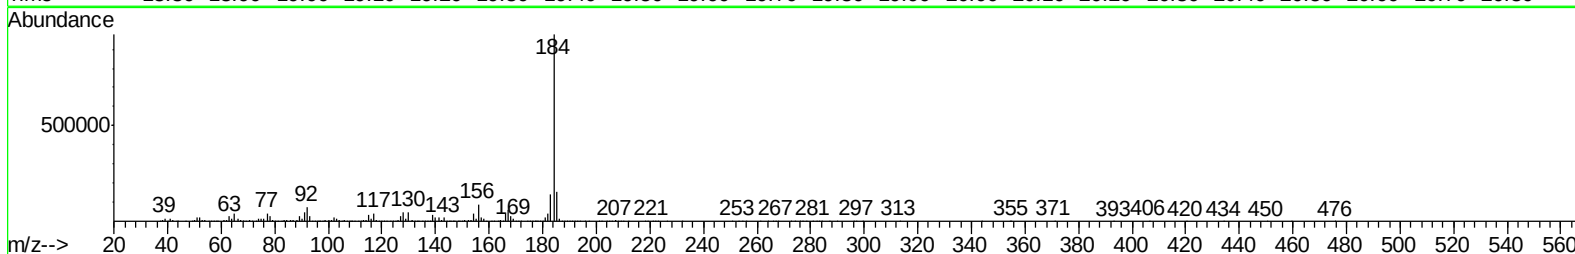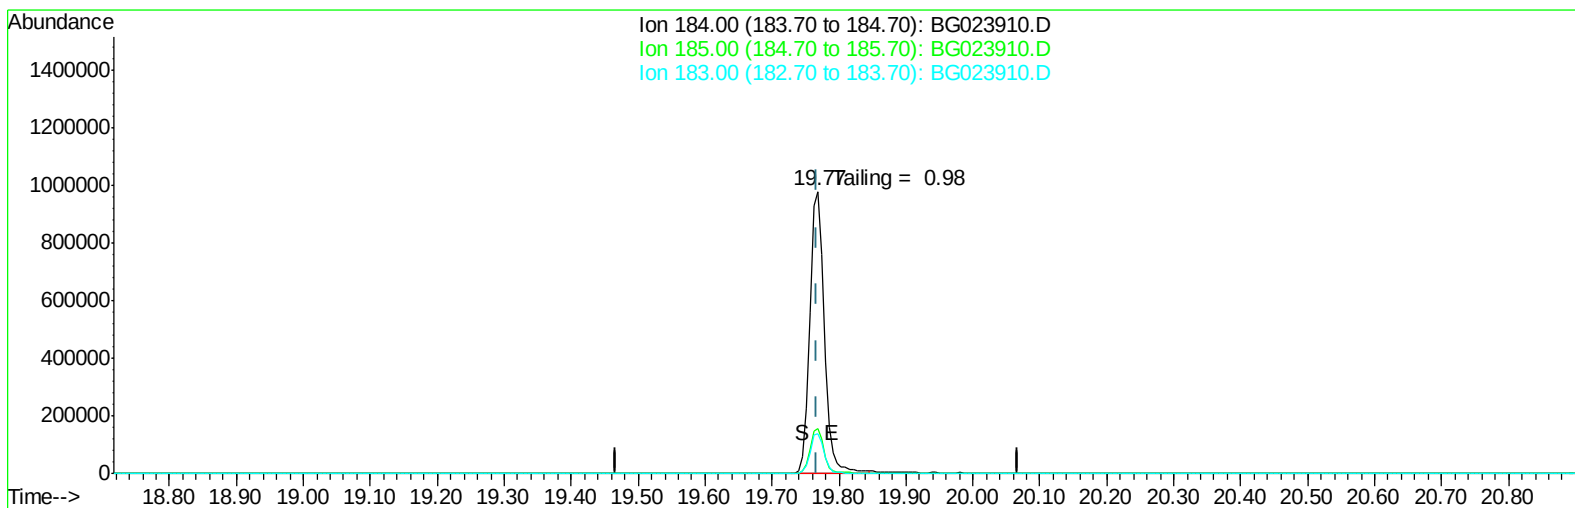

TIC: BG023910.D

(76) Benzidine

19.768min (+0.001) 730084.17ng

response 1522148

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.06
183.00	13.40	14.32
0.00	0.00	0.00