

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
 Data File : BG023904.D
 Acq On : 25 Aug 2016 21:43
 Operator : UM/SJ
 Sample : H4592-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-2

Quant Time: Aug 26 01:40:54 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 24 17:42:04 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	121207	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	505199	20.00	ng	0.00
38) Acenaphthene-d10	14.76	164	327315	20.00	ng	0.00
63) Phenanthrene-d10	17.52	188	785452	20.00	ng	0.00
75) Chrysene-d12	21.84	240	860677	20.00	ng	0.00
86) Perylene-d12	25.22	264	785983	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	568220	78.91	ng	0.00
7) Phenol-d6	7.25	99	621997	55.46	ng	0.00
23) Nitrobenzene-d5	9.27	82	834632	82.13	ng	0.00
41) 2,4,6-Tribromophenol	16.26	330	493841	103.15	ng	0.00
44) 2-Fluorobiphenyl	13.38	172	1616107	83.28	ng	0.00
78) Terphenyl-d14	20.13	244	2388260	87.37	ng	0.00
Target Compounds						
49) Dimethylphthalate	14.21	163	148183	5.90	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023904.D
Acq On : 25 Aug 2016 21:43
Operator : UM/SJ
Sample : H4592-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-2

Quant Time: Aug 26 01:40:54 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

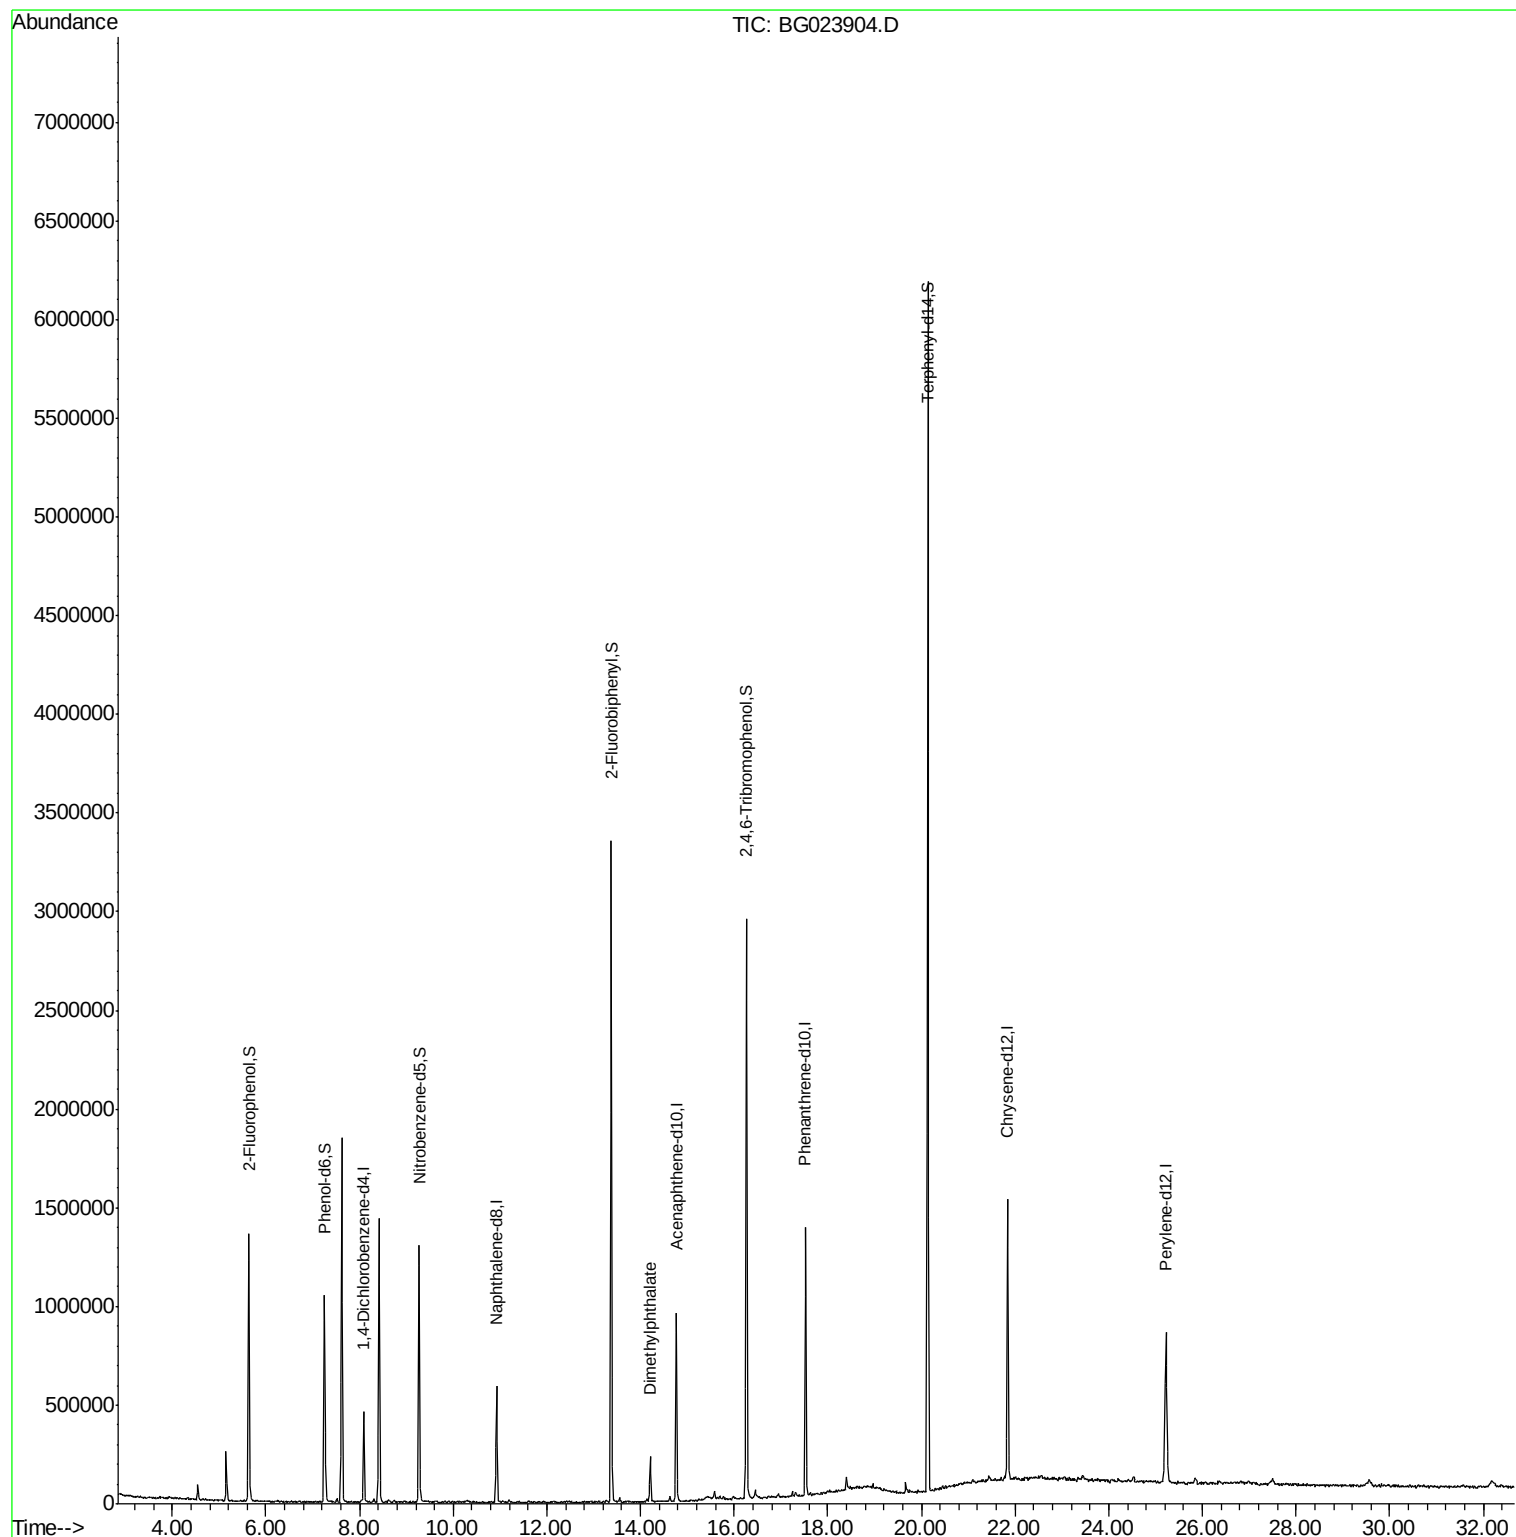




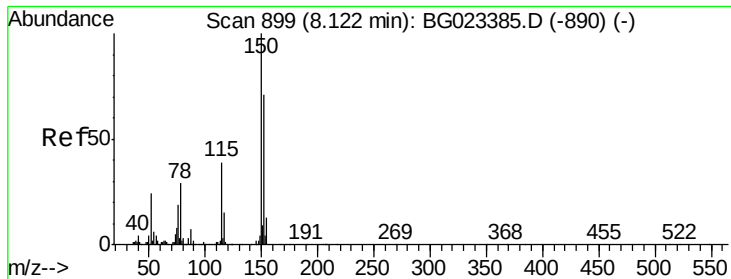


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.09 min Scan# 894
Delta R.T. -0.00 min
Lab File: BG023904.D
Acq: 25 Aug 2016 21:43

Instrument :
BNA_G
ClientSampleId :
MW-2




Tgt Ion	Ratio	Lower	Upper
152	100		
150	148.4	144.7	217.1
115	62.9	64.0	96.0

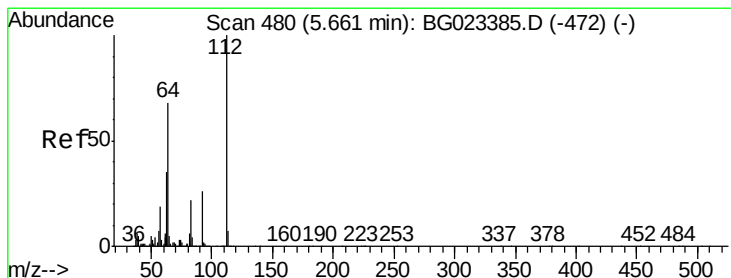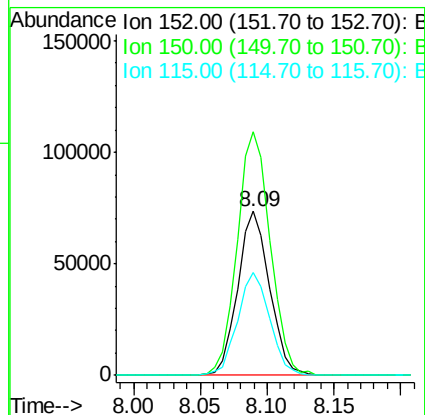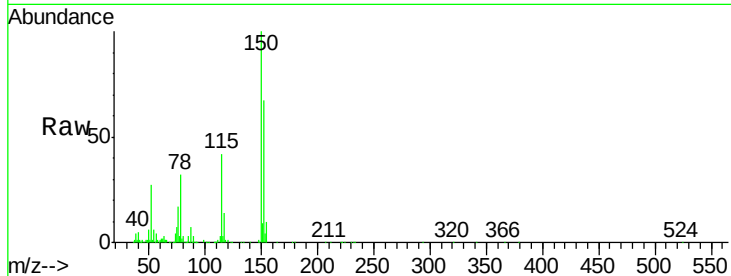


#5

2-Fluorophenol
Concen: 78.91 ng
RT: 5.63 min Scan# 476
Delta R.T. -0.00 min
Lab File: BG023904.D
Acq: 25 Aug 2016 21:43

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.0	59.0	88.4
63	38.9	37.8	56.8

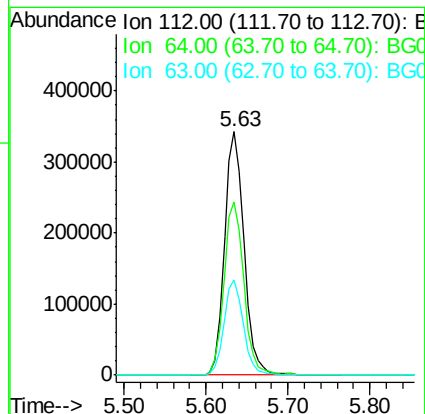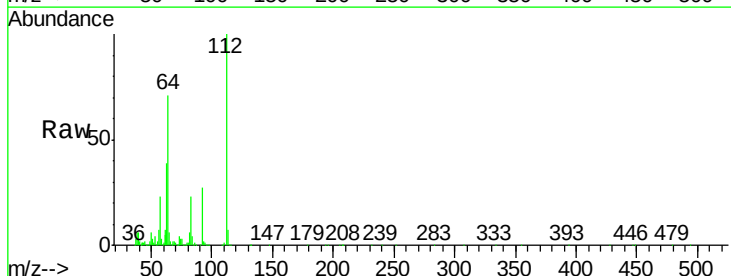

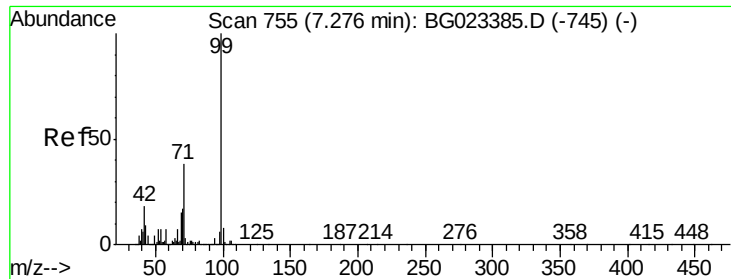

#7

Phenol-d6

Concen: 55.46 ng

RT: 7.25 min Scan# 751

Delta R.T. -0.00 min

Lab File: BG023904.D

Acq: 25 Aug 2016 21:43

Instrument :

BNA_G

ClientSampleId :

MW-2


Tgt Ion: 99 Resp: 621997

Ion Ratio Lower Upper




99 100

42 19.0 17.8 26.6

71 41.2 41.5 62.3#

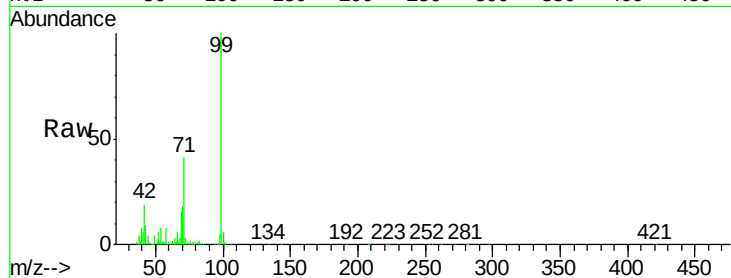

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

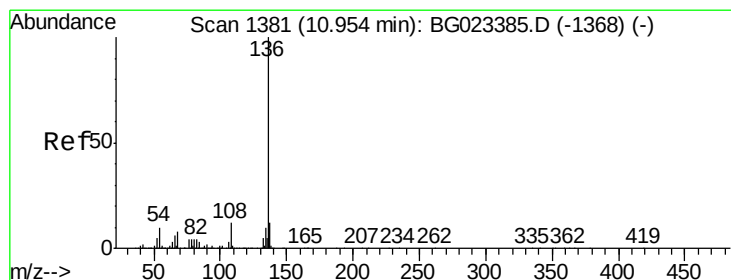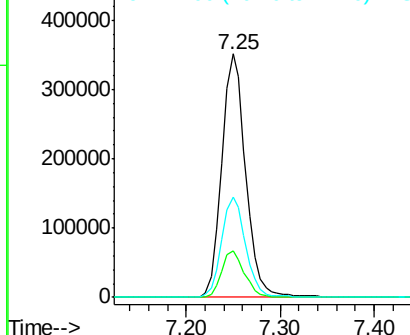

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1377

Delta R.T. -0.00 min

Lab File: BG023904.D

Acq: 25 Aug 2016 21:43

Tgt Ion: 136 Resp: 505199


Ion Ratio Lower Upper

136 100



137 11.0 9.6 14.4


54 8.6 7.3 10.9

68 7.0 5.3 7.9

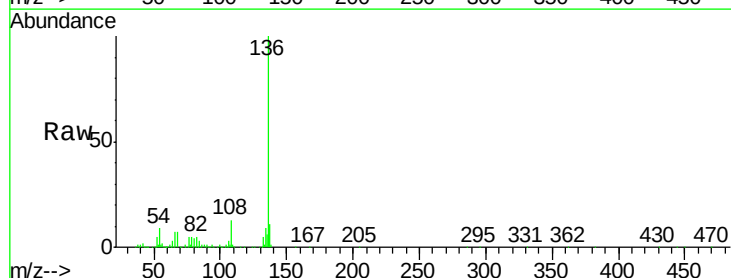

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




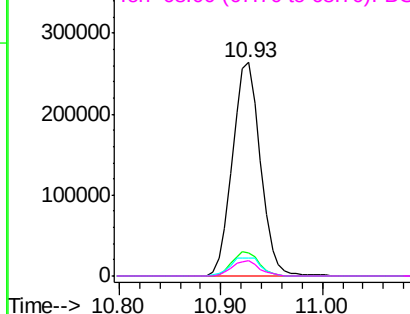




#23
Nitrobenzene-d5
Concen: 82.13 ng
RT: 9.27 min Scan# 1095
Delta R.T. -0.00 min
Lab File: BG023904.D
Acq: 25 Aug 2016 21:43




Instrument :
BNA_G
ClientSampleId :
MW-2


Tgt Ion	Ratio	Lower	Upper
82	100		
128	36.2	24.4	36.6
54	50.4	41.4	62.0

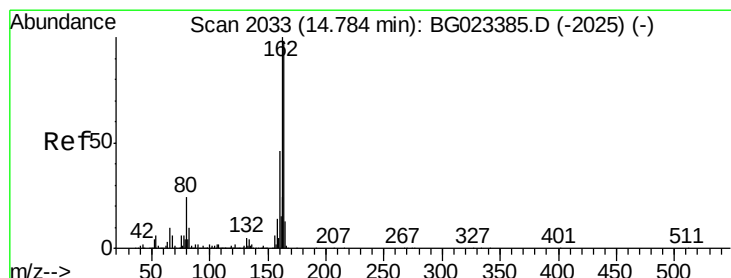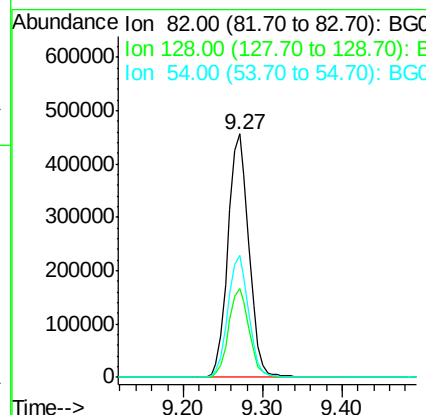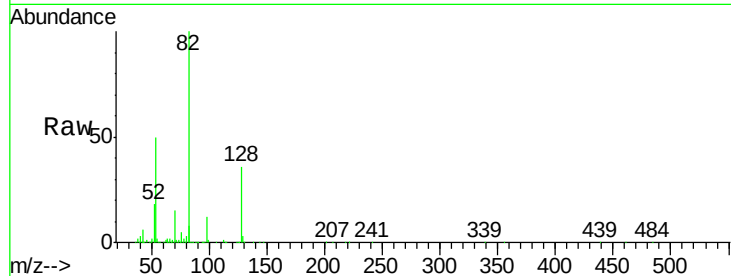

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.76 min Scan# 2030
Delta R.T. -0.00 min
Lab File: BG023904.D
Acq: 25 Aug 2016 21:43

Tgt Ion	Ratio	Lower	Upper
164	100		
162	108.3	87.7	131.5
160	44.8	37.2	55.8



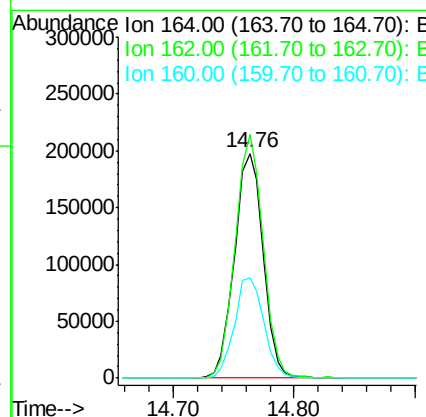
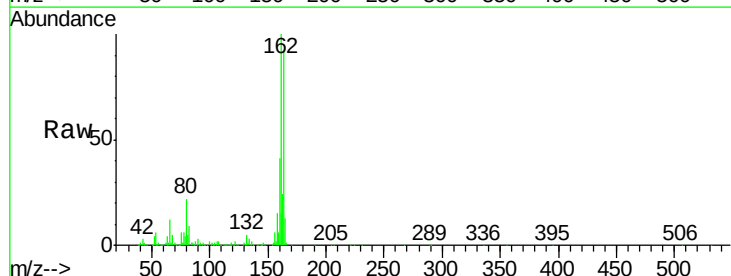




#41
 2,4,6-Tribromophenol
 Concen: 103.15 ng
 RT: 16.26 min Scan# 2285
 Delta R.T. -0.00 min
 Lab File: BG023904.D
 Acq: 25 Aug 2016 21:43




Instrument :
 BNA_G
 ClientSampleId :
 MW-2


Tgt Ion:330 Resp: 493841
 Ion Ratio Lower Upper
 330 100
 332 97.7 77.4 116.2
 141 42.4 31.7 47.5

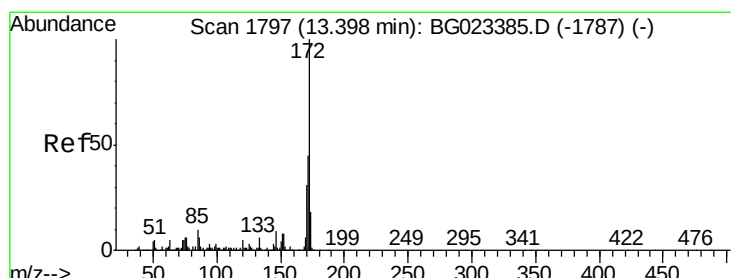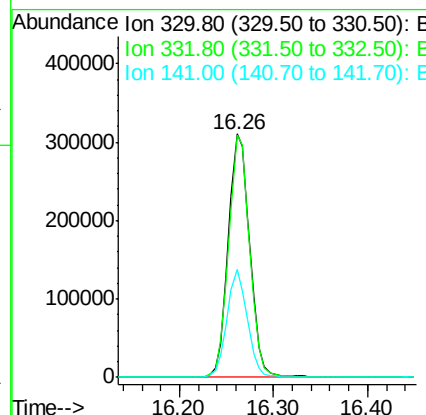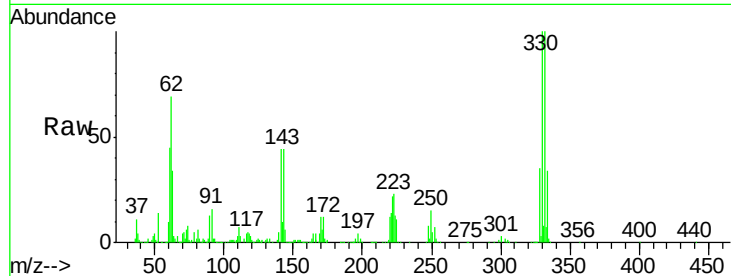

#44
 2-Fluorobiphenyl
 Concen: 83.28 ng
 RT: 13.38 min Scan# 1794
 Delta R.T. -0.00 min
 Lab File: BG023904.D
 Acq: 25 Aug 2016 21:43

Tgt Ion:172 Resp: 1616107
 Ion Ratio Lower Upper
 172 100
 171 40.5 31.6 47.4
 170 26.4 21.3 31.9

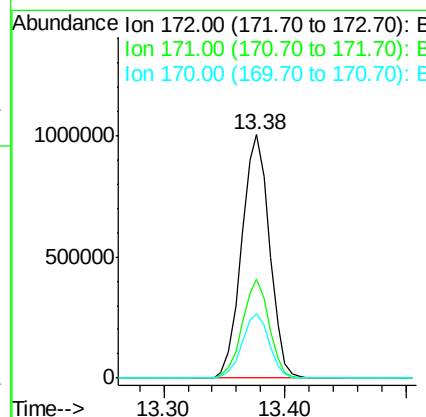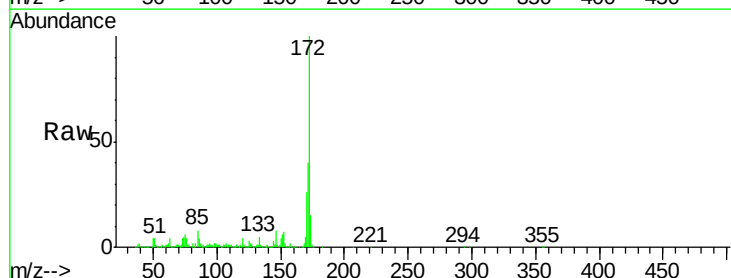



#49

Dimethylphthalate

Concen: 5.90 ng

RT: 14.21 min Scan# 1936

Delta R.T. -0.00 min

Lab File: BG023904.D

Acq: 25 Aug 2016 21:43

Instrument :

BNA_G

ClientSampleId :

MW-2


Tgt Ion:163 Resp: 148183

Ion Ratio Lower Upper

163 100

194 4.4 3.6 5.4




164 10.5 8.1 12.1

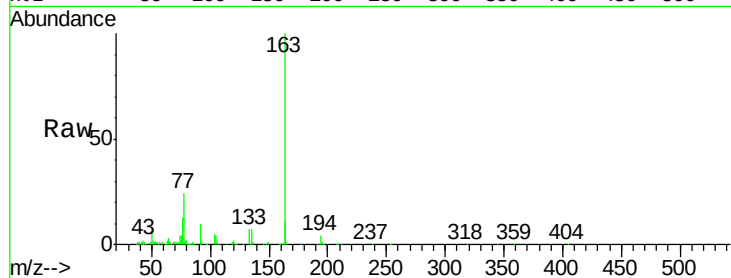

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

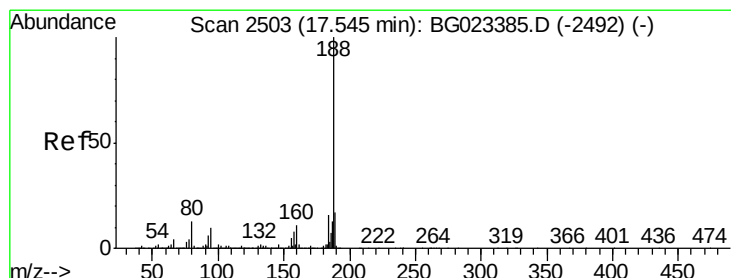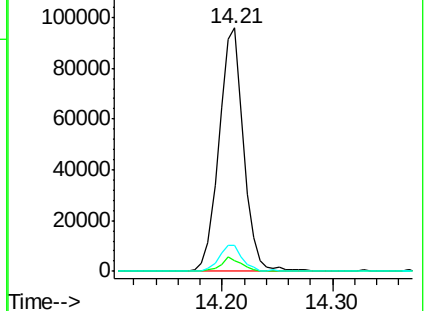

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.52 min Scan# 2500

Delta R.T. -0.00 min

Lab File: BG023904.D

Acq: 25 Aug 2016 21:43


Tgt Ion:188 Resp: 785452

Ion Ratio Lower Upper

188 100

94 8.8 5.2 7.8#



80 11.4 7.2 10.8#

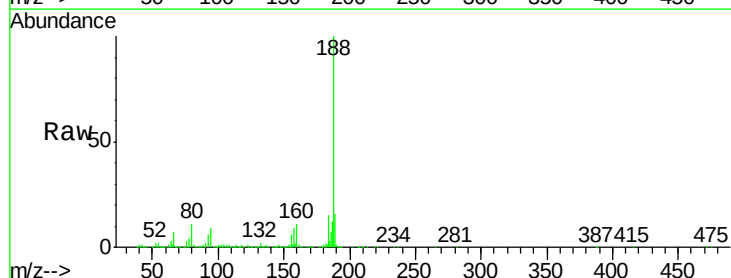


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

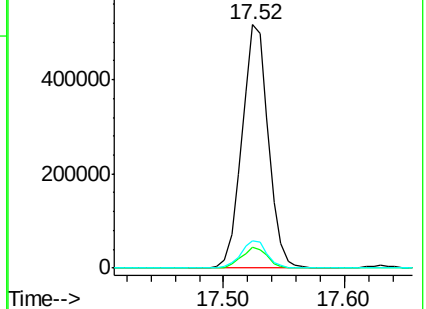

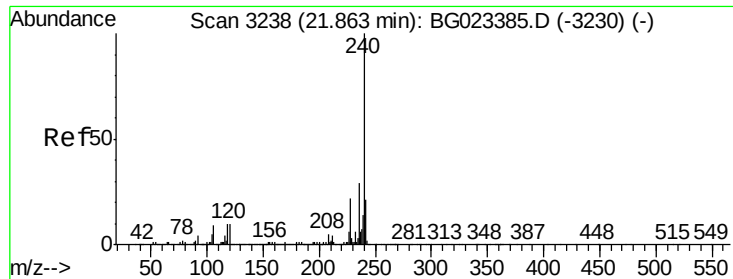

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.84 min Scan# 3235

Delta R.T. -0.00 min

Lab File: BG023904.D

Acq: 25 Aug 2016 21:43

Instrument :

BNA_G

ClientSampleId :

MW-2


Tgt Ion:240 Resp: 860677

Ion Ratio Lower Upper

240 100

120 8.4 4.1 6.1#




236 25.1 21.1 31.7

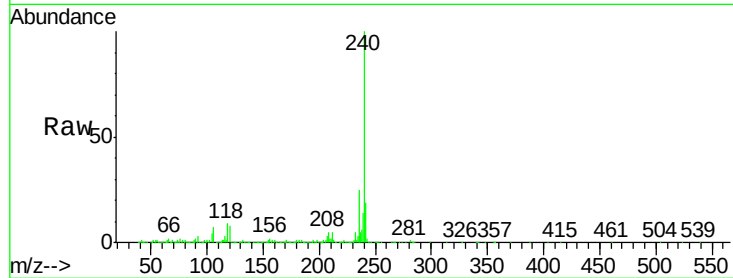

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

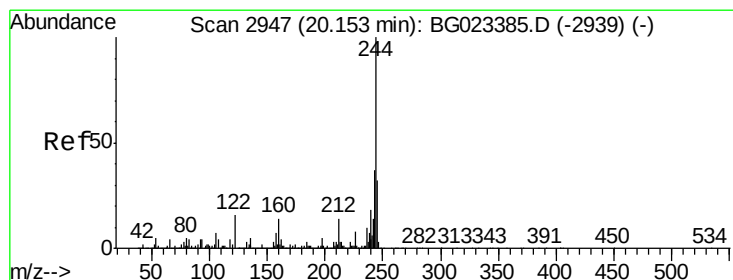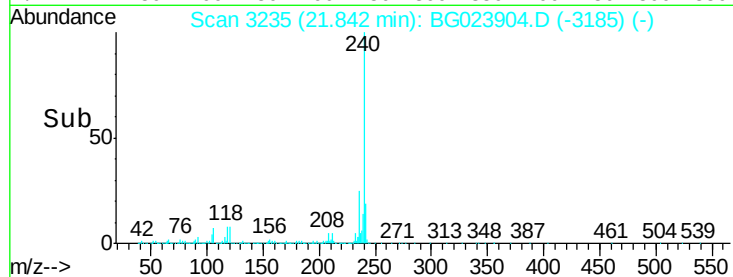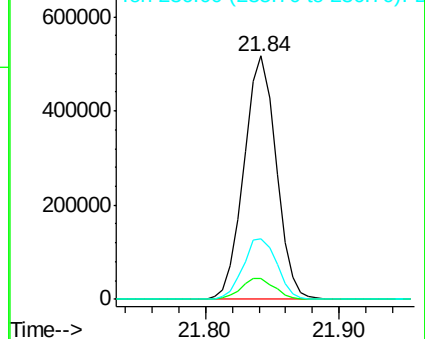

#78

Terphenyl-d14

Concen: 87.37 ng

RT: 20.13 min Scan# 2944

Delta R.T. -0.00 min

Lab File: BG023904.D

Acq: 25 Aug 2016 21:43


Tgt Ion:244 Resp: 2388260

Ion Ratio Lower Upper

244 100

212 11.8 10.8 16.2



122 12.1 8.0 12.0#

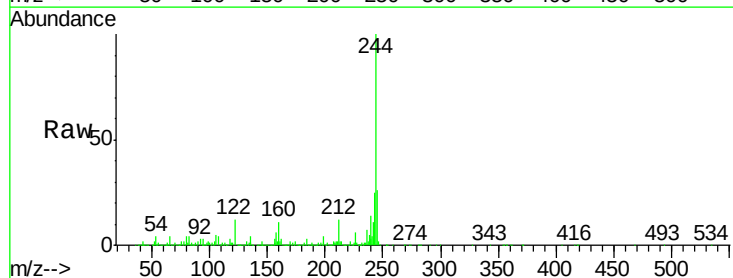


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

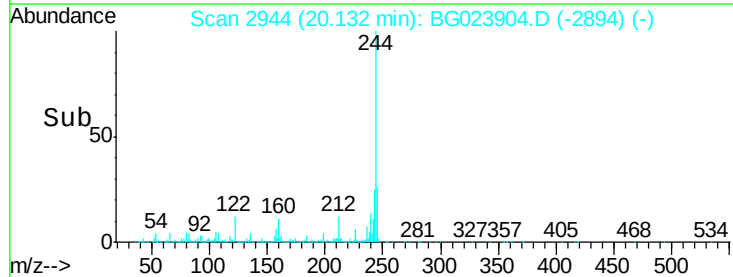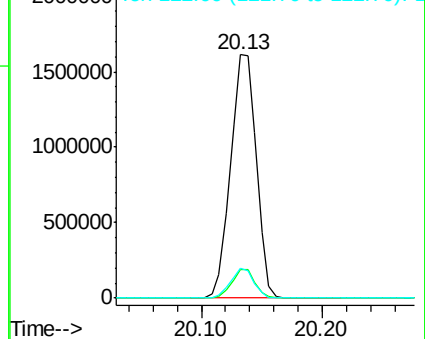

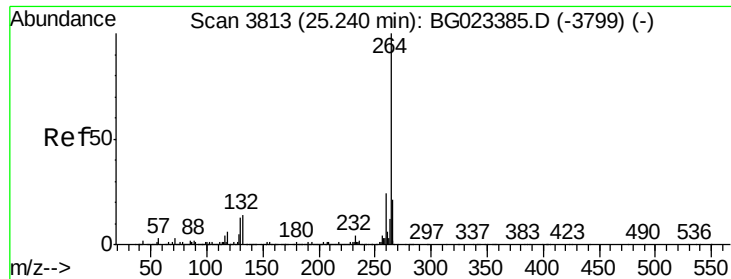

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.22 min Scan# 3810
Delta R.T. -0.00 min
Lab File: BG023904.D
Acq: 25 Aug 2016 21:43

Instrument :
BNA_G
ClientSampleId :
MW-2

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.4	18.4	27.6
265	21.5	18.9	28.3

