

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
 Data File : BG023916.D
 Acq On : 26 Aug 2016 6:59
 Operator : UM/SJ
 Sample : H4588-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FIELDBLANK

Quant Time: Aug 26 07:37:03 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 24 17:42:04 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	121811	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	534352	20.00	ng	0.00
38) Acenaphthene-d10	14.77	164	342145	20.00	ng	0.00
63) Phenanthrene-d10	17.53	188	814782	20.00	ng	0.00
75) Chrysene-d12	21.85	240	825719	20.00	ng	0.00
86) Perylene-d12	25.24	264	807727	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	380340	52.56	ng	0.00
7) Phenol-d6	7.26	99	356757	31.65	ng	0.00
23) Nitrobenzene-d5	9.28	82	848458	78.94	ng	0.00
41) 2,4,6-Tribromophenol	16.27	330	483997	96.71	ng	0.00
44) 2-Fluorobiphenyl	13.38	172	1635234	80.61	ng	0.00
78) Terphenyl-d14	20.14	244	2221418	83.95	ng	0.00
Target Compounds						
76) Benzidine	19.77	184	191939	8.36	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023916.D
Acq On : 26 Aug 2016 6:59
Operator : UM/SJ
Sample : H4588-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FIELDBLANK

Quant Time: Aug 26 07:37:03 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 24 17:42:04 2016
Response via : Initial Calibration

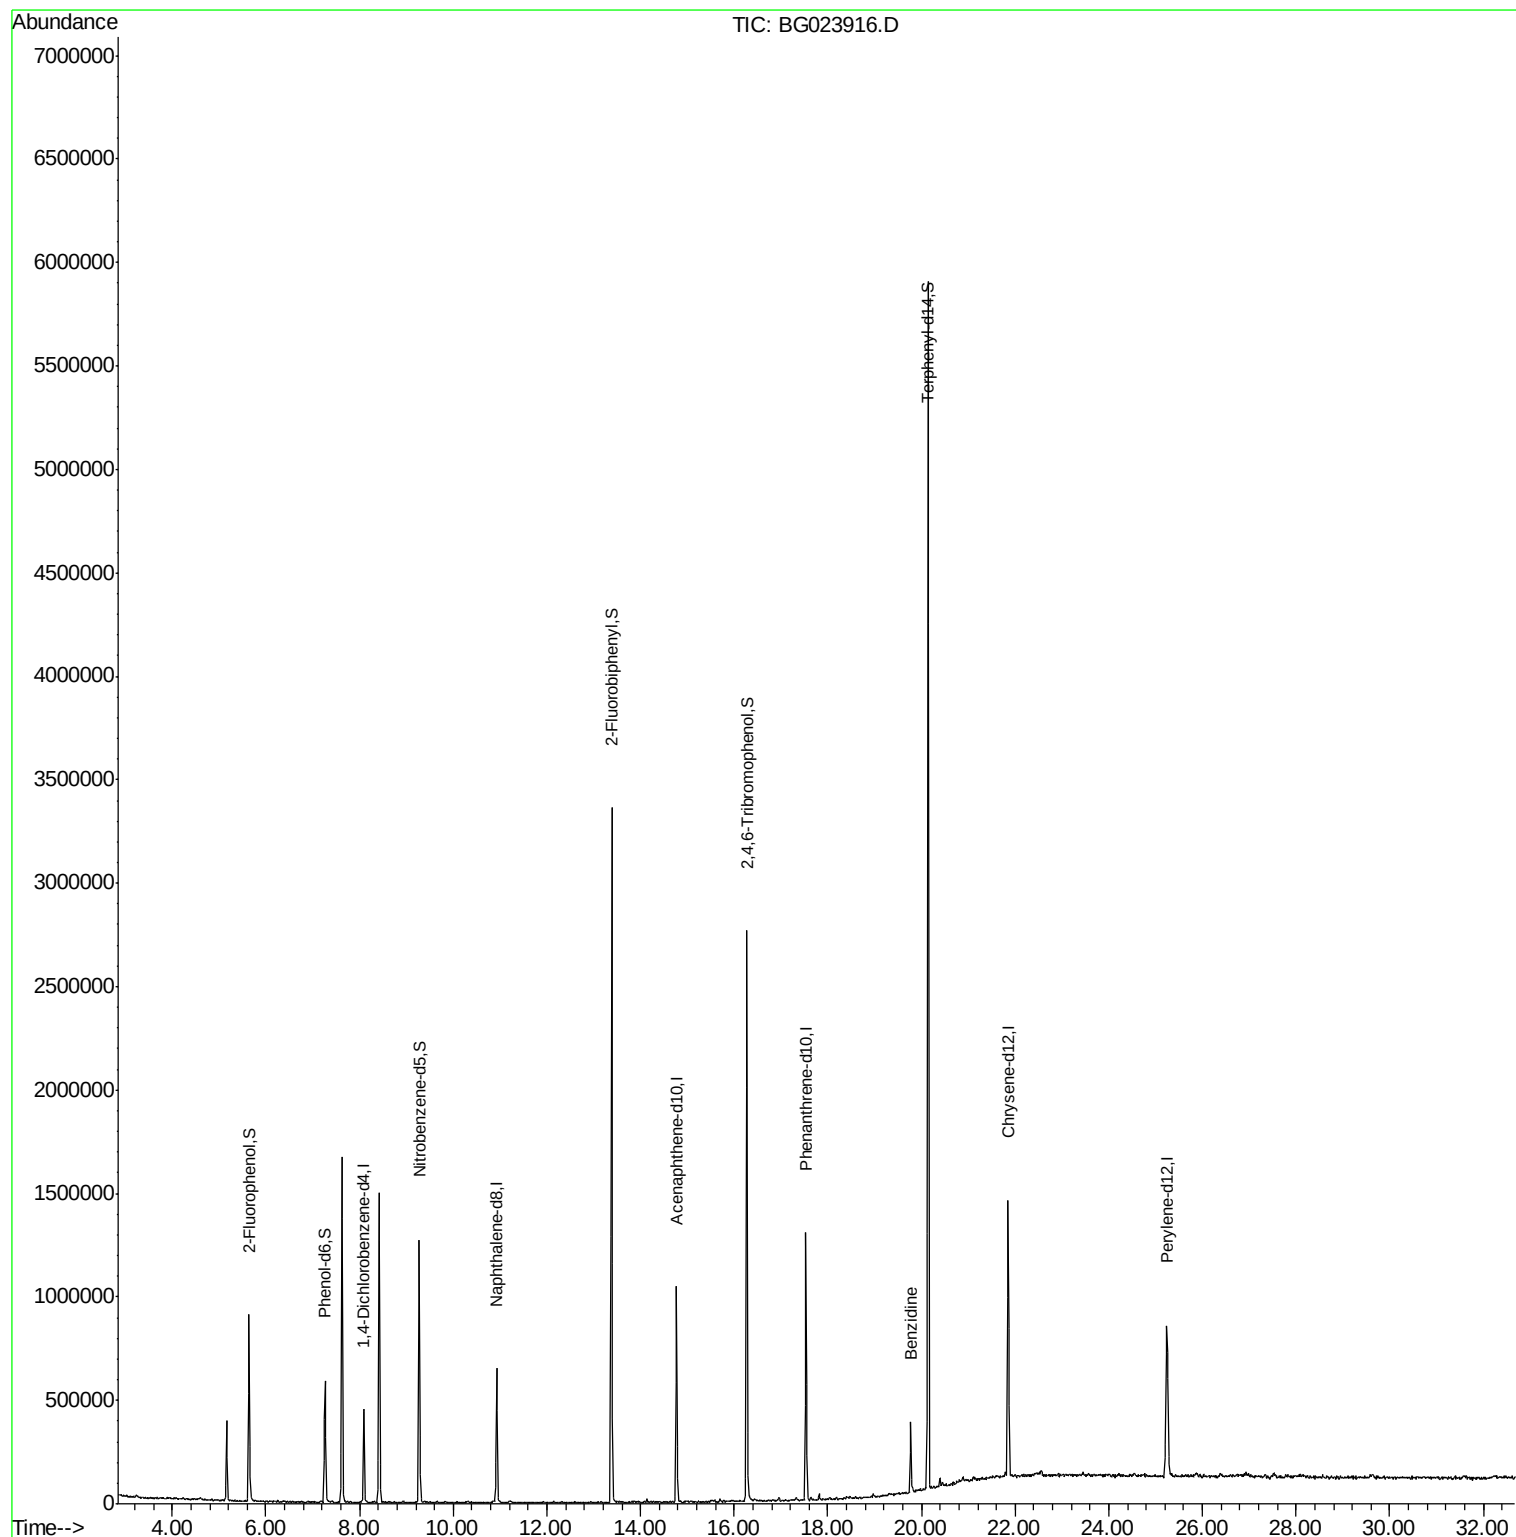




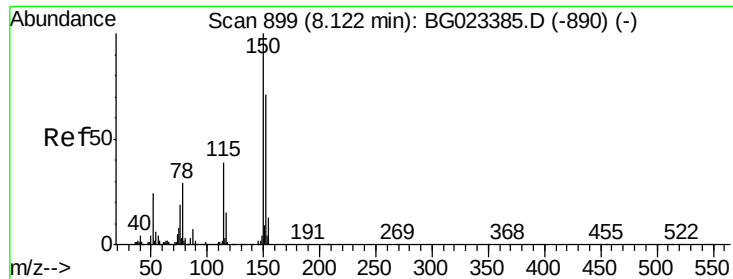


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.09 min Scan# 894
Delta R.T. -0.01 min
Lab File: BG023916.D
Acq: 26 Aug 2016 6:59

Instrument :
BNA_G
ClientSampleId :
FIELDBLANK




Tgt Ion	Ratio	Lower	Upper
152	100		
150	151.2	144.7	217.1
115	64.0	64.0	96.0

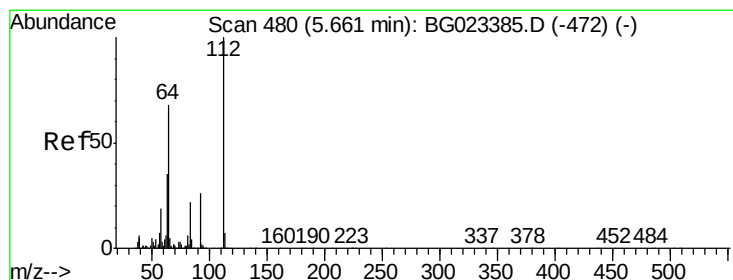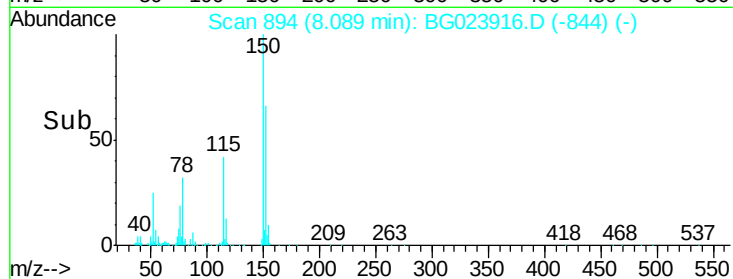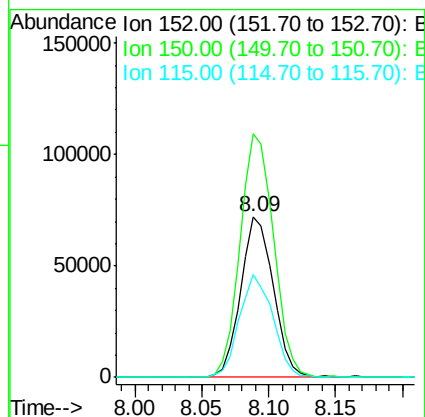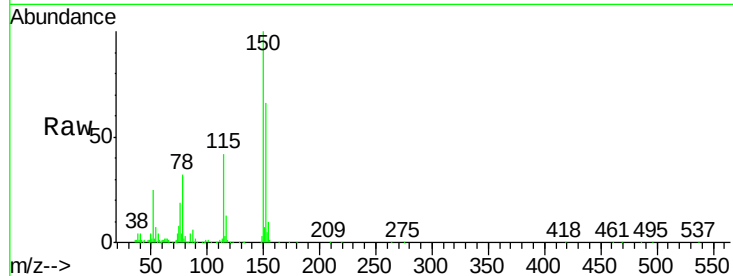


#5

2-Fluorophenol
Concen: 52.56 ng
RT: 5.64 min Scan# 477
Delta R.T. -0.00 min
Lab File: BG023916.D
Acq: 26 Aug 2016 6:59

Tgt Ion	Ratio	Lower	Upper
112	100		
64	74.1	59.0	88.4
63	41.0	37.8	56.8

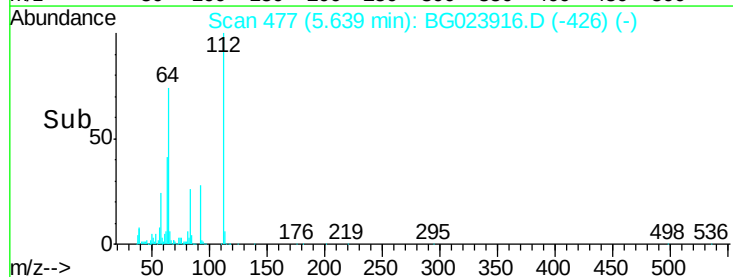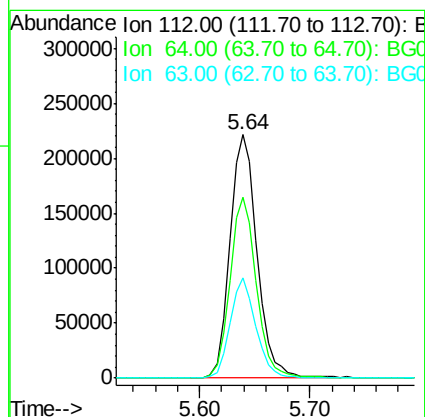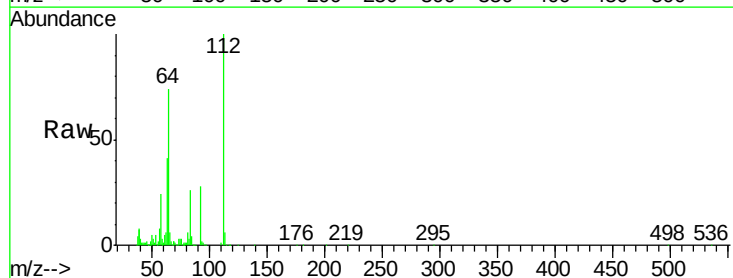

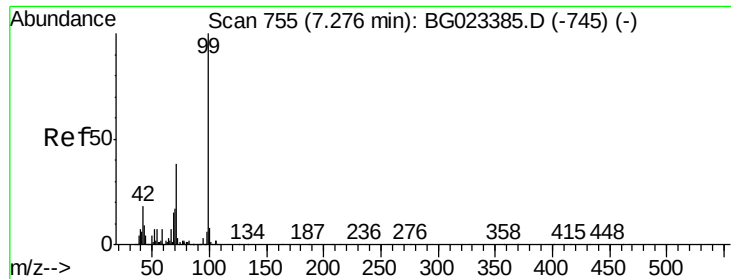

#7

Phenol-d6

Concen: 31.65 ng

RT: 7.26 min Scan# 753

Delta R.T. 0.01 min

Lab File: BG023916.D

Acq: 26 Aug 2016 6:59

Instrument :

BNA_G

ClientSampleId :

FIELDBLANK


Tgt Ion: 99 Resp: 356757

Ion Ratio Lower Upper




99 100

42 18.6 17.8 26.6

71 41.7 41.5 62.3

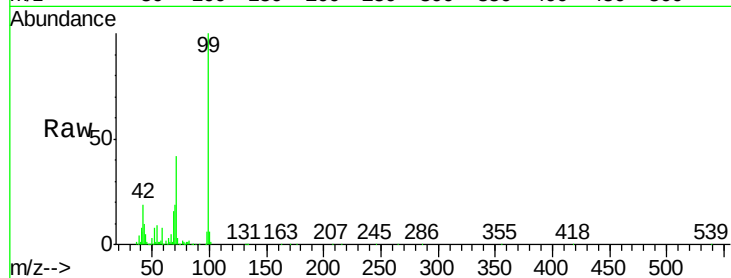

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

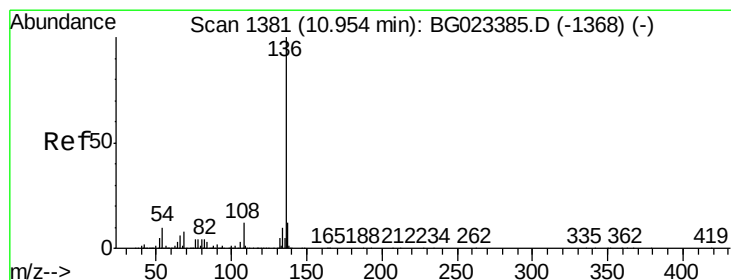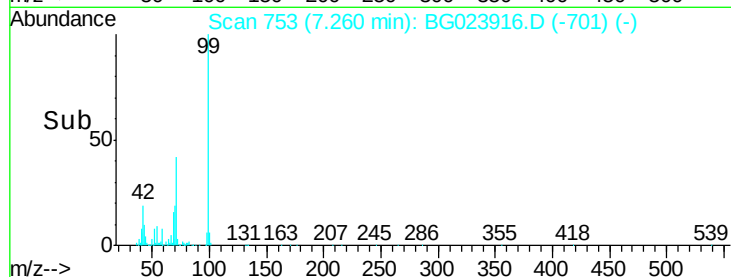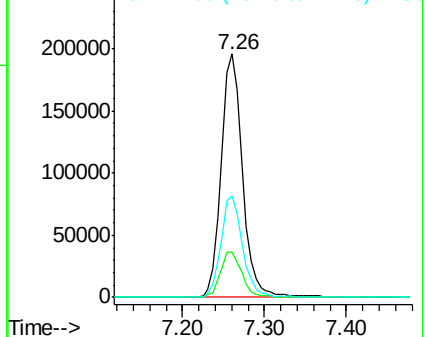

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1377

Delta R.T. -0.01 min

Lab File: BG023916.D

Acq: 26 Aug 2016 6:59

Tgt Ion: 136 Resp: 534352


Ion Ratio Lower Upper

136 100



137 10.8 9.6 14.4


54 9.5 7.3 10.9

68 7.1 5.3 7.9

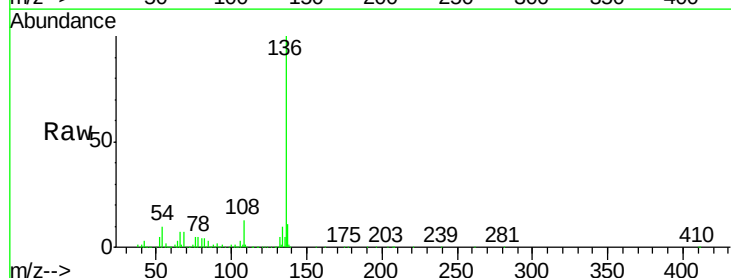

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



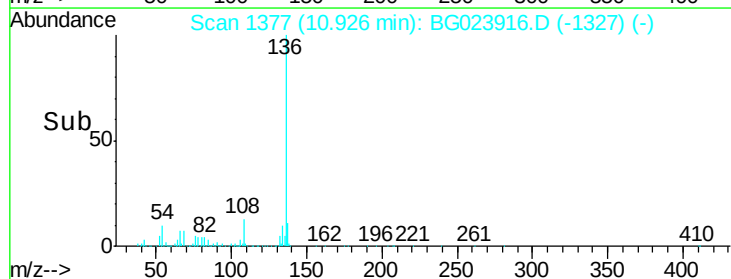
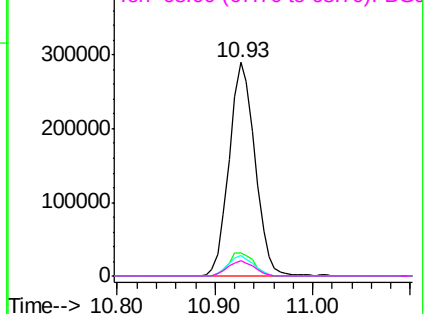


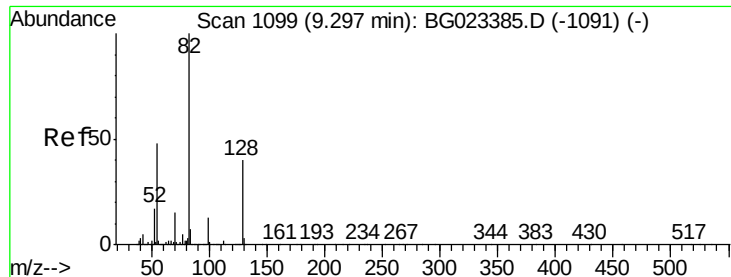

#23
 Nitrobenzene-d5
 Concen: 78.94 ng
 RT: 9.28 min Scan# 1096
 Delta R.T. -0.00 min
 Lab File: BG023916.D
 Acq: 26 Aug 2016 6:59




Instrument :
 BNA_G
 ClientSampleId :
 FIELDBLANK


Tgt Ion	Ratio	Lower	Upper
82	100		
128	36.4	24.4	36.6
54	49.1	41.4	62.0

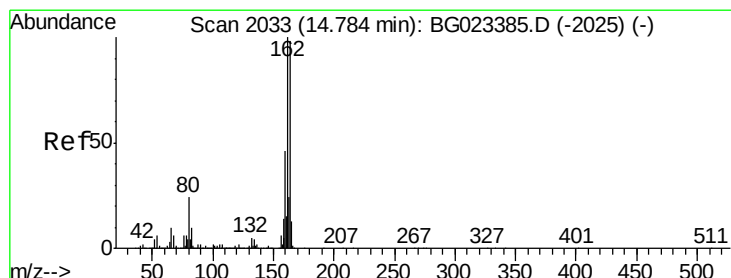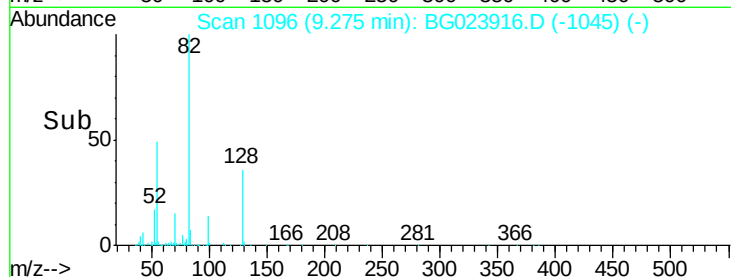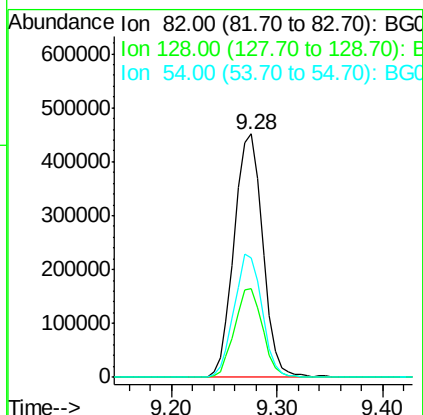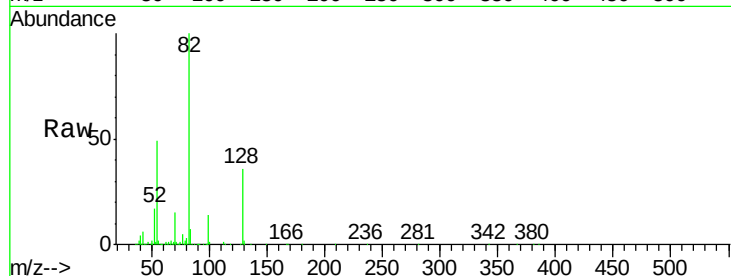

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.77 min Scan# 2031
 Delta R.T. -0.00 min
 Lab File: BG023916.D
 Acq: 26 Aug 2016 6:59

Tgt Ion	Ratio	Lower	Upper
164	100		
162	109.6	87.7	131.5
160	47.1	37.2	55.8

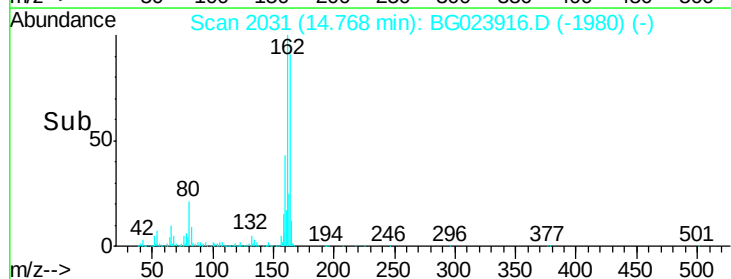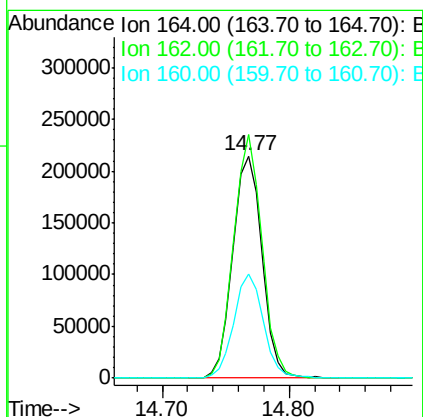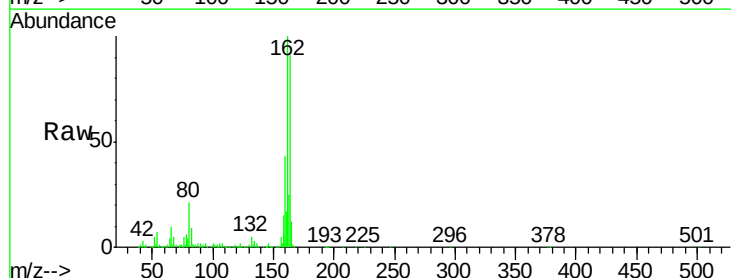


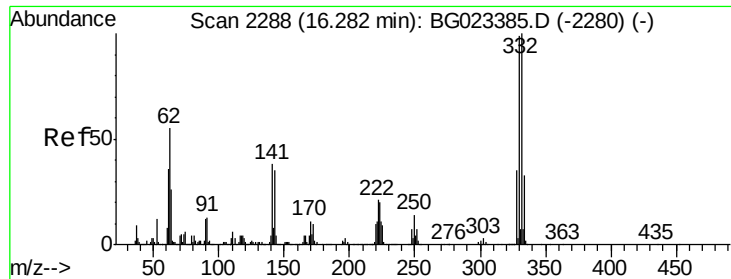




#41
 2,4,6-Tribromophenol
 Concen: 96.71 ng
 RT: 16.27 min Scan# 2287
 Delta R.T. 0.01 min
 Lab File: BG023916.D
 Acq: 26 Aug 2016 6:59

Instrument :
 BNA_G
 ClientSampleId :
 FIELDBLANK

Tgt Ion:330 Resp: 483997
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.4 116.2
 141 42.1 31.7 47.5

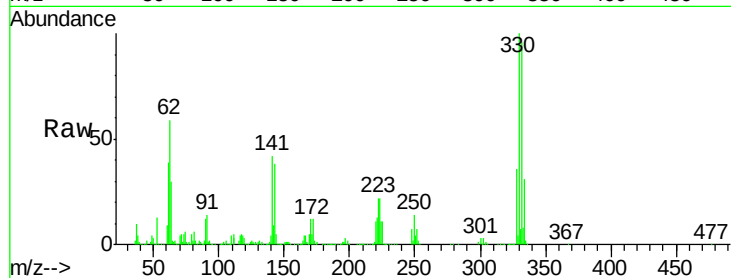


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

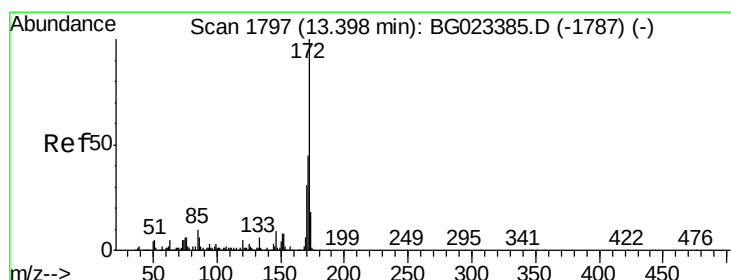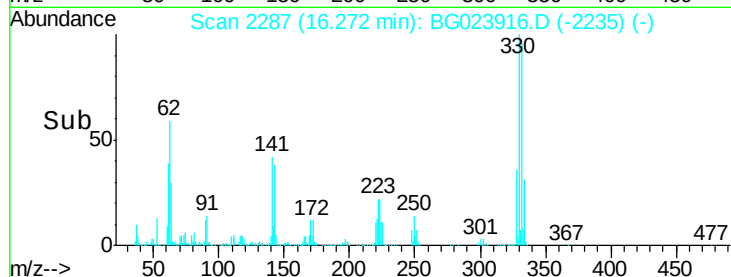
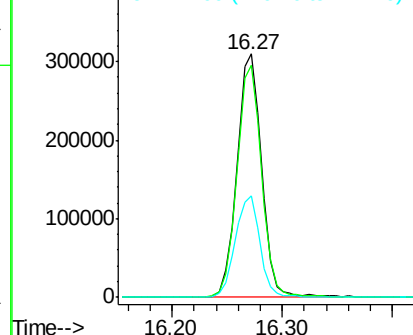



#44
 2-Fluorobiphenyl
 Concen: 80.61 ng
 RT: 13.38 min Scan# 1795
 Delta R.T. -0.00 min
 Lab File: BG023916.D
 Acq: 26 Aug 2016 6:59

Tgt Ion:172 Resp: 1635234
 Ion Ratio Lower Upper
 172 100
 171 39.9 31.6 47.4
 170 26.3 21.3 31.9

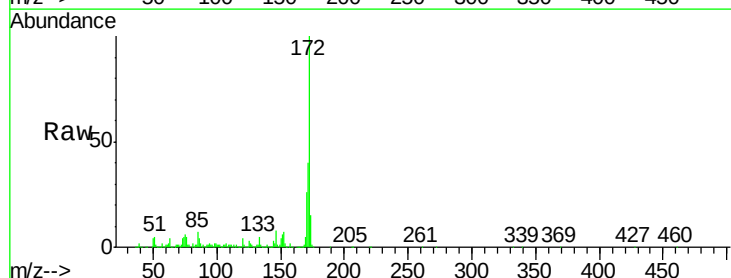

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



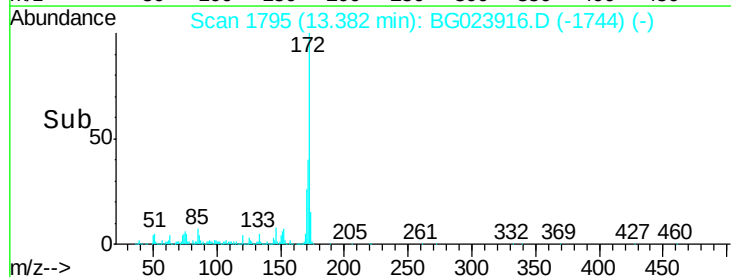
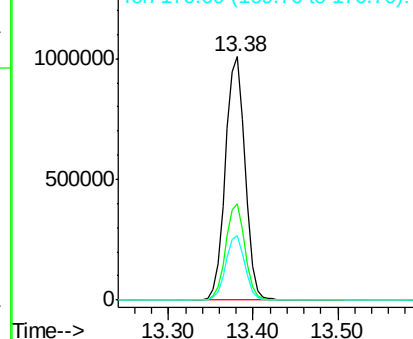


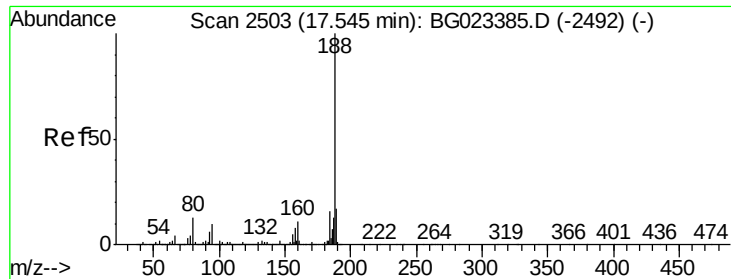

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.53 min Scan# 2502
Delta R.T. 0.01 min
Lab File: BG023916.D
Acq: 26 Aug 2016 6:59




Instrument :
BNA_G
ClientSampleId :
FIELDBLANK


Tgt Ion:188 Resp: 814782
Ion Ratio Lower Upper
188 100
94 8.0 5.2 7.8#
80 11.1 7.2 10.8#

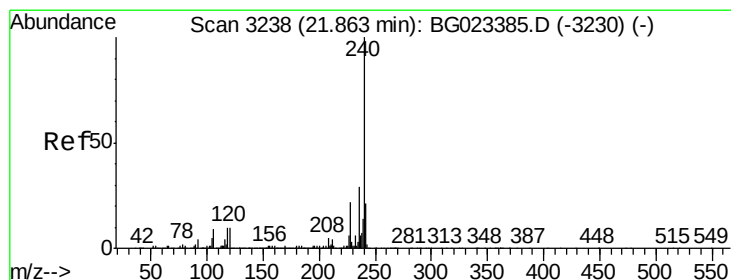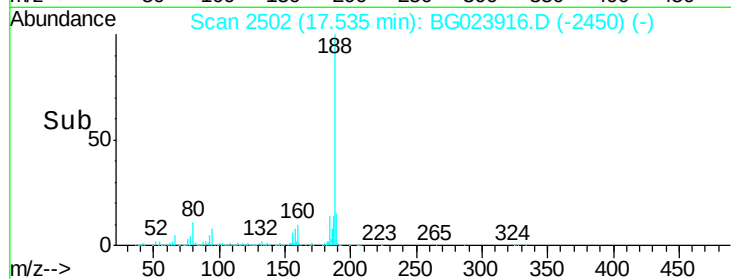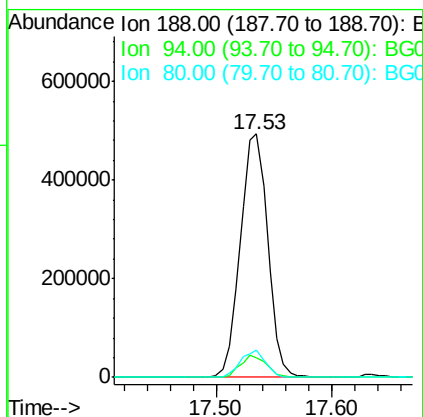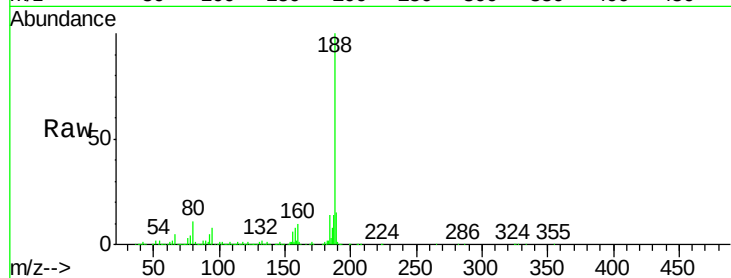

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.85 min Scan# 3237
Delta R.T. 0.01 min
Lab File: BG023916.D
Acq: 26 Aug 2016 6:59

Tgt Ion:240 Resp: 825719
Ion Ratio Lower Upper
240 100
120 8.3 4.1 6.1#
236 26.6 21.1 31.7


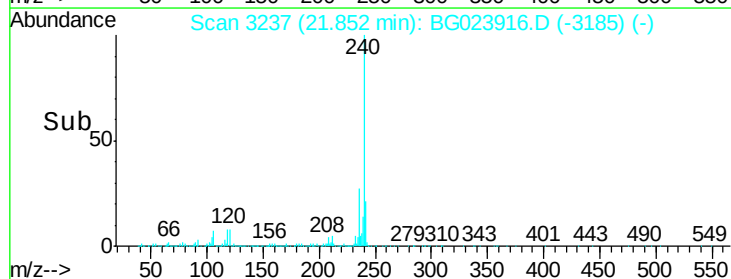
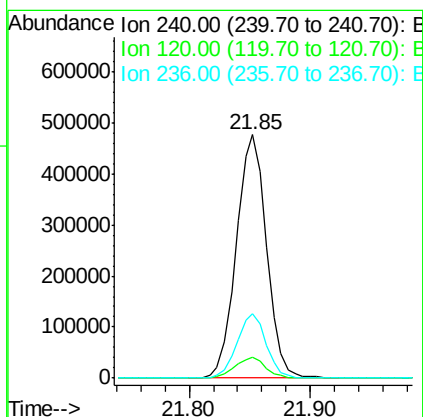
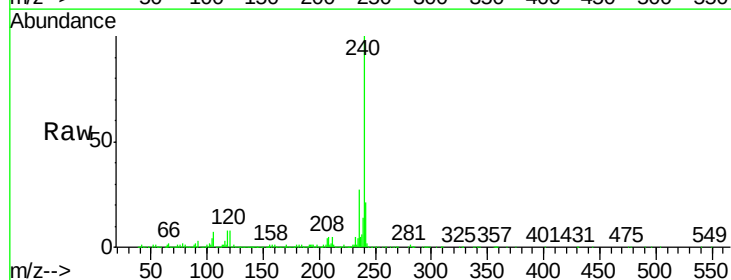


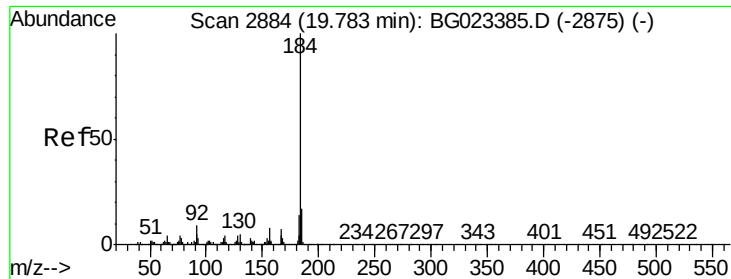

#76
Benzidine
Concen: 8.36 ng
RT: 19.77 min Scan# 2883
Delta R.T. 0.01 min
Lab File: BG023916.D
Acq: 26 Aug 2016 6:59




Instrument :
BNA_G
ClientSampleId :
FIELDBLANK


Tgt Ion:184 Resp: 191939
Ion Ratio Lower Upper
184 100
185 16.3 12.6 19.0
183 13.2 10.7 16.1

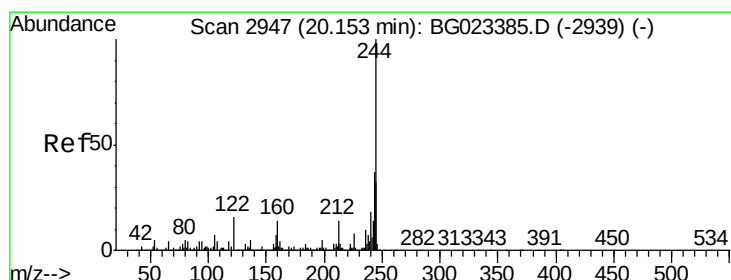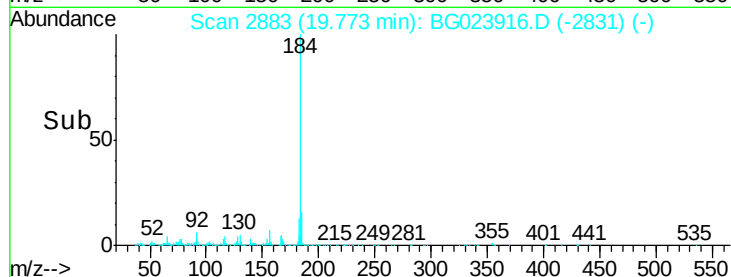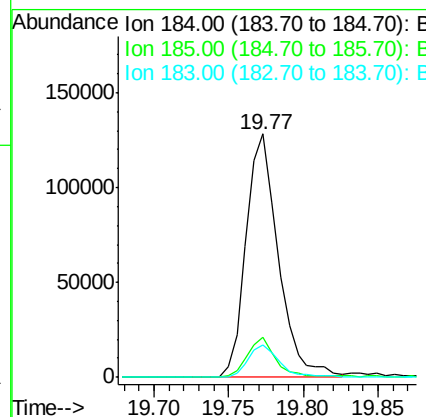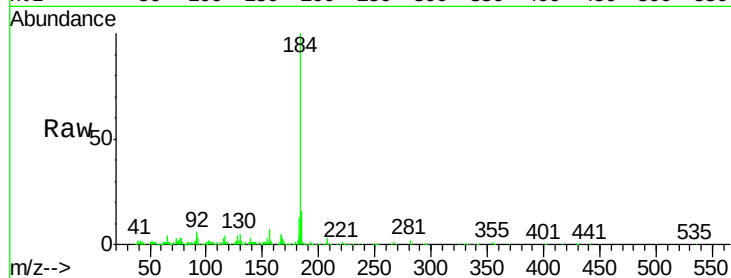

#78
Terphenyl-d14
Concen: 83.95 ng
RT: 20.14 min Scan# 2946
Delta R.T. 0.01 min
Lab File: BG023916.D
Acq: 26 Aug 2016 6:59

Tgt Ion:244 Resp: 2221418
Ion Ratio Lower Upper
244 100
212 11.3 10.8 16.2
122 11.0 8.0 12.0

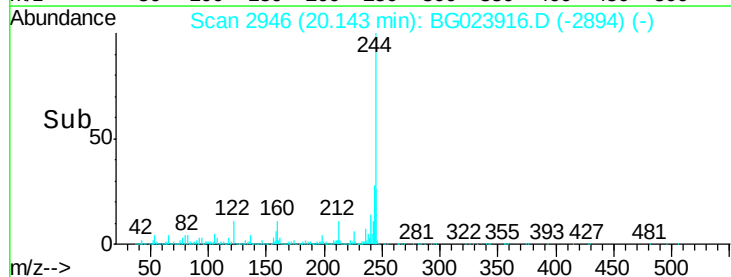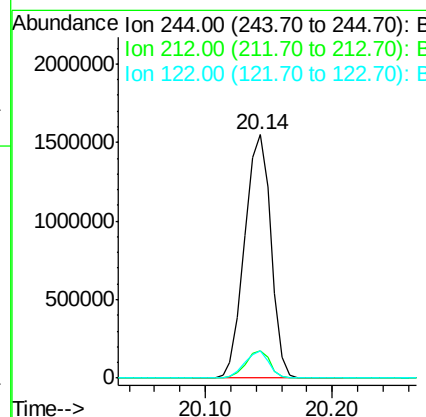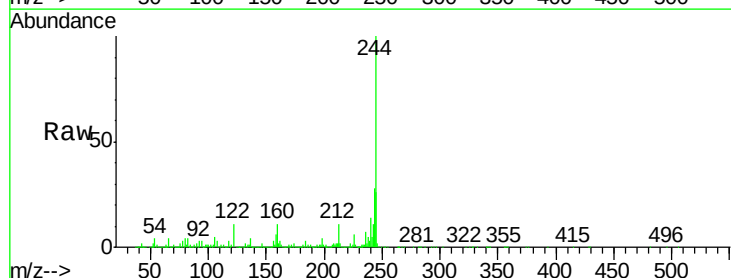

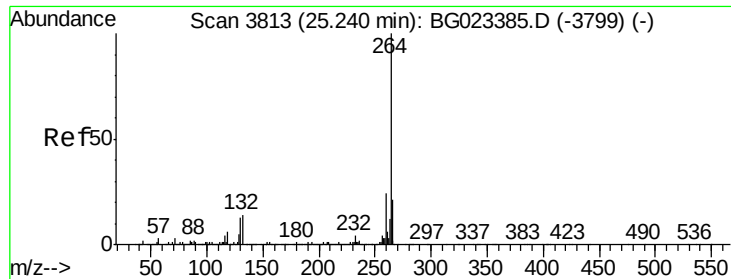

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.24 min Scan# 3814
Delta R.T. 0.02 min
Lab File: BG023916.D
Acq: 26 Aug 2016 6:59

Instrument :
BNA_G
ClientSampleId :
FIELDBLANK

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.7	18.4	27.6
265	21.9	18.9	28.3

