


Data Path : Z:\HPCHEM1\BNA_G\Data\BG082516\
 Data File : BG023892.D
 Acq On : 25 Aug 2016 8:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 26 11:26:50 2016

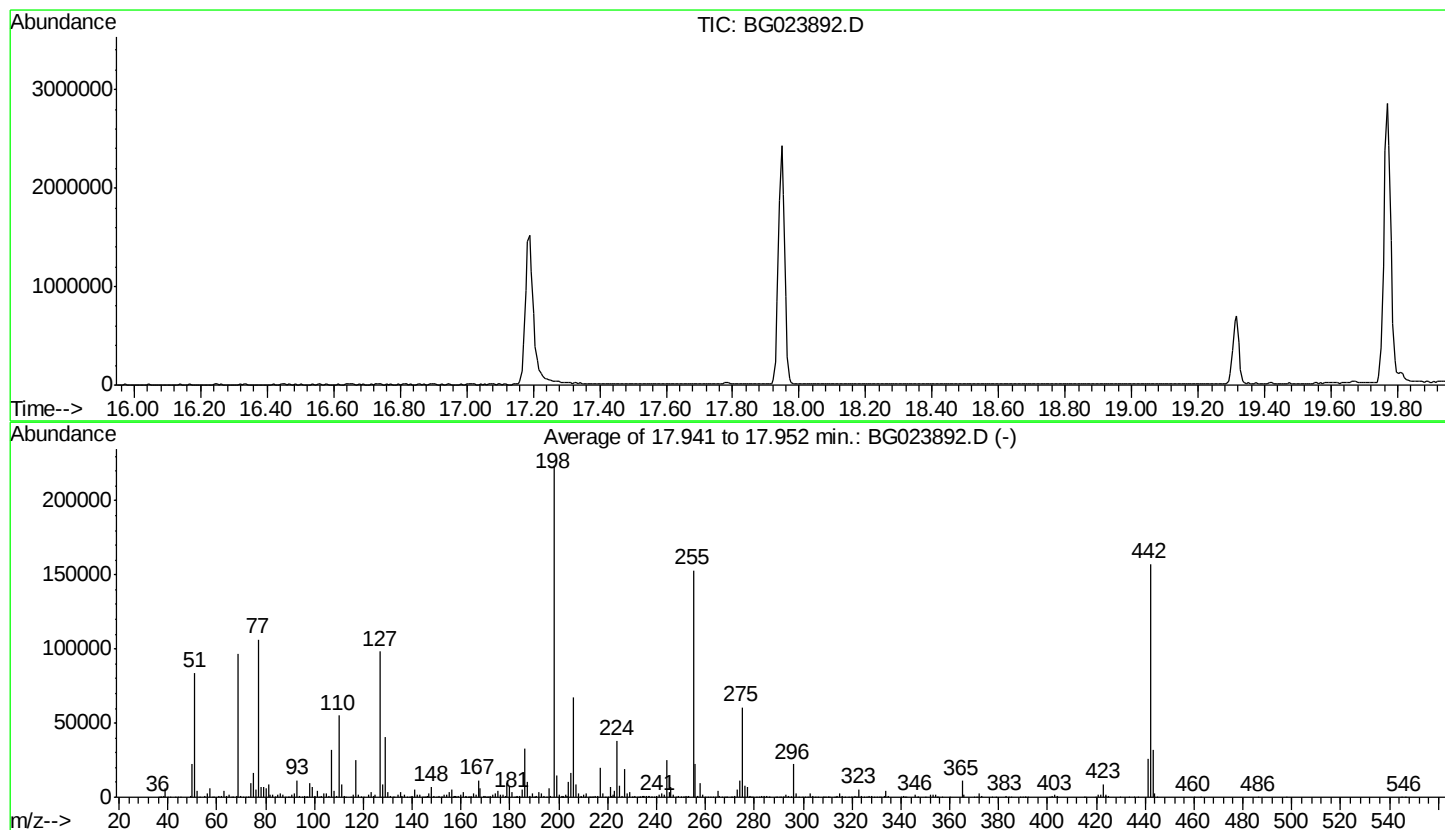

AutoFind: Scans 2571, 2572, 2573; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	83967	PASS
68	69	0.00	2	1.2	1134	PASS
69	198	0.00	100	43.3	96773	PASS
70	69	0.00	2	0.6	608	PASS
127	198	10	80	44.0	98349	PASS
197	198	0.00	2	0.3	734	PASS
198	198	100	100	100.0	223616	PASS
199	198	5	9	6.6	14772	PASS
275	198	10	60	27.1	60658	PASS
365	198	1	100	5.0	11172	PASS
441	442	0.01	24	16.4	25858	PASS
442	198	50	100	70.4	157512	PASS
443	442	15	24	20.3	32032	PASS