


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082516\
Data File : BG023895.D
Acq On : 25 Aug 2016 15:04
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 26 11:26:50 2016

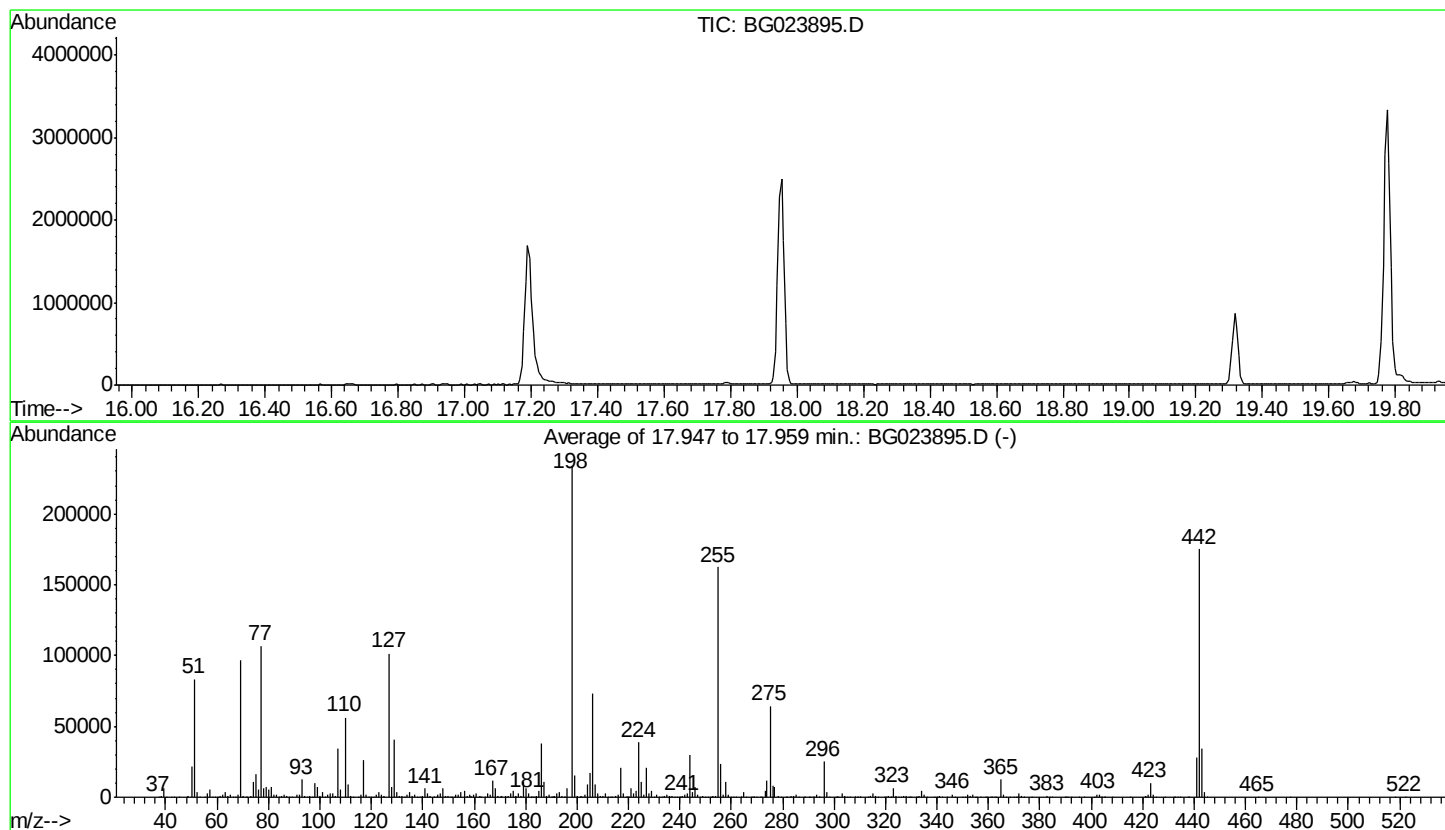

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	83565	PASS
68	69	0.00	2	1.5	1485	PASS
69	198	0.00	100	41.2	96453	PASS
70	69	0.00	2	0.6	626	PASS
127	198	10	80	43.2	101221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	234048	PASS
199	198	5	9	6.5	15270	PASS
275	198	10	60	27.6	64522	PASS
365	198	1	100	5.2	12251	PASS
441	442	0.01	24	16.2	28445	PASS
442	198	50	100	74.8	175082	PASS
443	442	15	24	19.5	34200	PASS