


Data Path : Z:\HPCHEM1\BNA_G\Data\BG082516\
 Data File : BG023910.D
 Acq On : 26 Aug 2016 1:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 26 11:26:50 2016

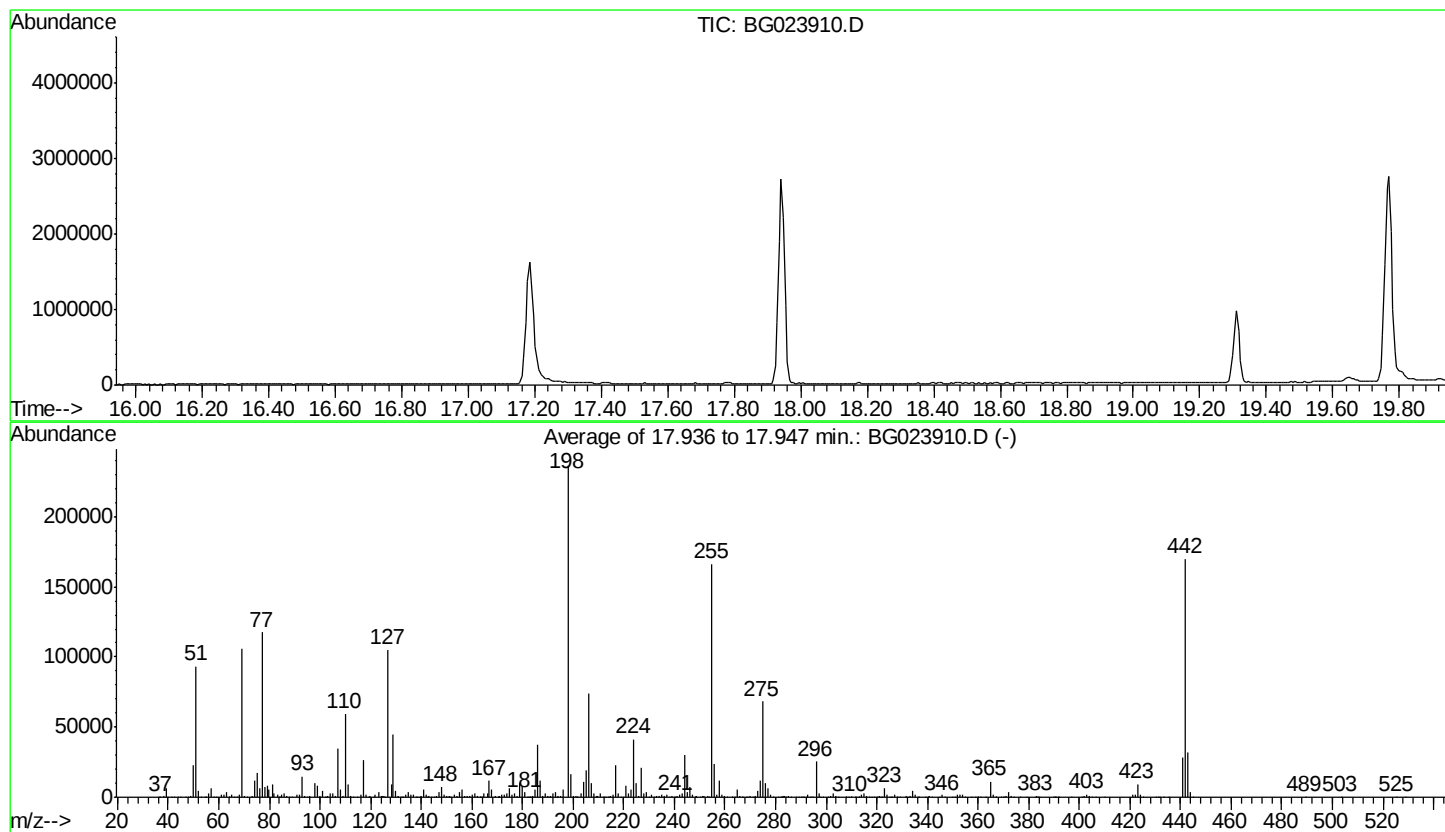

AutoFind: Scans 2570, 2571, 2572; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	93536	PASS
68	69	0.00	2	1.6	1717	PASS
69	198	0.00	100	44.9	106078	PASS
70	69	0.00	2	0.5	526	PASS
127	198	10	80	44.4	104965	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	236394	PASS
199	198	5	9	6.8	16135	PASS
275	198	10	60	28.8	68053	PASS
365	198	1	100	4.8	11320	PASS
441	442	0.01	24	16.9	28765	PASS
442	198	50	100	71.9	169856	PASS
443	442	15	24	19.0	32320	PASS