

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082517\
 Data File : BG028491.D
 Acq On : 25 Aug 2017 14:26
 Operator : SJ/JU
 Sample : PB101739BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK39

Quant Time: Aug 25 23:13:19 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 25 23:11:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	35823	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	158067	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	114461	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.70	188	283528	20.00	ng/ul	0.00
75) Chrysene-d12	22.03	240	318138	20.00	ng/ul	0.00
83) Perylene-d12	25.54	264	311500	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.82	96	4275	5.56	ng/uL	0.00
5) Phenol-d5	7.49	99	108235	27.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.65	67	71047	28.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.87	132	80159	32.30	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	95300	28.98	ng/ul	0.00
19) Nitrobenzene-d5	9.50	128	43161	34.92	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	51944	38.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.77	165	96635	34.46	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	123908	39.70	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	348604	34.24	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	398450	34.71	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	44911	27.75	ng/ul	0.00
57) Fluorene-d10	15.94	176	300582	32.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	50543	27.44	ng/ul	0.00
70) Anthracene-d10	17.80	188	486107	35.75	ng/ul	0.00
76) Pyrene-d10	20.07	212	563635	34.55	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	532859	36.54	ng/ul	0.01

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.03	70	2979	1.118	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082517\
Data File : BG028491.D
Acq On : 25 Aug 2017 14:26
Operator : SJ/JU
Sample : PB101739BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK39

Quant Time: Aug 25 23:13:19 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 25 23:11:18 2017
Response via : Initial Calibration

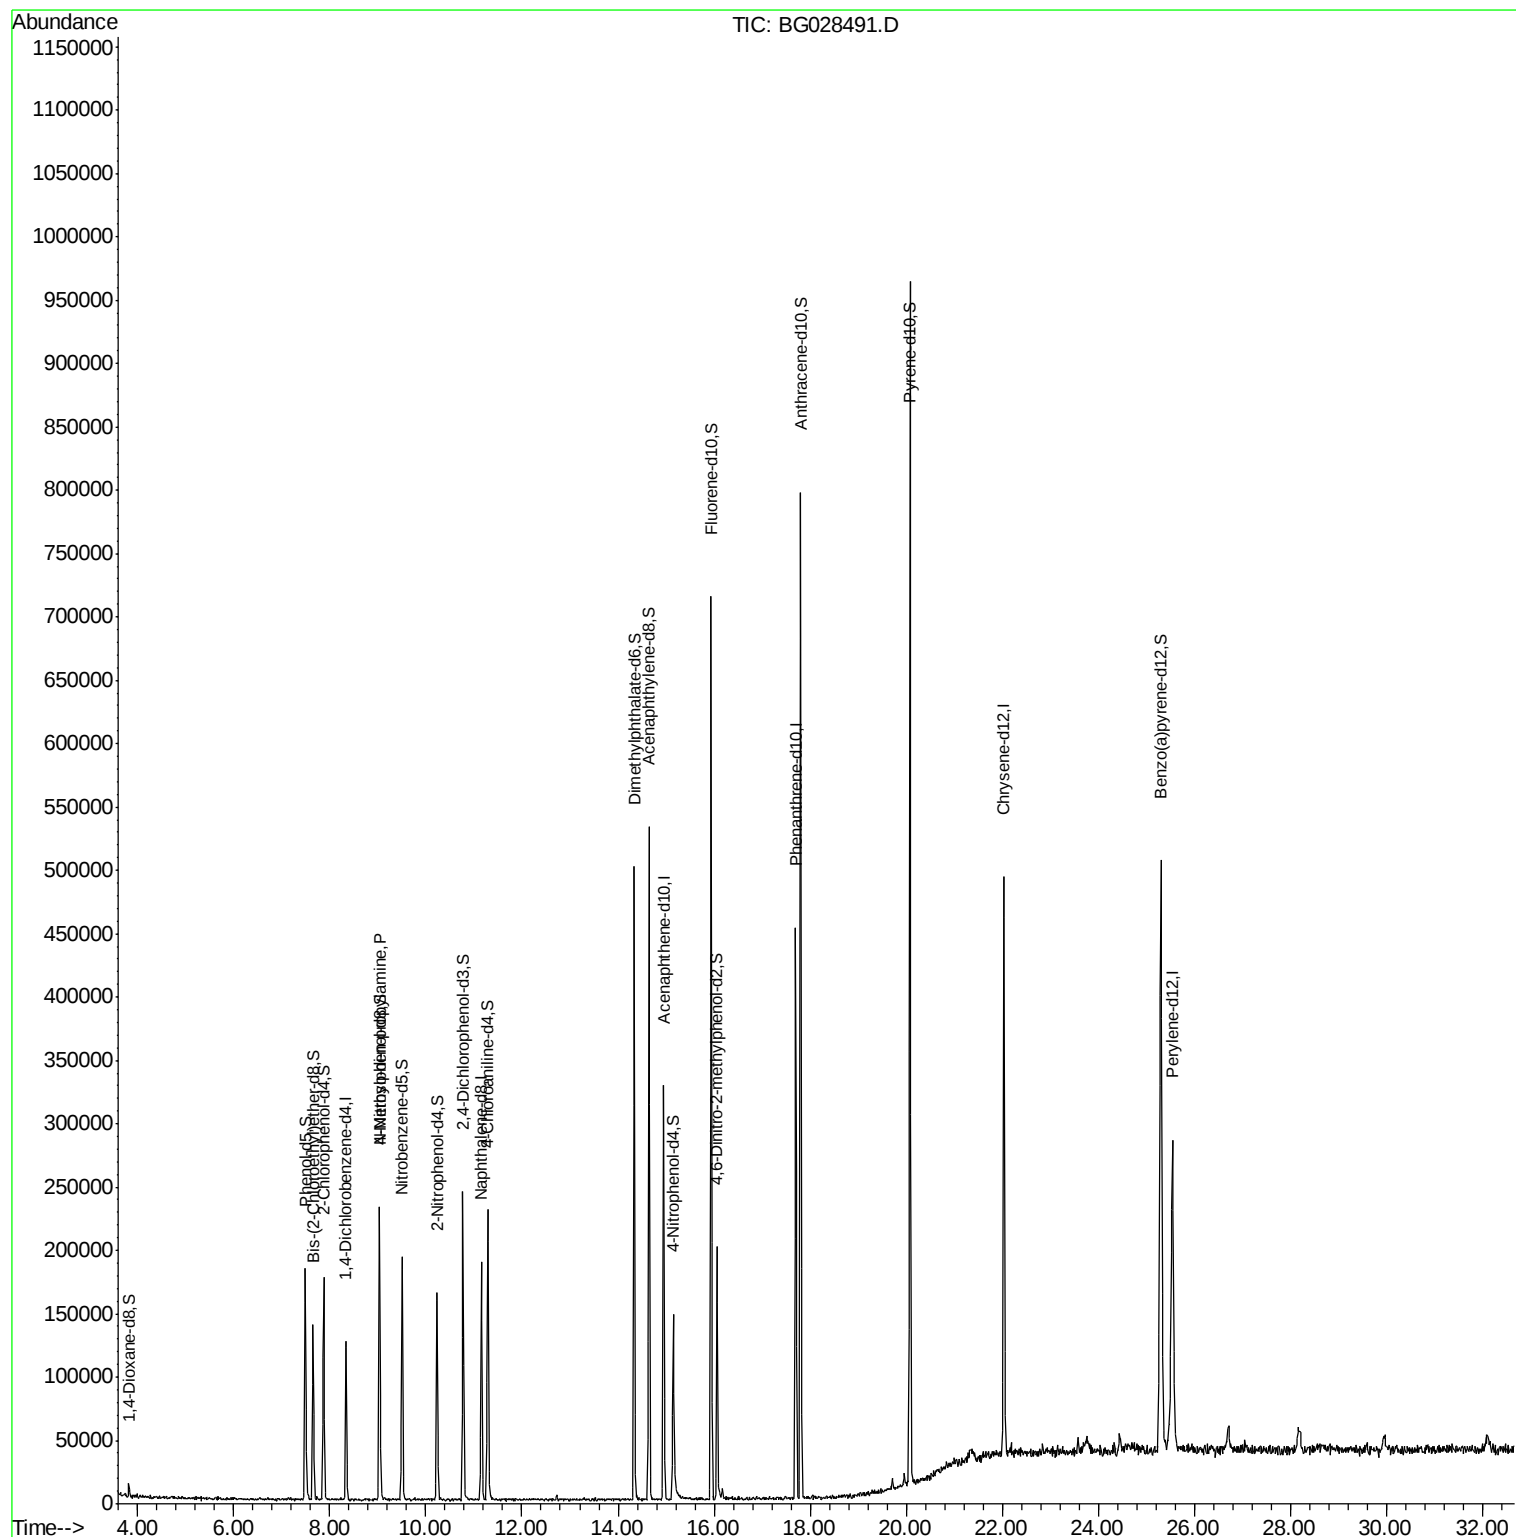

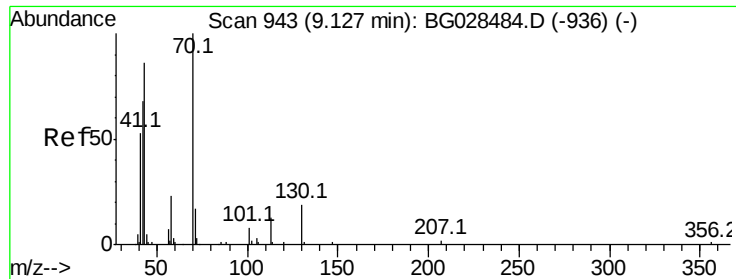

#15

N-Nitroso-di-n-propylamine

Concen: 1.118 ng/ul

RT: 9.03 min Scan# 927

Delta R.T. -0.09 min

Lab File: BG028491.D

Acq: 25 Aug 2017 14:26

Instrument :

BNA_G

ClientSampleId :

SBLK39

Tot Ion: 70 Resp: 2979



Ion Ratio Lower Upper

70 100

42 303.0 59.0 88.6#

101 0.0 6.6 9.8#

130 0.0 15.6 23.4#

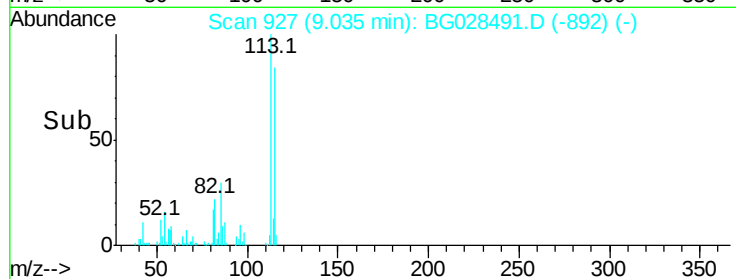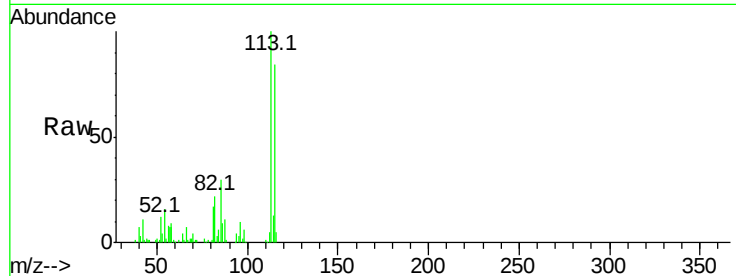

Abundance Ion 70.00 (69.70 to 70.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 101.00 (100.70 to 101.70): BGC

Ion 130.00 (129.70 to 130.70): BGC

