

Data Path : Z:\HPCHEM1\BNA_G\Data\BG082517\
 Data File : BG028487.D
 Acq On : 25 Aug 2017 11:50
 Operator : SJ/JU
 Sample : PB101454BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK54

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.682	14	16	21	rBV4	3180	3917	0.27%	0.028%
2	3.817	34	39	48	rVB7	9424	21437	1.46%	0.155%
3	3.894	51	52	55	rVB2	2263	2132	0.15%	0.015%
4	4.546	161	163	167	rBV2	2285	3267	0.22%	0.024%
5	4.705	185	190	192	rVB4	2074	3207	0.22%	0.023%
6	5.051	241	249	255	rBV5	2174	5814	0.40%	0.042%
7	5.151	259	266	269	rVB5	1856	4116	0.28%	0.030%
8	5.186	269	272	275	rBV3	1990	2567	0.17%	0.019%
9	5.245	280	282	289	rBV3	2014	4293	0.29%	0.031%
10	5.310	291	293	295	rVB2	2607	2374	0.16%	0.017%
11	5.627	341	347	353	rBV3	2725	8362	0.57%	0.061%
12	5.791	370	375	381	rBV4	1768	3261	0.22%	0.024%
13	5.844	381	384	389	rVV4	2059	2546	0.17%	0.018%
14	5.938	398	400	404	rVB3	2186	2500	0.17%	0.018%
15	6.056	417	420	423	rVB4	1686	2291	0.16%	0.017%
16	6.314	459	464	466	rBV3	2023	2324	0.16%	0.017%
17	6.455	483	488	491	rBV4	1984	2165	0.15%	0.016%
18	6.508	494	497	498	rBV2	2381	2055	0.14%	0.015%
19	6.544	502	503	508	rVB4	2428	2694	0.18%	0.020%
20	6.814	541	549	552	rBV4	2311	4894	0.33%	0.035%
21	7.178	608	611	612	rVB3	2426	2146	0.15%	0.016%
22	7.278	625	628	634	rBV3	1582	2872	0.20%	0.021%
23	7.489	655	664	680	rVB	182662	334323	22.74%	2.421%
24	7.648	682	691	703	rBV	126772	220280	14.98%	1.595%
25	7.736	705	706	711	rVB3	2139	2385	0.16%	0.017%
26	7.871	721	729	740	rBV	170974	310031	21.09%	2.245%
27	8.247	789	793	798	rVB3	1372	2351	0.16%	0.017%
28	8.336	798	808	818	rBV	112119	206430	14.04%	1.495%
29	9.035	919	927	940	rBV2	218468	413705	28.14%	2.996%
30	9.505	997	1007	1017	rBV	178721	338884	23.05%	2.454%
31	9.634	1025	1029	1034	rBV3	1598	2041	0.14%	0.015%
32	9.734	1042	1046	1050	rVB3	1463	2346	0.16%	0.017%
33	9.763	1050	1051	1057	rBV3	1339	2202	0.15%	0.016%
34	10.227	1123	1130	1143	rBV	157398	297999	20.27%	2.158%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG082517\
 Data File : BG028487.D
 Acq On : 25 Aug 2017 11:50
 Operator : SJ/JU
 Sample : PB101454BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK54

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

35	10.692	1208	1209	1214	rVB2	1330	2013	0.14%	0.015%
36	10.774	1214	1223	1236	rBV	224046	438591	29.83%	3.176%
37	10.974	1250	1257	1260	rBV3	1781	3389	0.23%	0.025%
38	11.156	1280	1288	1301	rVB	177179	328244	22.33%	2.377%
39	11.285	1301	1310	1321	rBV	208606	414207	28.17%	3.000%
40	11.420	1330	1333	1336	rVB2	1867	2347	0.16%	0.017%
41	11.467	1336	1341	1345	rBV2	2085	3398	0.23%	0.025%
42	11.596	1362	1363	1370	rVB	2116	2828	0.19%	0.020%
43	11.861	1403	1408	1411	rBV3	1972	2332	0.16%	0.017%
44	11.920	1413	1418	1419	rBV2	1635	2079	0.14%	0.015%
45	12.037	1434	1438	1444	rVB3	1948	2630	0.18%	0.019%
46	12.354	1486	1492	1499	rBV2	2207	4744	0.32%	0.034%
47	12.413	1499	1502	1505	rVB3	2114	2377	0.16%	0.017%
48	12.625	1536	1538	1543	rVB2	2047	2372	0.16%	0.017%
49	12.725	1551	1555	1563	rVB4	3759	7141	0.49%	0.052%
50	12.971	1594	1597	1601	rBV3	1755	2158	0.15%	0.016%
51	13.018	1601	1605	1609	rBV3	1301	2618	0.18%	0.019%
52	13.089	1616	1617	1624	rVB4	1745	3055	0.21%	0.022%
53	13.142	1624	1626	1630	rBV2	1561	1992	0.14%	0.014%
54	13.706	1718	1722	1726	rBV	2419	5397	0.37%	0.039%
55	13.811	1737	1740	1743	rBV3	1995	3291	0.22%	0.024%
56	14.334	1822	1829	1843	rBV	470505	716157	48.71%	5.186%
57	14.646	1874	1882	1891	rBV	486500	783953	53.32%	5.677%
58	14.951	1923	1934	1943	rBV2	302543	512717	34.87%	3.713%
59	15.045	1943	1950	1955	rVB2	1659	3267	0.22%	0.024%
60	15.145	1959	1967	1987	rBV	148723	338070	22.99%	2.448%
61	15.445	2014	2018	2021	rVB3	1403	2229	0.15%	0.016%
62	15.703	2058	2062	2066	rBV2	1509	2425	0.16%	0.018%
63	15.797	2075	2078	2080	rBV	1581	2032	0.14%	0.015%
64	15.938	2093	2102	2112	rBV	662569	1021251	69.46%	7.396%
65	16.062	2115	2123	2138	rBV2	185468	321387	21.86%	2.327%
66	16.179	2138	2143	2149	rVB3	7995	12324	0.84%	0.089%
67	16.432	2181	2186	2189	rBV2	2247	3385	0.23%	0.025%
68	16.614	2215	2217	2221	rBV2	2659	3044	0.21%	0.022%
69	16.867	2255	2260	2262	rBV	1854	2638	0.18%	0.019%
70	17.043	2288	2290	2294	rVB2	2283	2324	0.16%	0.017%
71	17.090	2294	2298	2300	rBV3	1674	2217	0.15%	0.016%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG082517\
 Data File : BG028487.D
 Acq On : 25 Aug 2017 11:50
 Operator : SJ/JU
 Sample : PB101454BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK54

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

72	17.190	2312	2315	2319	rVB4	2174	2432	0.17%	0.018%
73	17.237	2319	2323	2326	rBV3	2559	3108	0.21%	0.023%
74	17.331	2334	2339	2341	rVB	2137	2418	0.16%	0.018%
75	17.360	2341	2344	2347	rBV3	1669	2073	0.14%	0.015%
76	17.484	2360	2365	2370	rVB3	2662	5368	0.37%	0.039%
77	17.572	2376	2380	2381	rVB2	2020	2140	0.15%	0.015%
78	17.701	2392	2402	2410	rBV	424574	647231	44.02%	4.687%
79	17.801	2412	2419	2432	rVB	778047	1194623	81.25%	8.651%
80	17.965	2446	2447	2450	rBV	2941	2291	0.16%	0.017%
81	18.306	2502	2505	2509	rVB2	3379	5185	0.35%	0.038%
82	18.341	2509	2511	2515	rBV3	3331	5249	0.36%	0.038%
83	18.506	2537	2539	2543	rVB3	3325	3092	0.21%	0.022%
84	18.559	2543	2548	2553	rBV4	2913	6122	0.42%	0.044%
85	18.594	2553	2554	2557	rBV2	3098	2331	0.16%	0.017%
86	18.641	2558	2562	2564	rVB4	2842	2282	0.16%	0.017%
87	18.676	2564	2568	2569	rBV5	2241	2523	0.17%	0.018%
88	18.788	2585	2587	2590	rBV3	2491	3387	0.23%	0.025%
89	18.853	2596	2598	2600	rVB3	2315	2028	0.14%	0.015%
90	18.964	2613	2617	2622	rVB6	4050	7034	0.48%	0.051%
91	19.070	2630	2635	2637	rBV5	3806	5705	0.39%	0.041%
92	19.376	2685	2687	2689	rBV3	3459	2487	0.17%	0.018%
93	19.710	2740	2744	2749	rBV4	11247	20172	1.37%	0.146%
94	19.957	2783	2786	2792	rVB6	10812	14187	0.96%	0.103%
95	20.075	2798	2806	2815	rBV	930022	1413158	96.12%	10.234%
96	22.031	3132	3139	3149	rBV	453144	784533	53.36%	5.681%
97	24.434	3546	3548	3557	rVB6	21289	38638	2.63%	0.280%
98	25.292	3683	3694	3714	rBV2	465522	1470244	100.00%	10.647%
99	25.533	3720	3735	3753	rVB	225929	844202	57.42%	6.113%
100	26.691	3927	3932	3945	rVB6	35662	123892	8.43%	0.897%


Sum of corrected areas: 13808969

Data Path : Z:\HPCHEM1\BNA_G\Data\BG082517\
Data File : BG028487.D
Acq On : 25 Aug 2017 11:50
Operator : SJ/JU
Sample : PB101454BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK54

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

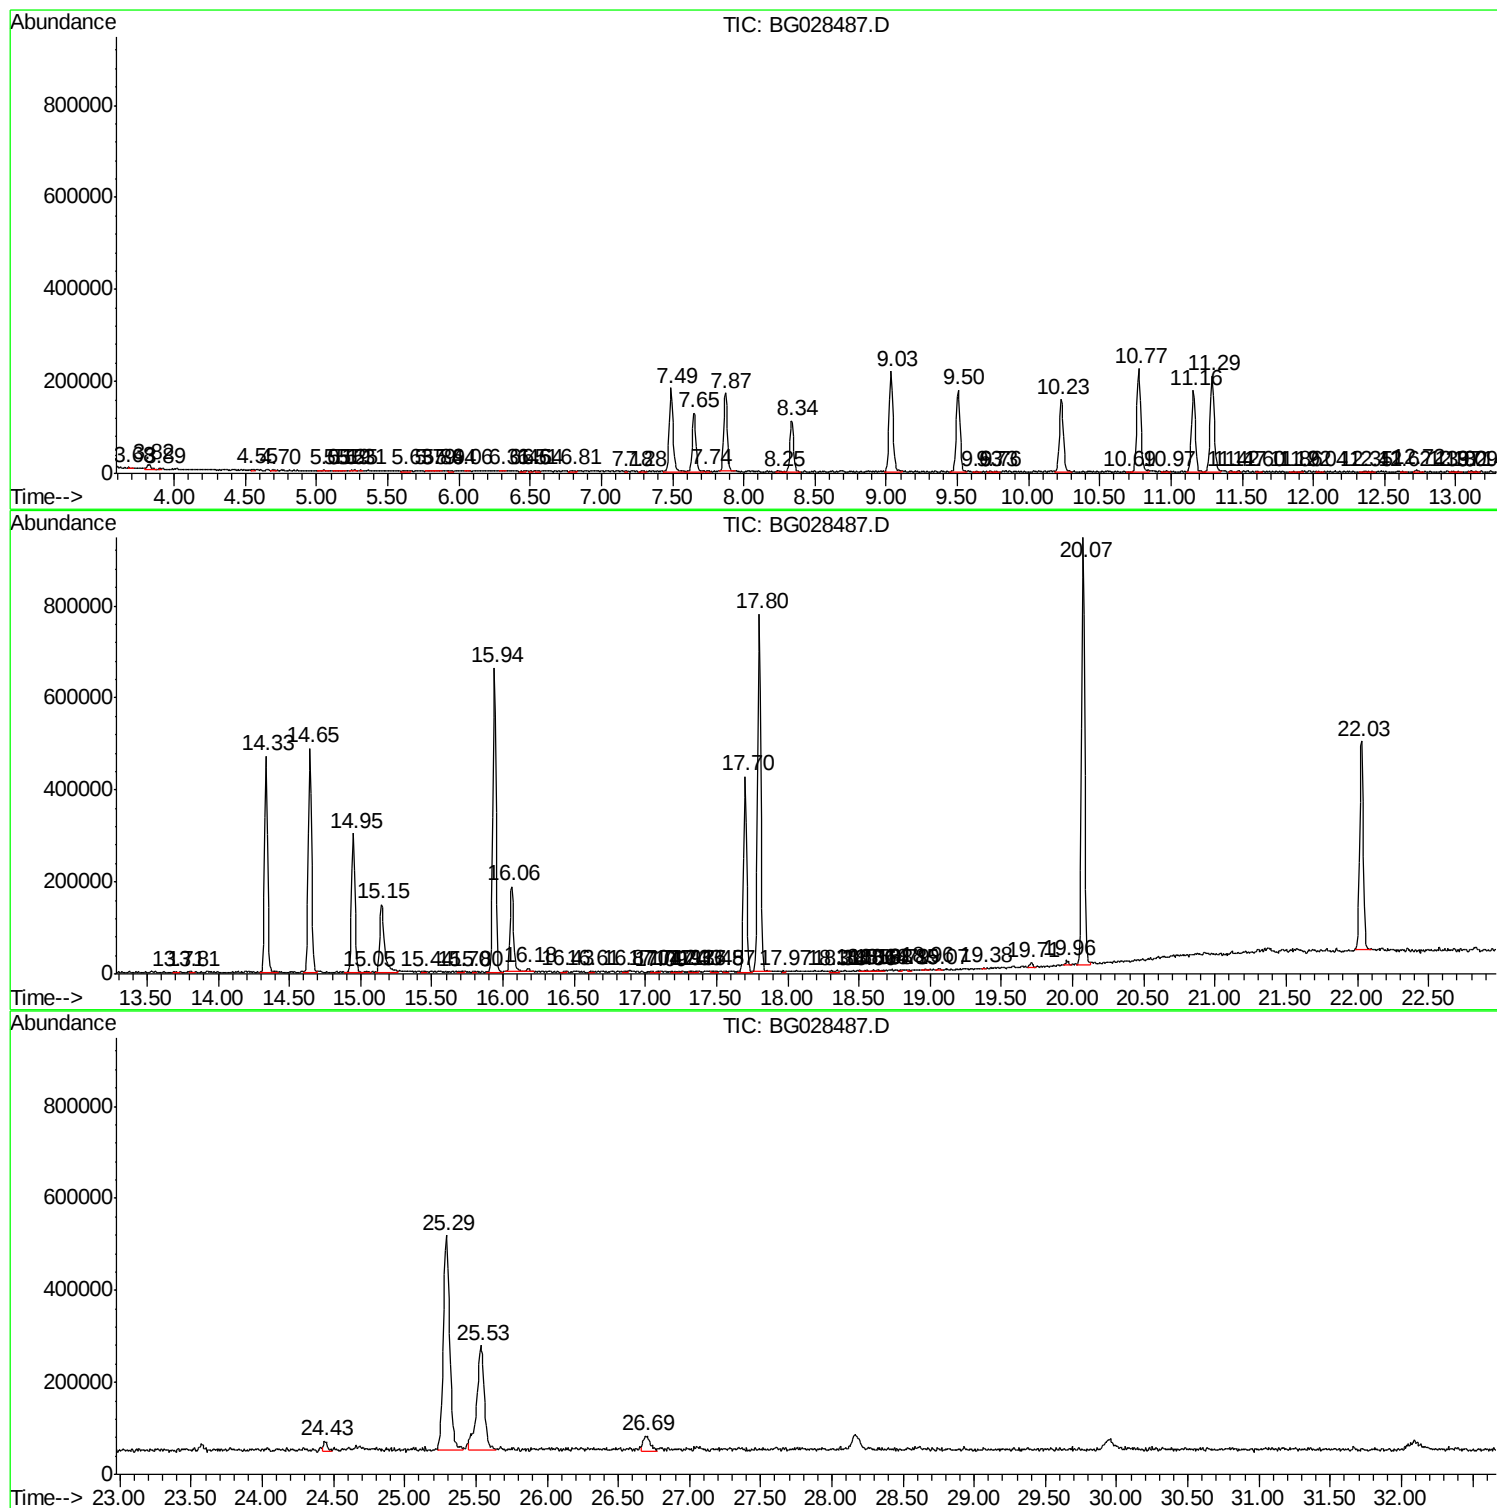

Data Path : Z:\HPCHEM1\BNA_G\Data\BG082517\
Data File : BG028487.D
Acq On : 25 Aug 2017 11:50
Operator : SJ/JU
Sample : PB101454BL
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
SBLK54

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.
26.69	2.94 ng/ul	123892	Perylene-d12		25.53
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Dotriacontane	451	C32H66	000544-85-4	43
2	Octacosane	394	C28H58	000630-02-4	43
3	Tetradecane	198	C14H30	000629-59-4	43
4	Docosane, 7-butyl-	366	C26H54	055282-15-0	43
5	Undecane, 4-ethyl-	184	C13H28	017312-59-3	43

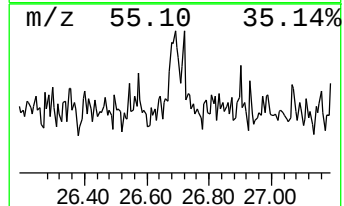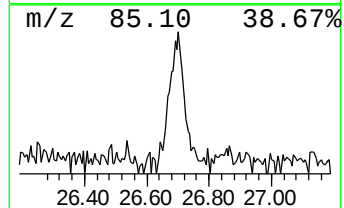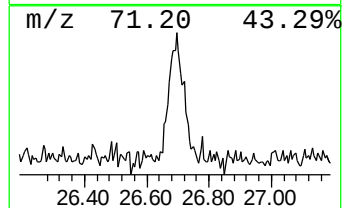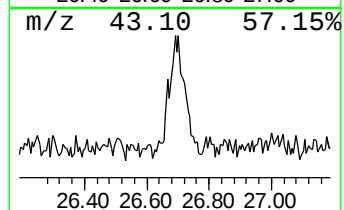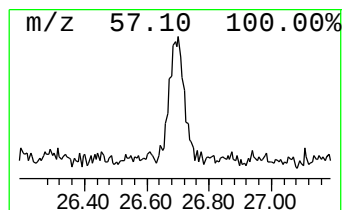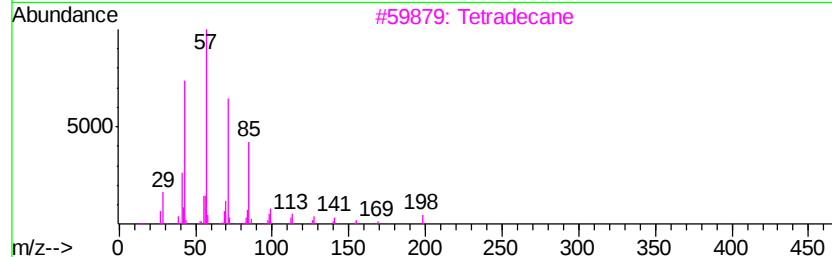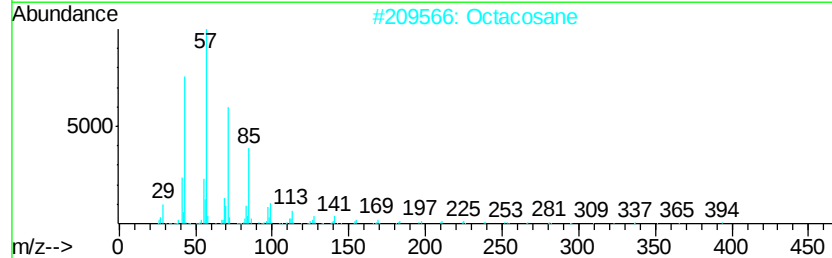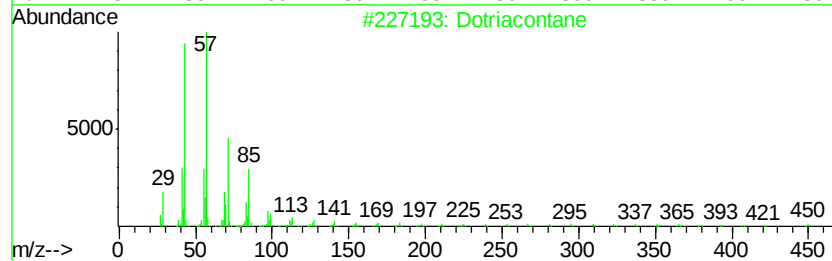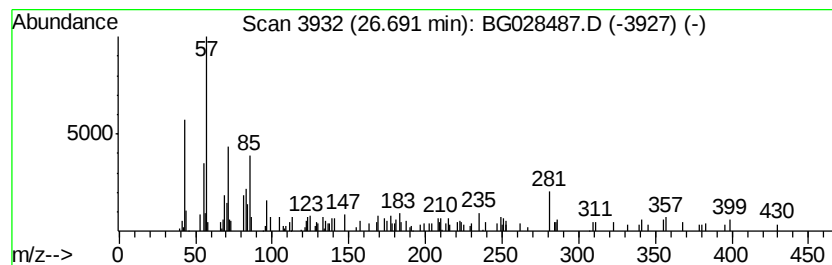

Data Path : Z:\HPCHEM1\BNA_G\Data\BG082517\
Data File : BG028487.D
Acq On : 25 Aug 2017 11:50
Operator : SJ/JU
Sample : PB101454BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK54

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	26.69	2.9	ng/ul	123892	6	25.53	844202	20.0

m/z	Abundance
40.00	2129.0
41.10	267.0
44.00	427.0
48.90	194.0
57.20	316.0
69.00	207.0
73.10	160.0
81.10	339.0
84.90	160.0
95.00	181.0
97.00	190.0
98.00	186.0
103.20	150.0
105.00	167.0
143.00	206.0
207.00	228.0
207.90	153.0
311.40	171.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

m/z	Abundance
38.00	296.0
39.10	1703.0
40.10	1897.0
41.00	221.0
43.00	180.0
44.10	435.0
46.80	210.0
49.00	238.0
50.10	5035.0
51.10	22352.0
52.20	1357.0
55.20	517.0
56.10	849.0
57.00	1188.0
61.00	437.0
62.00	265.0
63.20	1009.0
65.10	449.0
66.90	187.0
68.10	583.0
69.00	20768.0
73.10	475.0
74.10	2425.0
75.10	3851.0
76.00	1379.0
77.10	23120.0
78.10	1342.0
79.00	1599.0
80.10	1261.0
81.00	2351.0
82.00	466.0
83.10	334.0
84.00	211.0
85.00	214.0
86.00	626.0
87.00	283.0
91.10	693.0
92.00	436.0
93.10	2495.0
93.90	220.0
98.10	1957.0
99.10	1065.0
100.10	174.0
101.00	695.0
103.00	377.0
104.00	1011.0
105.10	467.0
106.10	268.0
107.00	6827.0
108.10	1085.0
110.00	11453.0
111.00	2105.0
112.00	176.0
114.40	198.0
116.10	222.0
117.10	4664.0
118.10	493.0
121.90	385.0
123.00	922.0
124.00	349.0
125.00	671.0
127.00	21896.0
128.10	1409.0
129.00	8557.0
130.00	927.0
134.10	331.0
135.00	802.0
136.00	384.0
137.10	408.0
141.00	1651.0
142.10	712.0
143.10	441.0
144.80	159.0
147.00	690.0
148.00	1571.0
149.10	277.0
151.10	252.0
153.10	426.0
154.20	157.0
155.10	952.0
156.00	1367.0
156.90	284.0
157.80	396.0
158.90	218.0
159.90	629.0
161.00	533.0
162.00	267.0
163.20	185.0
165.10	402.0
166.10	547.0
167.10	2224.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

168.10	1124.0
168.90	340.0
171.00	192.0
172.00	263.0
173.00	476.0
174.00	760.0
175.00	944.0
177.00	690.0
179.00	2395.0
180.00	1605.0
181.20	464.0
182.10	261.0
185.00	1335.0
186.00	6806.0
187.10	2659.0
188.00	253.0
189.00	504.0
190.10	153.0
191.00	421.0
192.00	754.0
193.00	634.0
194.00	272.0
196.10	1640.0
196.60	715.0
198.00	54032.0
199.00	4481.0
200.10	471.0
201.80	226.0
203.00	348.0
204.10	1546.0
205.00	4368.0
206.00	15221.0
207.10	2539.0
207.90	495.0
209.00	381.0
210.30	236.0
211.10	875.0
213.00	281.0
216.10	502.0
217.00	3873.0
218.00	468.0
221.10	2044.0
222.00	816.0
223.00	725.0
224.00	8574.0
225.00	2021.0
226.00	269.0
227.00	3883.0
227.90	294.0
228.90	709.0
230.00	185.0
231.10	605.0
234.00	168.0
234.90	244.0
236.00	380.0
237.00	284.0
239.00	267.0
240.10	165.0
241.00	369.0
241.90	485.0
243.20	518.0
244.00	5606.0
245.00	560.0
246.10	1114.0
246.90	325.0
248.90	583.0
251.00	158.0
253.20	304.0
254.00	523.0
255.00	36760.0
256.00	5673.0
256.90	511.0
258.00	1435.0
258.90	475.0
260.90	155.0
264.10	153.0
265.00	903.0
271.00	270.0
273.00	833.0
274.00	2865.0
275.00	14255.0
276.00	1628.0
277.00	1294.0
277.90	241.0
280.90	151.0
283.20	253.0
283.80	160.0
285.00	315.0
286.90	212.0
288.00	203.0
292.10	152.0
292.90	331.0
296.00	4157.0
297.00	839.0
303.00	552.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

314.20	404.0
314.90	218.0
315.90	173.0
323.10	2007.0
324.20	273.0
327.00	273.0
327.90	278.0
332.10	296.0
333.20	307.0
334.10	903.0
335.10	225.0
341.10	255.0
345.90	310.0
352.00	280.0
353.10	226.0
354.00	319.0
365.00	1550.0
365.90	255.0
372.10	887.0
373.20	151.0
383.10	215.0
401.90	162.0
403.10	492.0
404.00	291.0
420.90	538.0
422.10	374.0
423.00	2625.0
424.00	322.0
441.00	6145.0
442.00	36408.0
443.00	7029.0
444.00	553.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

m/z	Abundance
38.10	171.0
39.10	1126.0
40.00	2080.0
41.10	412.0
44.00	469.0
49.00	220.0
50.10	6130.0
51.10	25344.0
52.10	1244.0
55.10	321.0
56.00	603.0
57.10	2004.0
61.00	405.0
62.10	425.0
63.00	661.0
65.10	463.0
67.20	235.0
69.00	24432.0
70.10	156.0
73.00	301.0
74.00	2463.0
75.10	3527.0
76.10	1160.0
77.10	24672.0
78.10	1376.0
79.00	1713.0
80.10	1285.0
81.00	1880.0
82.10	595.0
83.10	499.0
84.10	258.0
84.90	187.0
85.90	424.0
87.00	378.0
88.00	168.0
91.00	672.0
92.20	437.0
93.00	3203.0
94.10	323.0
96.10	164.0
98.10	2849.0
99.00	2095.0
100.00	181.0
101.00	1537.0
102.90	439.0
104.10	779.0
105.00	649.0
106.00	416.0
107.10	9337.0
108.10	1113.0
109.10	810.0
110.00	14656.0
111.10	2277.0
112.10	283.0
116.10	603.0
117.10	5243.0
117.90	458.0
119.10	179.0
120.00	220.0
121.20	187.0
121.90	468.0
123.10	1053.0
124.00	335.0
125.00	459.0
127.00	29008.0
128.10	3389.0
129.00	11055.0
130.00	1178.0
134.00	623.0
135.00	927.0
136.00	451.0
137.00	359.0
140.10	170.0
141.00	1416.0
142.10	705.0
143.00	664.0
146.10	303.0
147.00	676.0
148.00	1913.0
148.90	335.0
151.40	322.0
153.20	443.0
154.00	440.0
155.00	888.0
156.00	1584.0
157.00	423.0
158.10	465.0
160.20	599.0
161.00	1079.0
161.70	193.0
165.00	936.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

166.00	493.0
167.00	2672.0
167.90	1332.0
169.00	222.0
170.90	161.0
172.10	430.0
173.00	390.0
174.10	774.0
175.10	1371.0
175.90	237.0
177.00	769.0
178.00	228.0
179.00	2787.0
180.00	2288.0
181.00	961.0
182.10	265.0
184.20	223.0
185.10	1580.0
186.00	9668.0
187.00	2361.0
188.10	417.0
188.90	690.0
191.10	219.0
192.00	895.0
193.00	1257.0
193.60	255.0
194.10	242.0
195.00	240.0
196.00	1756.0
198.00	73464.0
198.90	4309.0
200.10	513.0
201.40	171.0
203.10	674.0
204.00	3130.0
205.00	4833.0
206.10	20432.0
207.00	2627.0
207.90	510.0
209.00	424.0
210.10	391.0
210.70	605.0
212.20	161.0
215.00	447.0
216.00	451.0
217.00	6225.0
218.00	579.0
219.10	173.0
221.00	2465.0
222.00	815.0
223.00	1046.0
224.00	11021.0
225.00	3168.0
226.10	329.0
227.00	5616.0
227.90	848.0
229.00	1212.0
230.00	234.0
230.90	191.0
234.00	337.0
235.10	438.0
235.90	158.0
236.90	439.0
240.10	200.0
241.00	338.0
242.00	844.0
243.10	528.0
244.00	7547.0
245.10	1207.0
246.10	1443.0
247.00	399.0
247.80	166.0
248.90	330.0
251.90	192.0
252.90	592.0
255.00	49624.0
256.00	6937.0
257.10	610.0
258.00	3204.0
259.00	485.0
265.00	1204.0
270.80	269.0
271.90	155.0
273.00	1602.0
274.00	3946.0
275.00	20840.0
276.10	3162.0
276.90	1634.0
278.10	510.0
280.90	162.0
283.10	317.0
284.10	297.0
285.00	370.0
289.00	219.0
293.00	466.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

294.10	232.0
296.00	5068.0
296.90	982.0
301.10	167.0
301.70	162.0
303.00	586.0
304.10	375.0
307.80	170.0
311.90	215.0
314.00	258.0
314.90	877.0
316.00	366.0
323.10	1509.0
324.00	465.0
327.00	450.0
332.00	325.0
334.10	1414.0
334.90	423.0
341.10	440.0
346.00	272.0
352.10	750.0
353.10	472.0
354.00	645.0
355.20	177.0
365.00	3130.0
366.00	558.0
371.10	278.0
372.00	1272.0
372.90	158.0
383.00	353.0
390.00	185.0
392.00	190.0
401.80	303.0
403.00	498.0
404.00	343.0
421.00	389.0
422.00	646.0
423.00	4001.0
424.00	539.0
425.10	218.0
433.60	207.0
441.00	10447.0
442.00	61304.0
443.00	11941.0
444.00	1199.0
544.50	183.0

Instrument :

BNA_G

ClientSampleId :

SBLK54

m/z	Abundance
37.10	213.0
38.10	194.0
39.10	995.0
40.00	1949.0
44.00	513.0
49.20	199.0
50.10	4238.0
51.10	17128.0
52.10	1544.0
55.00	334.0
56.10	798.0
57.00	1363.0
61.20	288.0
62.10	242.0
63.10	897.0
64.10	173.0
65.10	442.0
67.20	175.0
67.90	399.0
69.00	16600.0
70.10	236.0
74.10	2555.0
75.00	2555.0
76.10	1110.0
77.10	20856.0
78.10	1199.0
79.10	1040.0
80.00	1463.0
81.10	1991.0
82.00	304.0
83.10	638.0
85.00	315.0
85.90	474.0
87.00	236.0
91.00	364.0
92.10	456.0
93.10	2161.0
94.20	202.0
95.10	200.0
96.10	186.0
98.00	1785.0
99.00	1253.0
100.10	241.0
101.00	606.0
103.00	313.0
104.00	560.0
105.10	553.0
105.90	240.0
107.10	6759.0
108.10	1024.0
108.90	204.0
110.00	11291.0
111.00	1408.0
112.10	332.0
116.00	635.0
117.00	5006.0
117.90	277.0
121.50	171.0
122.10	394.0
123.10	532.0
124.20	338.0
125.00	469.0
127.10	21824.0
128.10	1935.0
129.00	7233.0
130.00	724.0
134.00	258.0
135.00	1237.0
136.20	494.0
137.00	242.0
139.90	165.0
141.00	1281.0
142.00	566.0
142.80	484.0
145.00	162.0
146.10	293.0
147.10	634.0
148.00	1356.0
149.20	324.0
150.00	154.0
153.10	579.0
154.00	434.0
155.00	560.0
156.00	1382.0
157.10	329.0
158.10	150.0
159.90	348.0
160.90	580.0
164.00	254.0
165.00	397.0
166.00	659.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

167.10	2114.0
168.00	1018.0
169.00	242.0
169.90	206.0
171.30	165.0
171.80	309.0
172.90	411.0
173.90	593.0
175.00	1098.0
175.90	295.0
176.90	469.0
178.10	220.0
179.00	1741.0
180.00	1582.0
181.00	823.0
183.00	228.0
184.00	335.0
185.10	1023.0
186.10	7576.0
187.10	1938.0
188.10	350.0
188.90	506.0
191.00	360.0
192.00	867.0
192.90	929.0
194.10	215.0
195.10	175.0
196.10	1706.0
196.80	851.0
198.00	60904.0
199.00	3931.0
200.00	472.0
200.90	261.0
201.10	250.0
201.40	272.0
202.90	602.0
204.00	2484.0
205.00	3378.0
206.10	16472.0
207.00	2414.0
208.00	511.0
210.00	306.0
211.00	390.0
213.10	208.0
215.10	173.0
216.10	395.0
217.00	4774.0
218.00	750.0
221.00	2107.0
222.00	592.0
223.00	954.0
224.00	9063.0
225.00	2681.0
226.10	170.0
227.00	4225.0
227.90	878.0
229.00	1109.0
231.00	375.0
232.90	155.0
233.80	189.0
235.00	296.0
236.20	223.0
236.90	452.0
240.10	162.0
241.00	365.0
242.00	463.0
242.60	300.0
243.20	551.0
244.00	7201.0
245.00	728.0
246.00	1753.0
247.00	396.0
249.10	325.0
251.00	191.0
253.10	249.0
255.00	42304.0
256.00	5615.0
256.90	317.0
258.00	2237.0
259.10	859.0
264.00	185.0
265.00	862.0
272.30	167.0
273.00	801.0
274.00	2874.0
275.00	17048.0
276.00	3272.0
277.00	1565.0
278.10	315.0
285.00	311.0
290.00	210.0
293.00	308.0
296.00	5639.0
296.90	668.0
303.10	727.0

Instrument :
BNA_G
ClientSampleId :
SBLK54

304.00	220.0
310.00	228.0
314.00	315.0
315.10	523.0
316.10	240.0
320.90	208.0
323.00	1858.0
324.10	377.0
327.00	586.0
328.10	285.0
333.20	210.0
334.00	1144.0
335.10	378.0
340.90	333.0
346.10	333.0
350.20	200.0
352.10	386.0
353.00	708.0
354.00	641.0
365.00	2892.0
366.00	319.0
371.00	342.0
372.00	967.0
382.90	602.0
388.60	250.0
399.30	168.0
402.10	253.0
403.00	528.0
421.00	503.0
422.20	506.0
423.10	3529.0
424.00	776.0
441.00	8763.0
442.00	62288.0
443.00	11832.0
444.10	818.0

Instrument :
BNA_G
ClientSampleId :
SBLK54