

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082519\
 Data File : BG042486.D
 Acq On : 25 Aug 2019 20:15
 Operator : HP/JU
 Sample : K4451-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B-1

Quant Time: Aug 26 08:38:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	49043	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	191351	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	137873	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	332184	20.00	ng	0.00
76) Chrysene-d12	21.68	240	366945	20.00	ng	-0.01
87) Perylene-d12	24.93	264	426883	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	299818	123.81	ng	0.00
7) Phenol-d6	7.17	99	409230	125.11	ng	0.00
23) Nitrobenzene-d5	9.16	82	232135	83.83	ng	-0.01
42) 2,4,6-Tribromophenol	16.15	330	239003	121.96	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	708262	86.88	ng	0.00
79) Terphenyl-d14	20.03	244	1343113	79.13	ng	0.00
Target Compounds						
50) Dimethylphthalate	14.10	163	131334	13.202	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082519\
Data File : BG042486.D
Acq On : 25 Aug 2019 20:15
Operator : HP/JU
Sample : K4451-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B-1

Quant Time: Aug 26 08:38:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

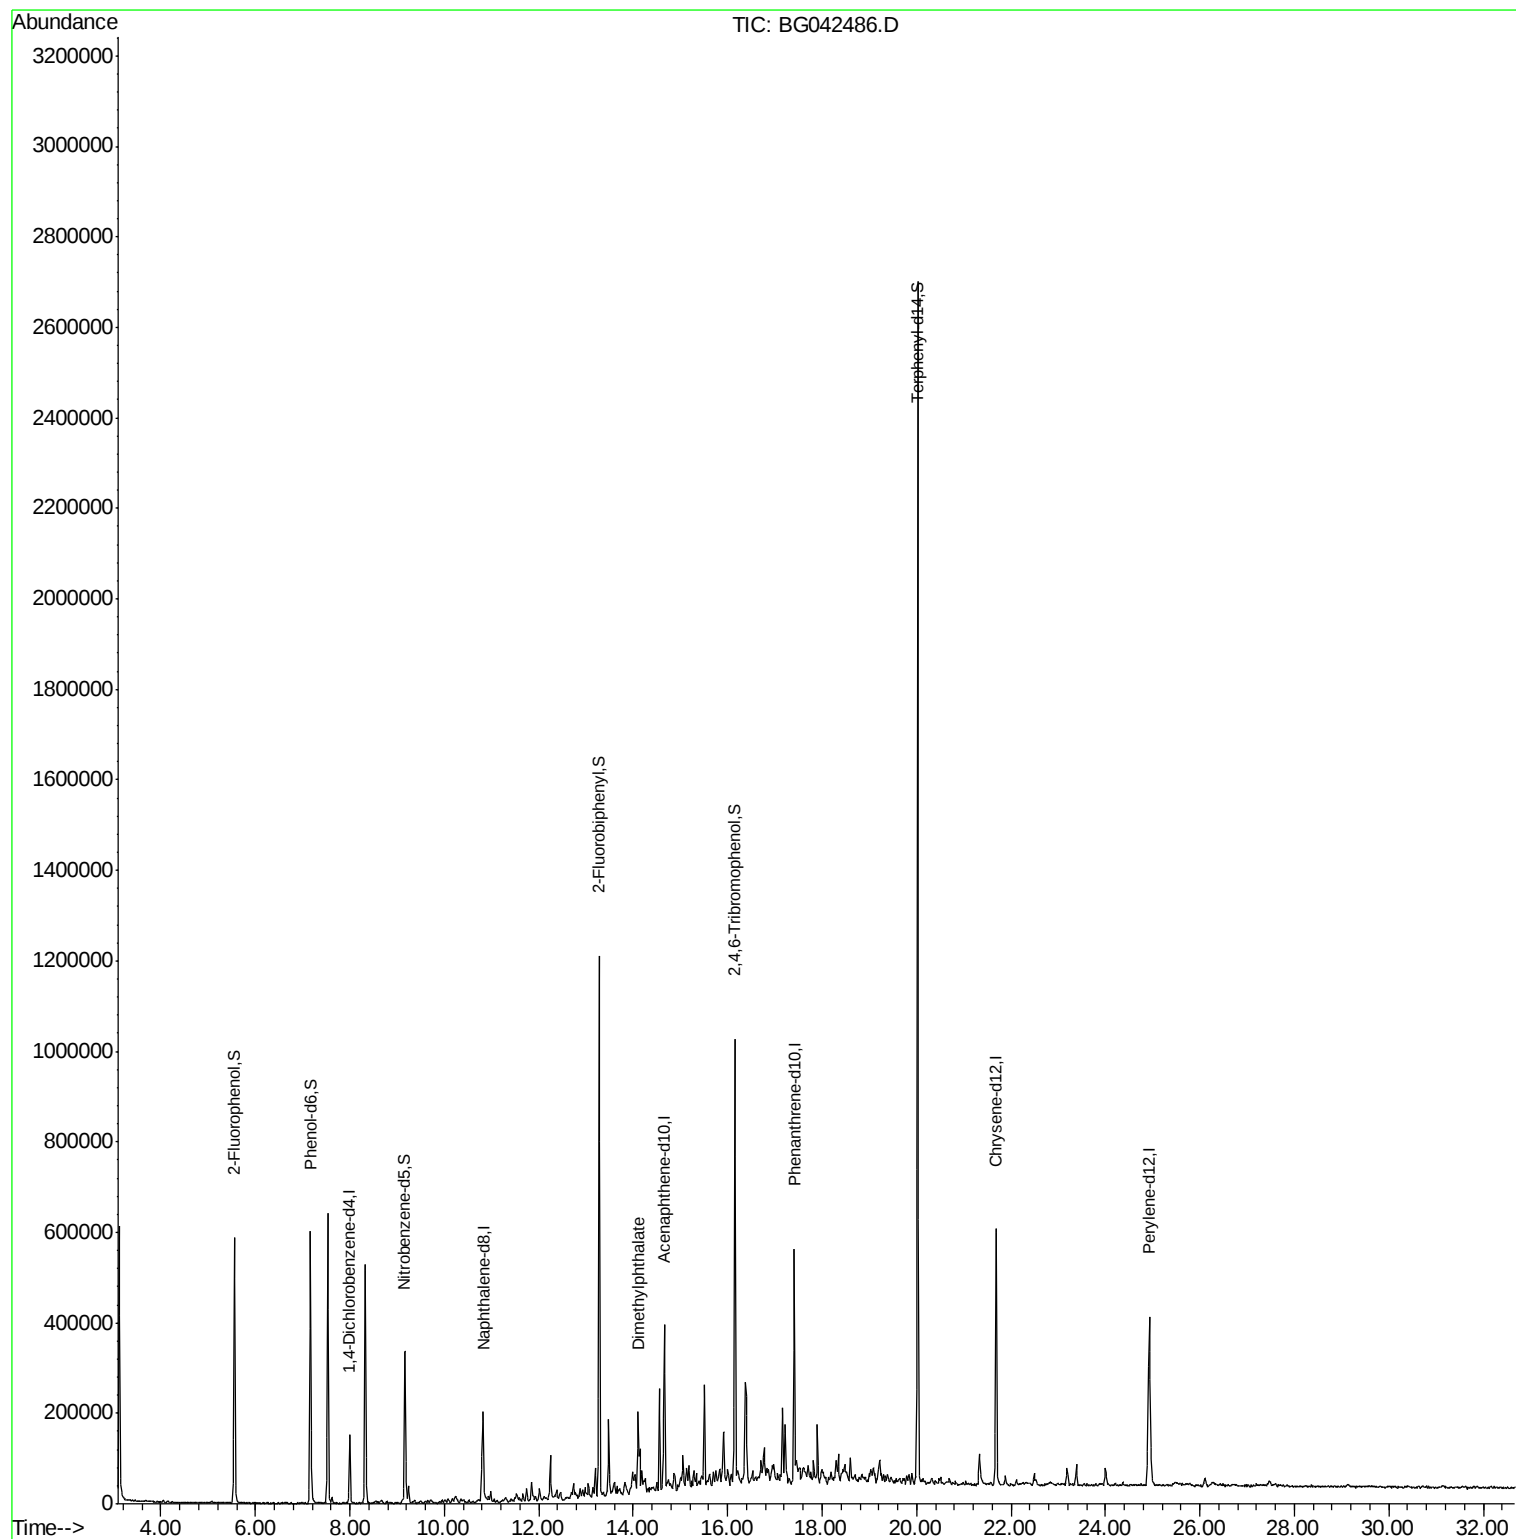




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.00 min Scan# 836
 Delta R.T. -0.01 min
 Lab File: BG042486.D
 Acq: 25 Aug 2019 20:15

Instrument :
 BNA_G
 ClientSampleId :
 B-1

Tot Ion:152 Resp: 49043
 Ion Ratio Lower Upper
 152 100
 150 159.6 125.4 188.0
 115 54.8 38.5 57.7

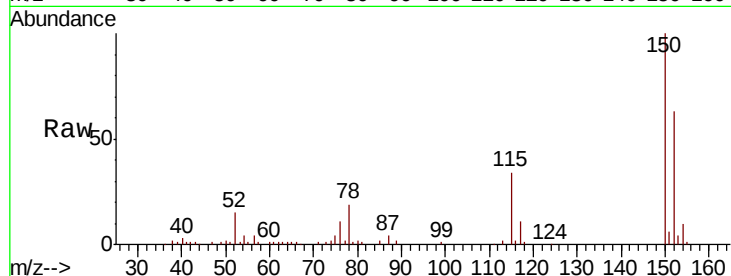


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

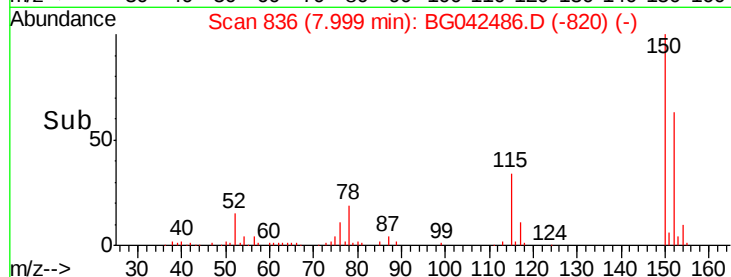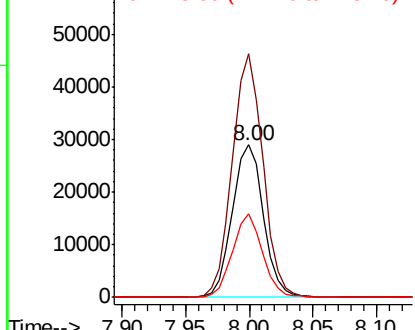



#5


2-Fluorophenol
 Concen: 123.814 ng
 RT: 5.56 min Scan# 420
 Delta R.T. -0.01 min
 Lab File: BG042486.D
 Acq: 25 Aug 2019 20:15

Tgt Ion:112 Resp: 299818
 Ion Ratio Lower Upper
 112 100
 64 55.5 42.8 64.2
 63 28.7 22.7 34.1

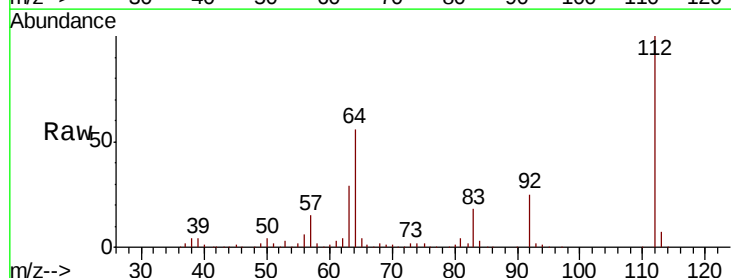

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

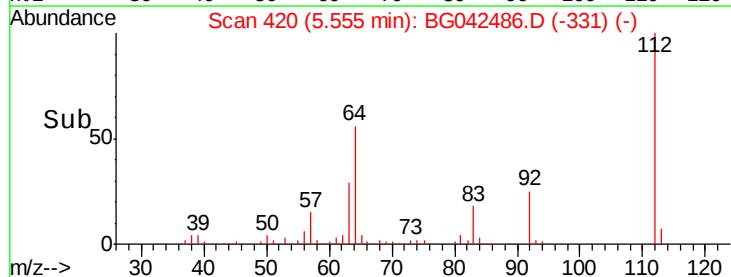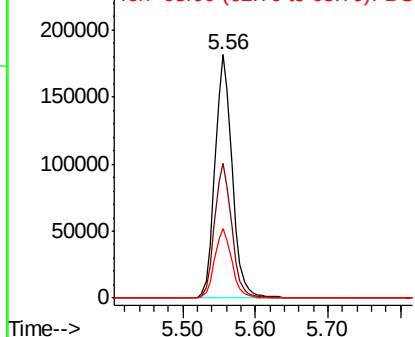

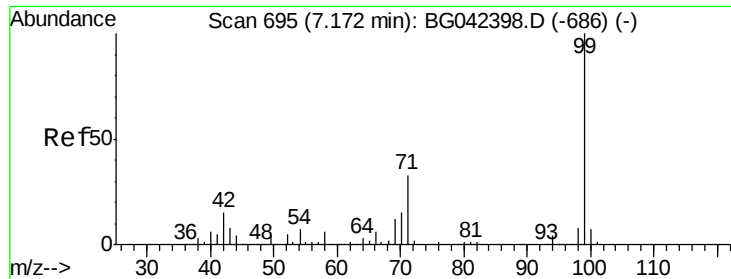

#7

Phenol-d6

Concen: 125.111 ng

RT: 7.17 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG042486.D

Acq: 25 Aug 2019 20:15

Instrument :

BNA_G

ClientSampleId :

B-1


Tot Ion: 99 Resp: 409230

Ion Ratio Lower Upper




99 100

42 14.0 12.0 18.0

71 31.7 26.3 39.5

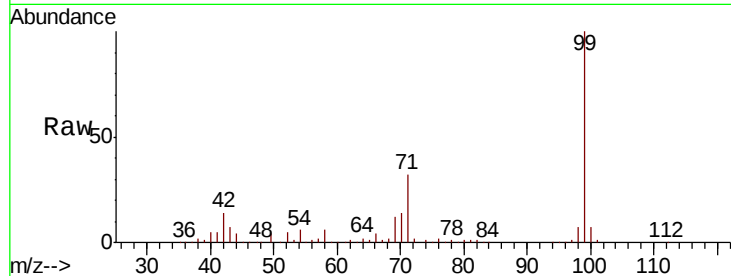

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

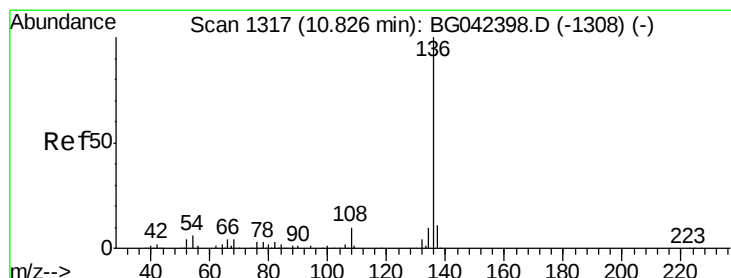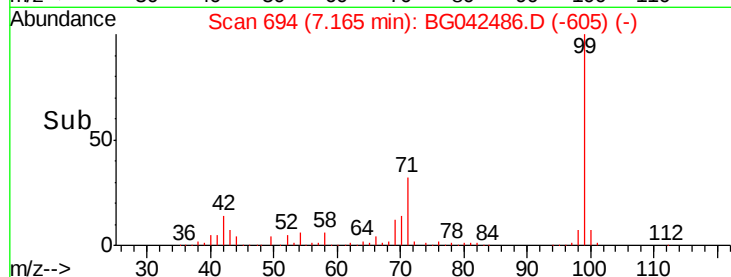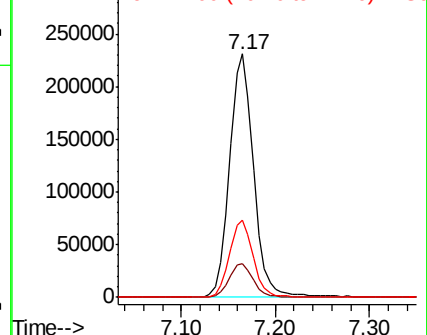

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG042486.D

Acq: 25 Aug 2019 20:15

Tgt Ion: 136 Resp: 191351


Ion Ratio Lower Upper

136 100



137 11.3 8.7 13.1


54 6.7 4.9 7.3

68 4.7 3.6 5.4

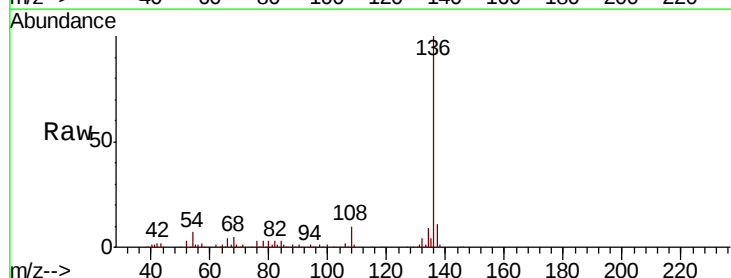

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

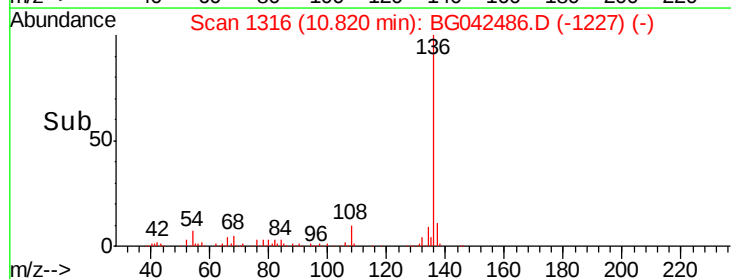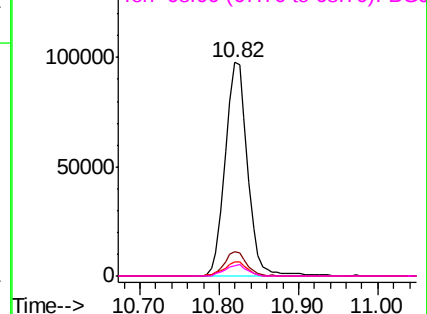


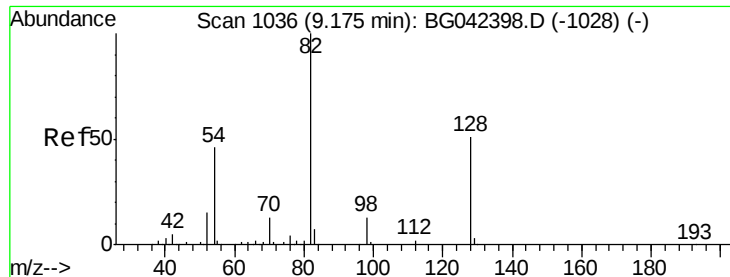




#23
 Nitrobenzene-d5
 Concen: 83.833 ng
 RT: 9.16 min Scan# 1034
 Delta R.T. -0.01 min
 Lab File: BG042486.D
 Acq: 25 Aug 2019 20:15

Instrument :
 BNA_G
 ClientSampleId :
 B-1

Tot Ion	82	Resp	232135
Ion Ratio	Lower	Upper	
82	100		
128	50.8	40.7	61.1
54	45.8	36.3	54.5

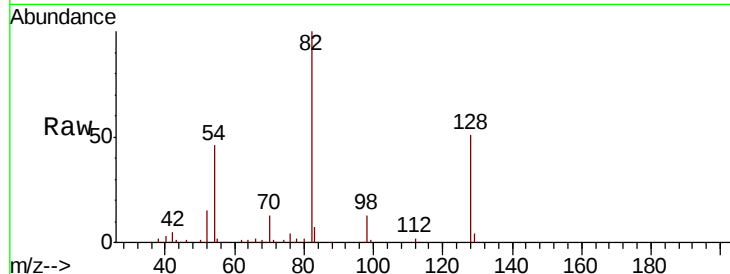


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

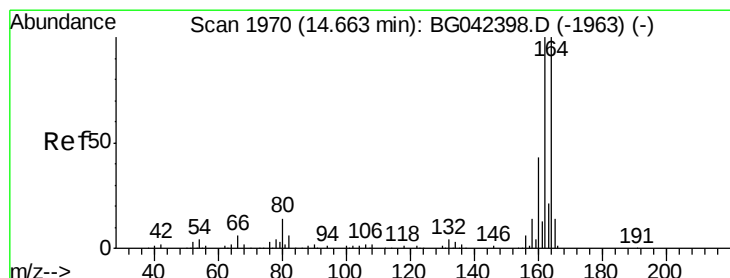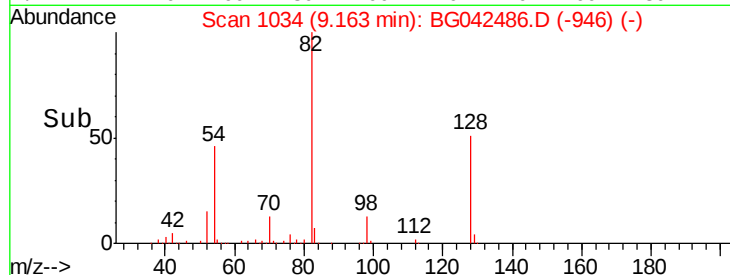
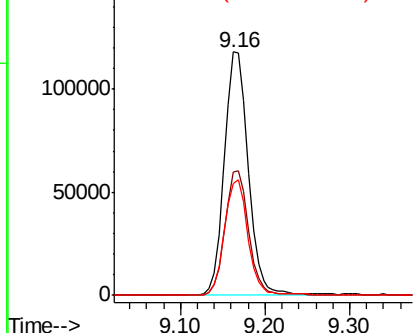



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1969
 Delta R.T. -0.01 min
 Lab File: BG042486.D
 Acq: 25 Aug 2019 20:15

Tgt Ion	164	Resp	137873
Ion Ratio	Lower	Upper	
164	100		
162	100.7	79.9	119.9
160	44.0	34.3	51.5

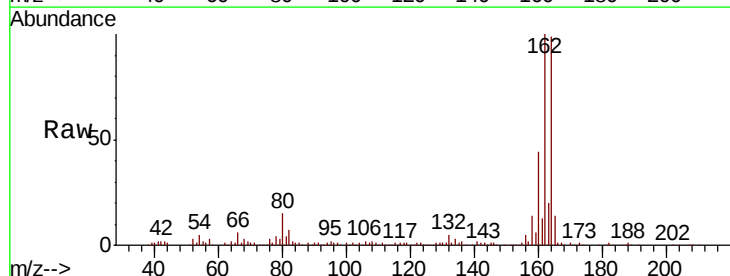

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

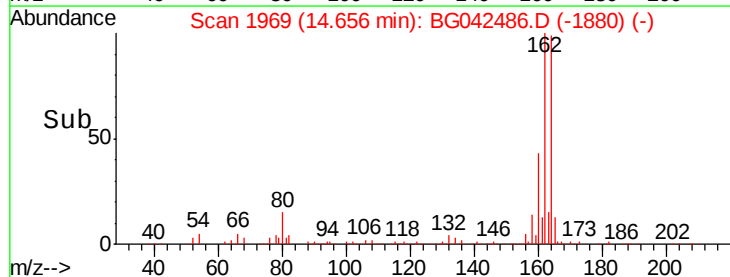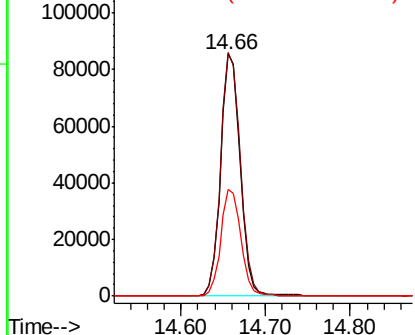

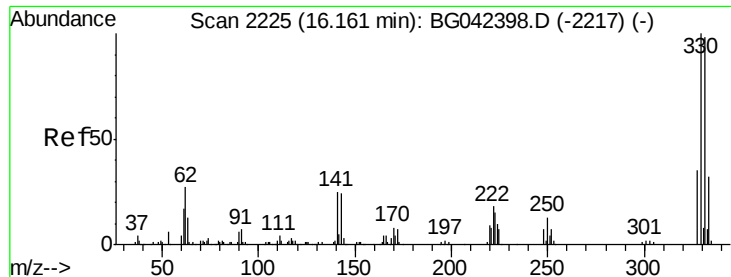

#42

2,4,6-Tribromophenol

Concen: 121.963 ng

RT: 16.15 min Scan# 2224

Delta R.T. -0.01 min

Lab File: BG042486.D

Acq: 25 Aug 2019 20:15

Instrument :

BNA_G

ClientSampleId :

B-1


Tot Ion:330 Resp: 239003

Ion Ratio Lower Upper




330 100

332 96.2 77.4 116.0

141 29.1 21.4 32.0

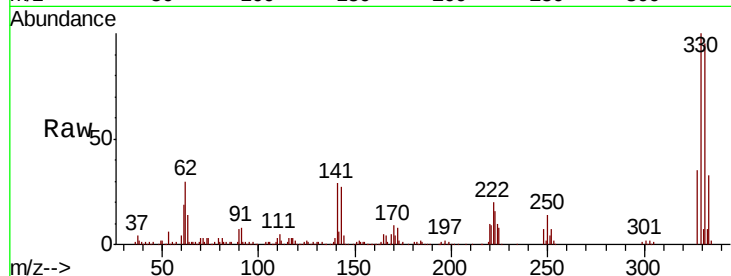

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

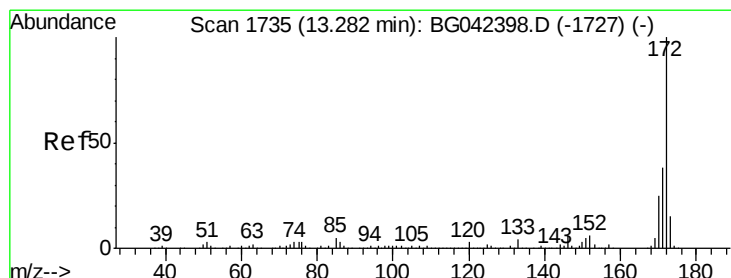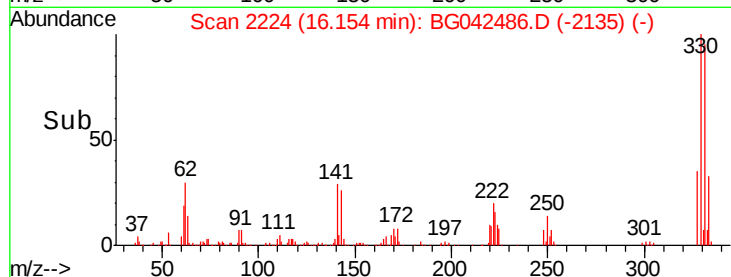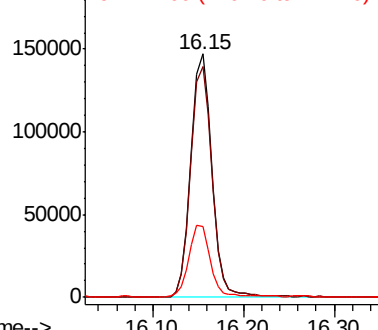

#45

2-Fluorobiphenyl

Concen: 86.882 ng

RT: 13.28 min Scan# 1734

Delta R.T. -0.01 min

Lab File: BG042486.D

Acq: 25 Aug 2019 20:15


Tgt Ion:172 Resp: 708262

Ion Ratio Lower Upper



172 100


171 38.3 30.5 45.7

170 24.6 20.2 30.2

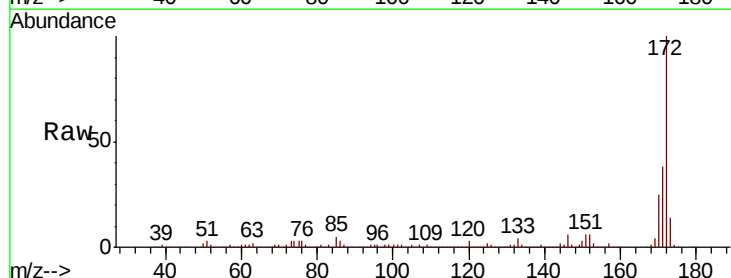

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

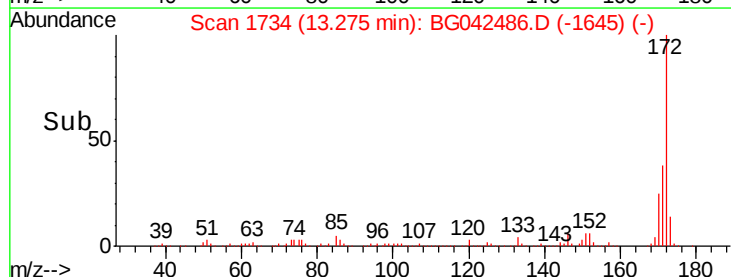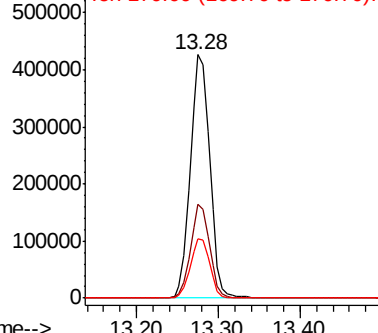

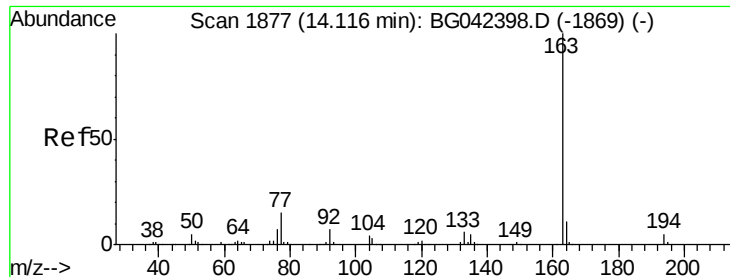

#50

Dimethylphthalate

Concen: 13.202 ng

RT: 14.10 min Scan# 1875

Delta R.T. -0.01 min

Lab File: BG042486.D

Acq: 25 Aug 2019 20:15

Instrument :

BNA_G

ClientSampled :

B-1


Tot Ion:163 Resp: 131334

Ion Ratio Lower Upper

163 100

194 5.4 4.2 6.2




164 11.2 8.8 13.2

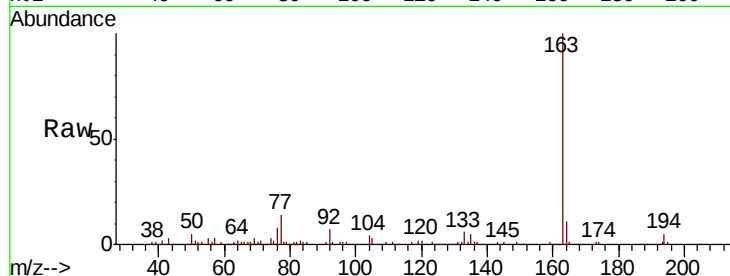

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

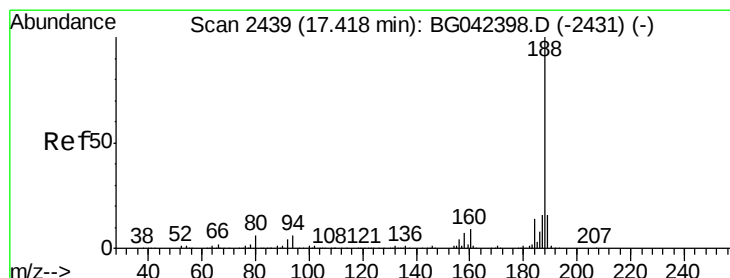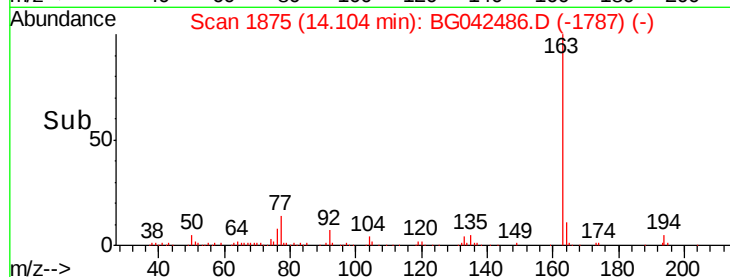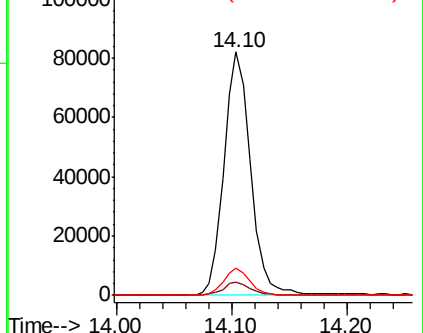

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2438

Delta R.T. -0.01 min

Lab File: BG042486.D

Acq: 25 Aug 2019 20:15


Tgt Ion:188 Resp: 332184

Ion Ratio Lower Upper

188 100

94 6.5 4.5 6.7



80 7.0 4.9 7.3

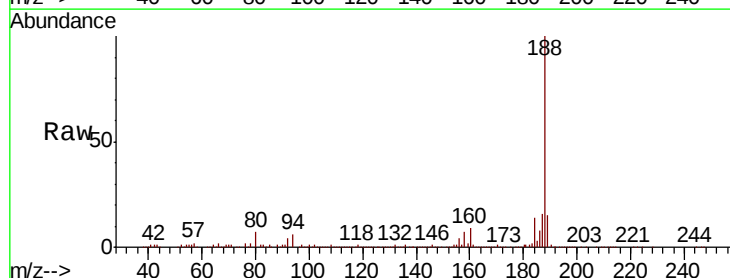


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



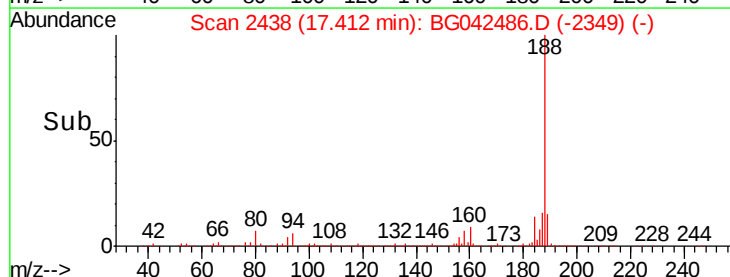
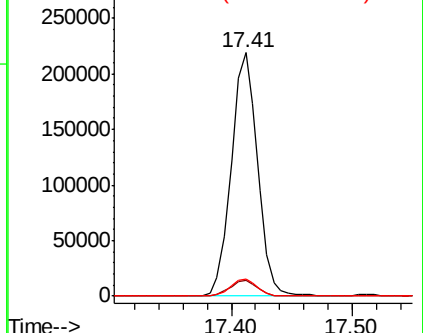


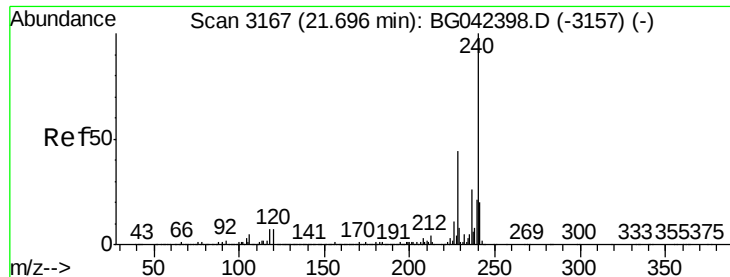

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.68 min Scan# 3165
 Delta R.T. -0.01 min
 Lab File: BG042486.D
 Acq: 25 Aug 2019 20:15




Instrument :
 BNA_G
 ClientSampled :
 B-1


Tot Ion	Ratio	Lower	Upper
240	100		
120	8.1	5.7	8.5
236	26.0	21.0	31.4

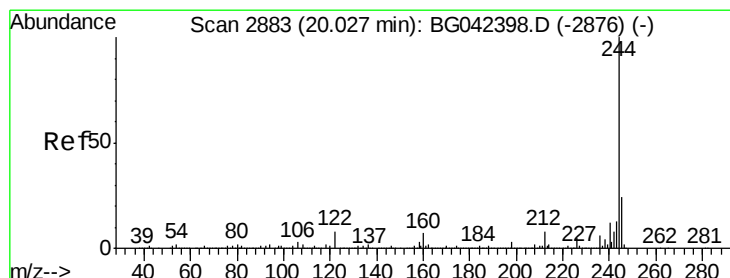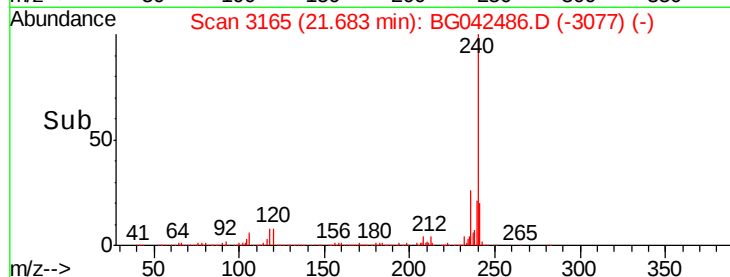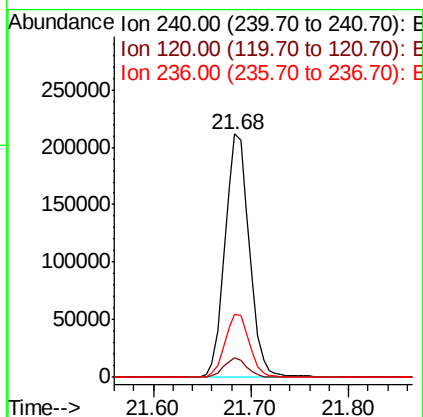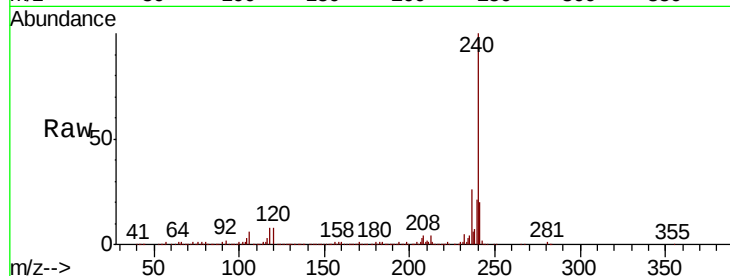

#79
 Terphenyl-d14
 Concen: 79.132 ng
 RT: 20.03 min Scan# 2883
 Delta R.T. -0.00 min
 Lab File: BG042486.D
 Acq: 25 Aug 2019 20:15

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.8	6.0	9.0
122	8.7	6.7	10.1

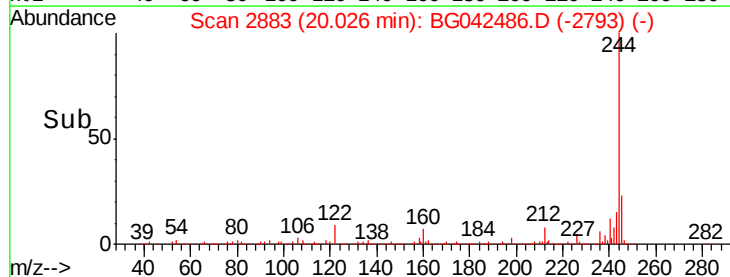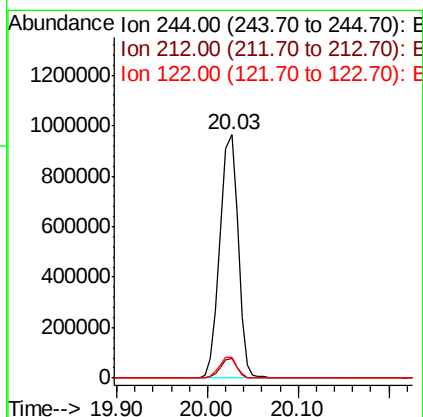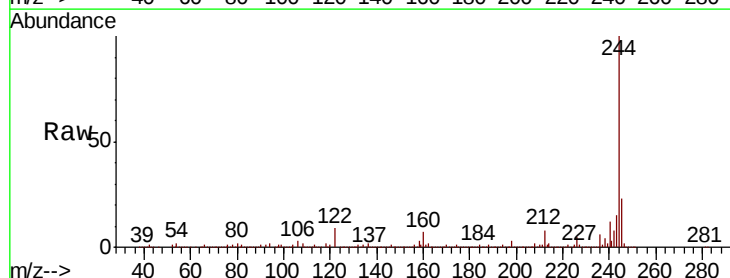

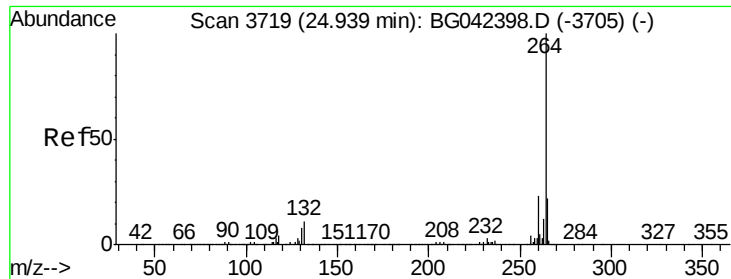

#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.93 min Scan# 3717
Delta R.T. -0.01 min
Lab File: BG042486.D
Acq: 25 Aug 2019 20:15

Instrument :
BNA_G
ClientSampleId :
B-1

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	18.5	27.7
265	21.7	17.6	26.4

