


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082519\
 Data File : BG042470.D
 Acq On : 25 Aug 2019 9:59
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 22 14:29:15 2019

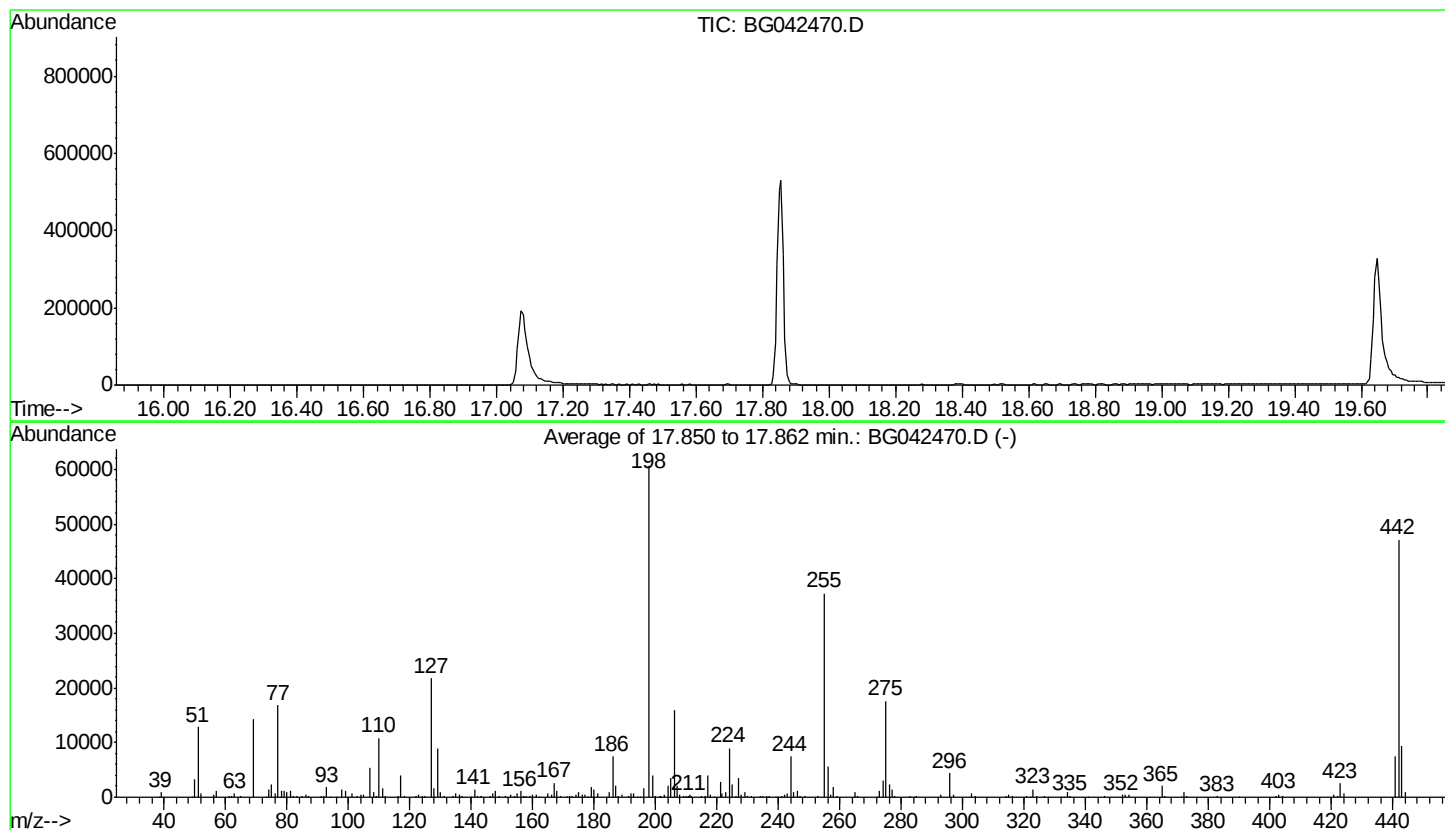

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	12865	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.5	14285	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.9	21780	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60669	PASS
199	198	5	9	6.7	4038	PASS
275	198	10	60	29.1	17663	PASS
365	198	1	100	3.4	2037	PASS
441	198	0.01	100	12.5	7580	PASS
442	198	50	100	77.7	47117	PASS
443	442	15	24	20.1	9455	PASS