
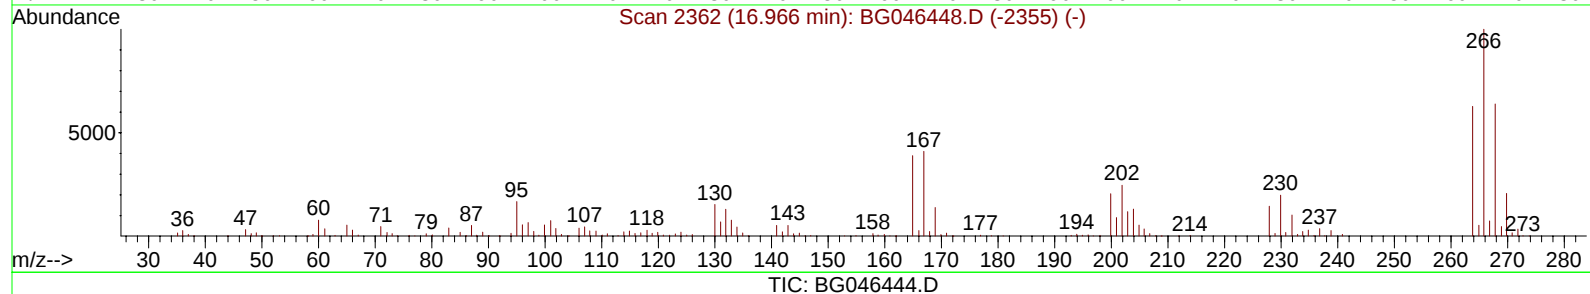
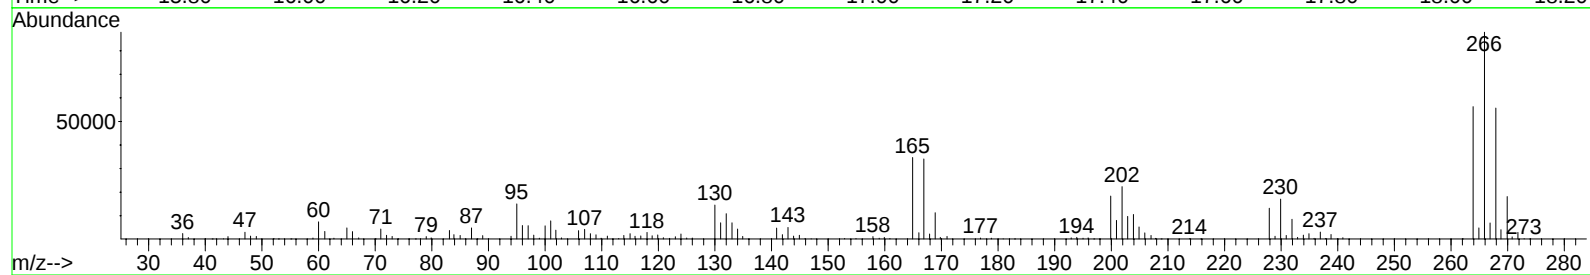


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082520\
Data File : BG046444.D
Acq On : 25 Aug 2020 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 18:43:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 25 18:00:34 2020
Response via : Initial Calibration

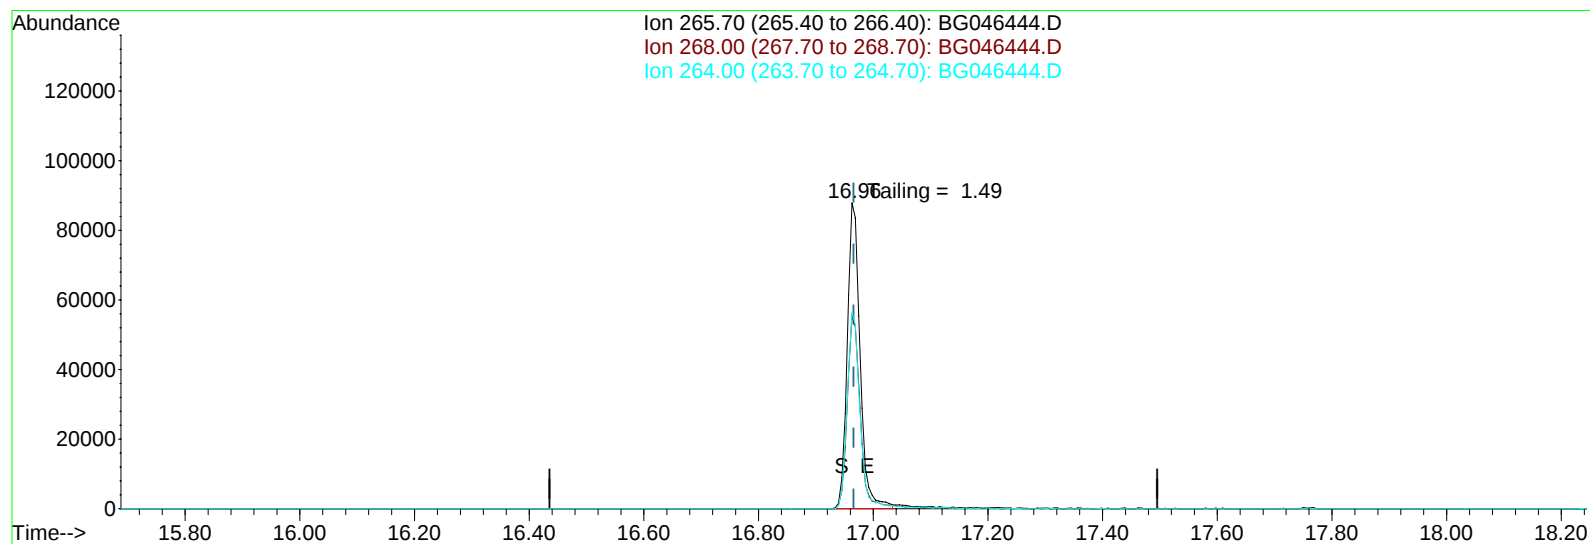

(70) Pentachlorophenol (C)




16.963min (-0.003) 33542.14ng

response 139032

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.39
264.00	62.70	64.11
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG082520\
Data File : BG046444.D
Acq On : 25 Aug 2020 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 18:43:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 25 18:00:34 2020
Response via : Initial Calibration

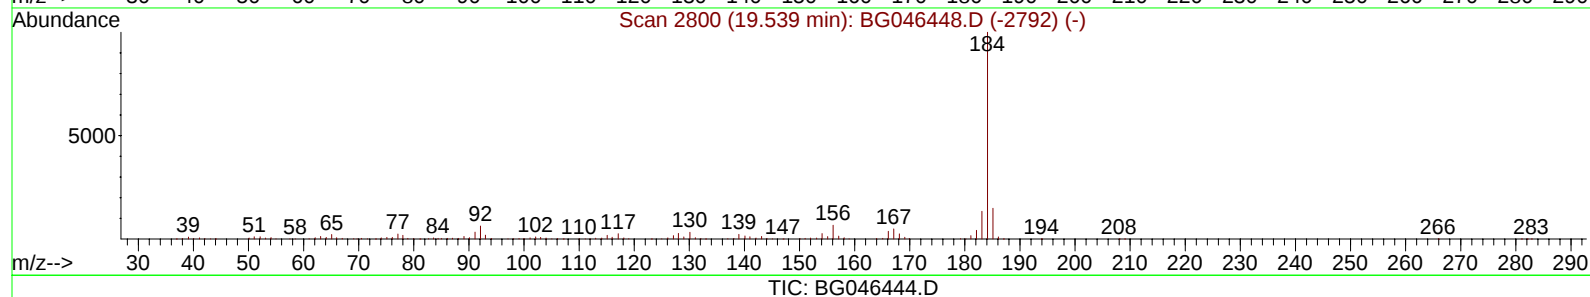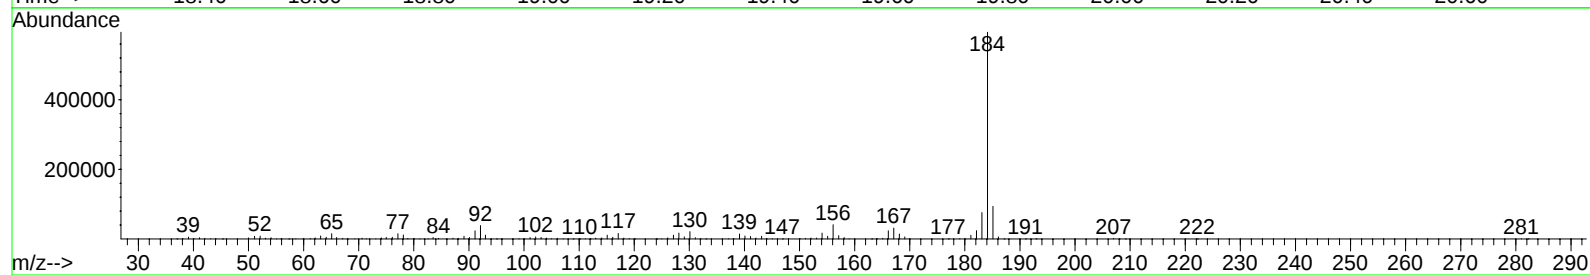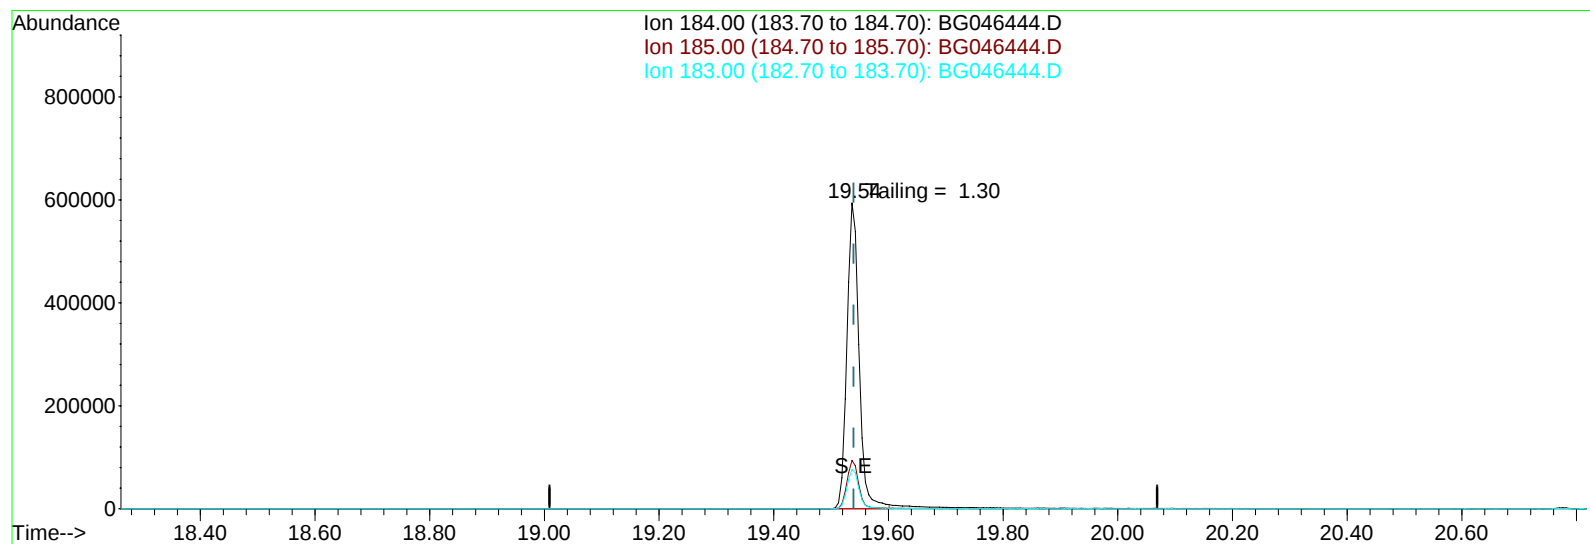

(77) Benzidine

19.536min (-0.003) 0.00ng

response 900300

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.80
183.00	13.40	12.82
0.00	0.00	0.00