


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082520\
 Data File : BG046444.D
 Acq On : 25 Aug 2020 9:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 25 18:00:34 2020

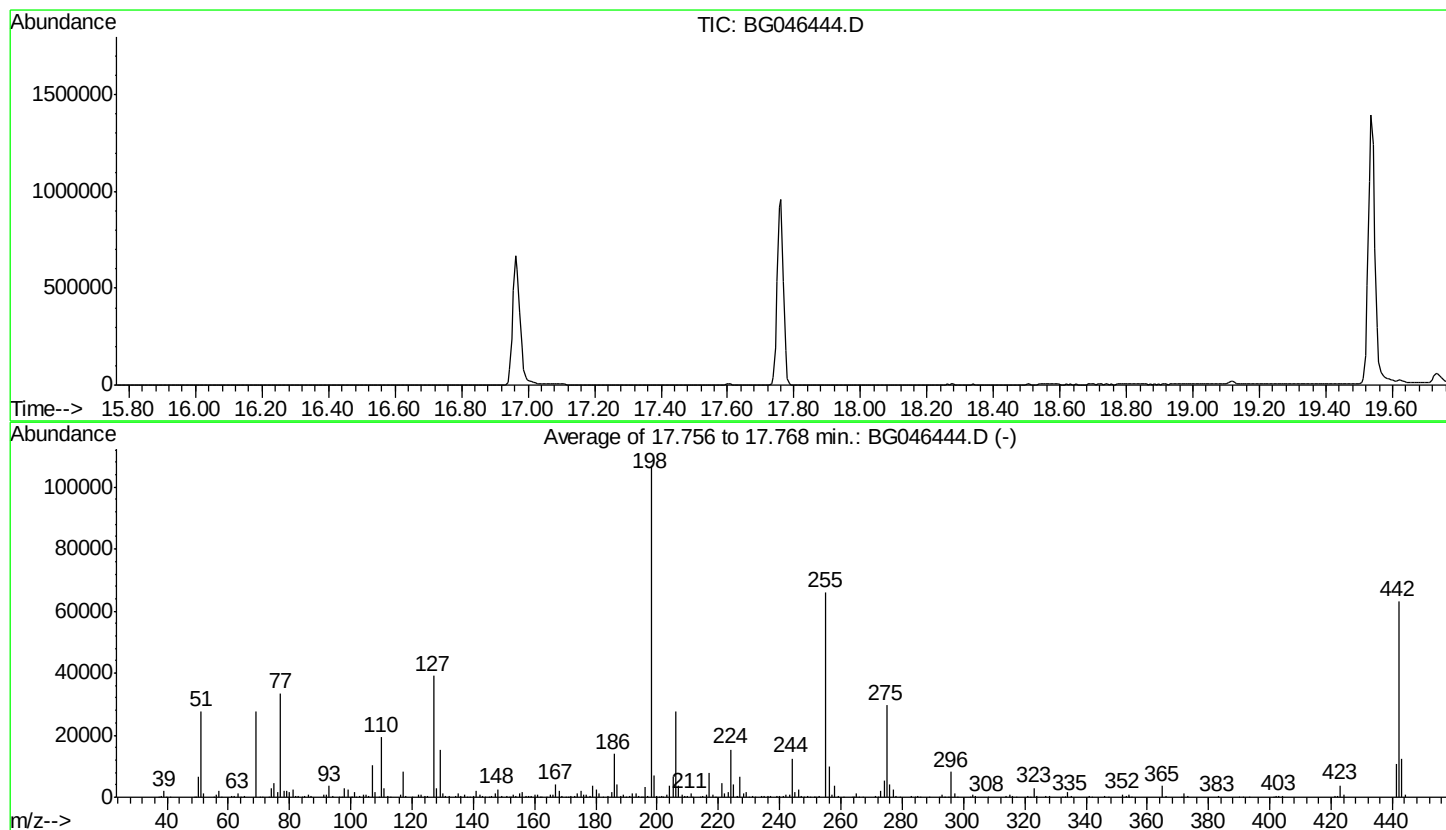

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	27491	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.7	27515	PASS
70	69	0.00	2	0.2	60	PASS
127	198	10	80	36.7	39184	PASS
197	198	0.00	2	0.3	351	PASS
198	198	100	100	100.0	106906	PASS
199	198	5	9	6.6	7006	PASS
275	198	10	60	27.7	29589	PASS
365	198	1	100	3.5	3705	PASS
441	198	0.01	100	9.9	10541	PASS
442	198	50	100	59.0	63029	PASS
443	442	15	24	19.8	12495	PASS