
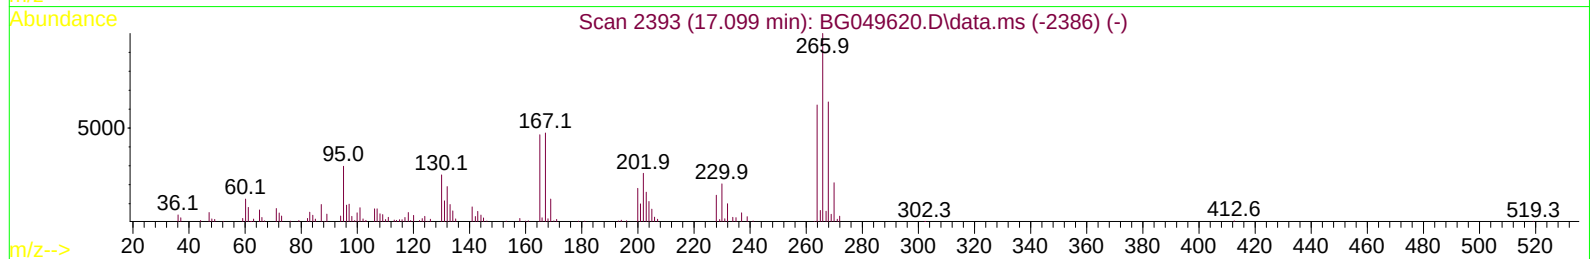
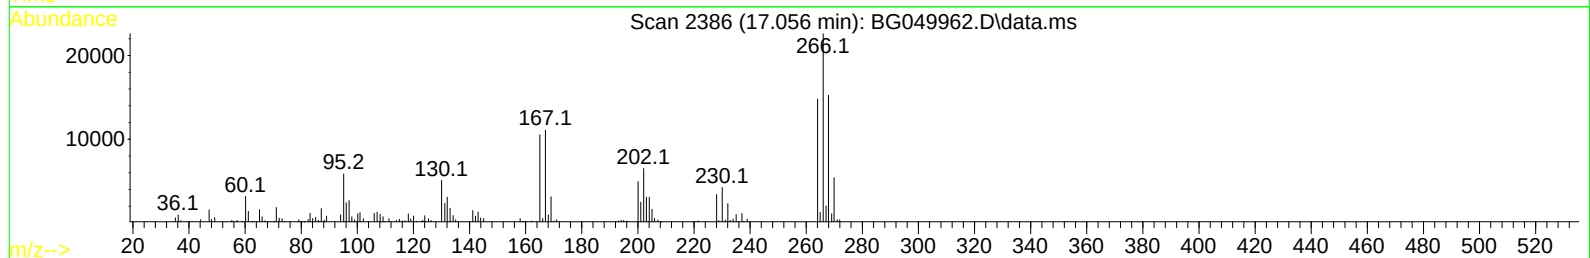


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
Data File : BG049962.D
Acq On : 25 Aug 2021 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 11:53:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 16:13:24 2021
Response via : Initial Calibration

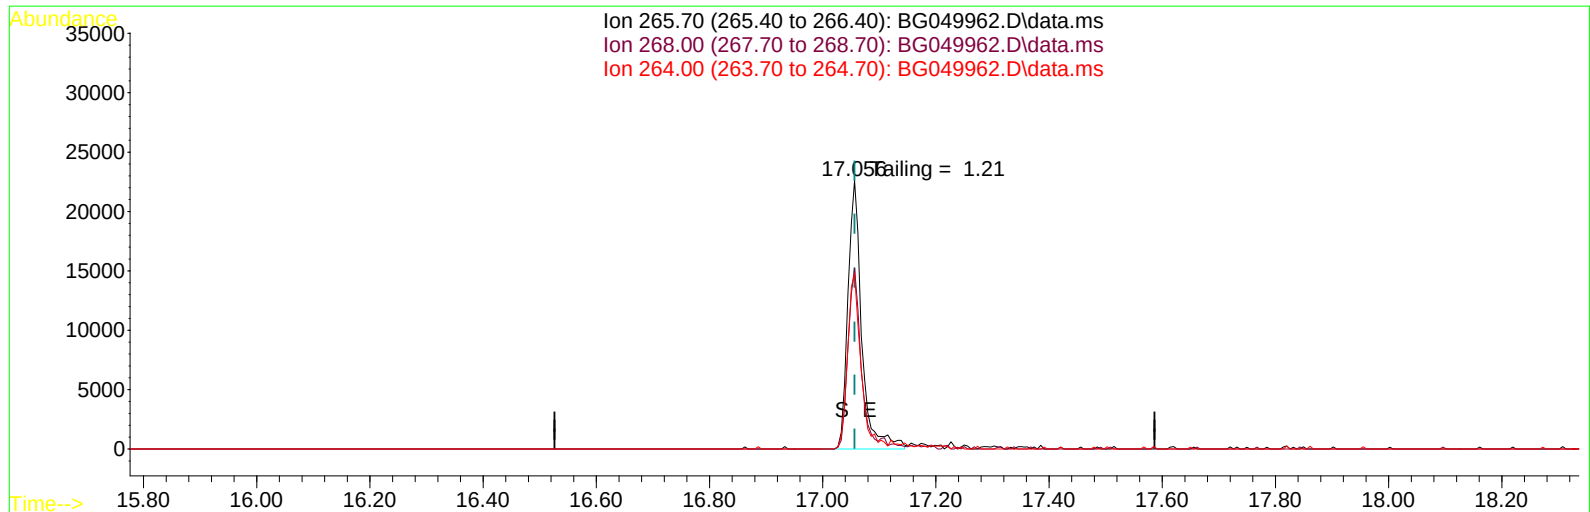

TIC: BG049962.D\data.ms

(70) Pentachlorophenol (C)




17.056min (+ 0.000) 18377.91 ng

response 38554

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.46
264.00	61.30	65.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
Data File : BG049962.D
Acq On : 25 Aug 2021 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 11:53:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 16:13:24 2021
Response via : Initial Calibration

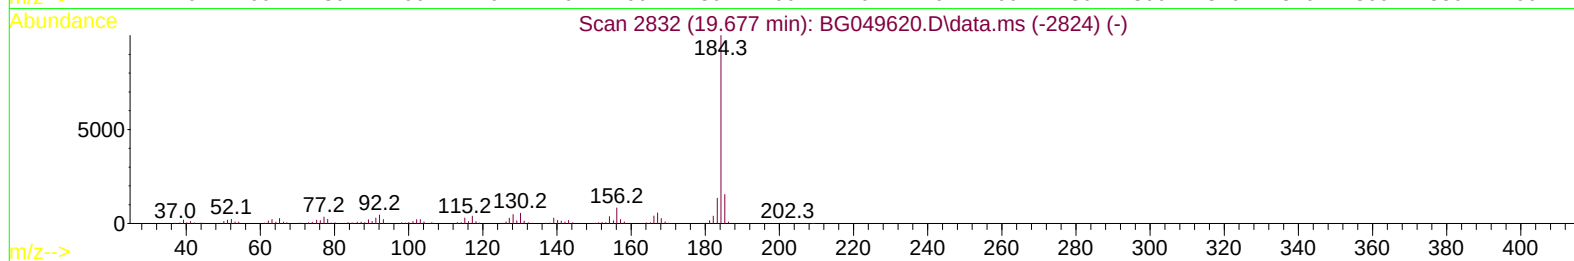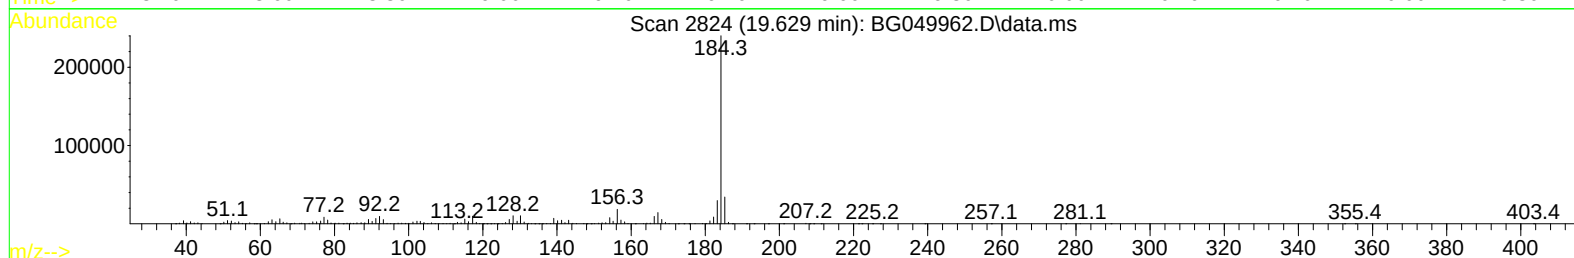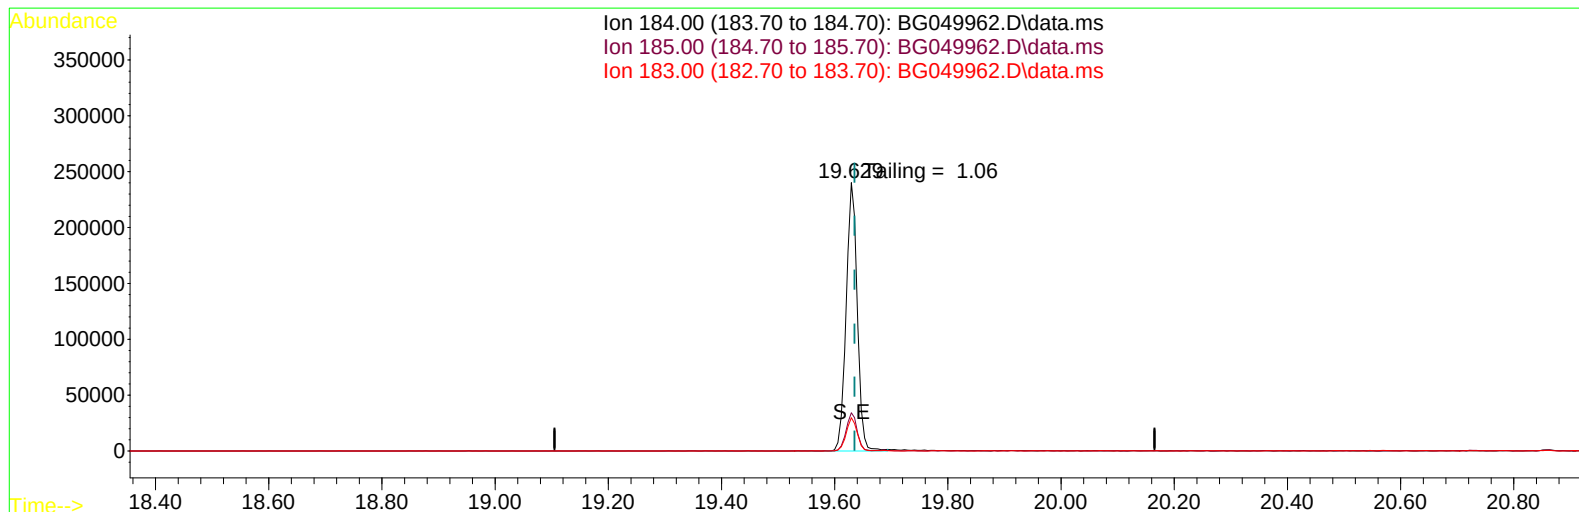

TIC: BG049962.D\data.ms

(77) Benzidine**19.629min (-0.006) 103814.00 ng****response 327172**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.25
183.00	11.70	12.42
0.00	0.00	0.00