

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
 Data File : BG049970.D
 Acq On : 25 Aug 2021 16:12
 Operator : CG/JU
 Sample : M3533-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-02-0824-21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.531	417	424	436	rBV	449187	742165	51.67%	8.383%
2	7.153	692	700	711	rBV	465580	833156	58.01%	9.411%
3	7.975	834	840	847	rVB2	122148	202638	14.11%	2.289%
4	9.150	1032	1040	1049	rVB	296746	534869	37.24%	6.041%
5	10.566	1274	1281	1288	rBV3	12778	25176	1.75%	0.284%
6	10.795	1312	1320	1327	rBV	161064	290196	20.20%	3.278%
7	13.250	1731	1738	1748	rBV	780061	1214062	84.53%	13.713%
8	14.637	1967	1974	1980	rBV	250763	392351	27.32%	4.432%
9	16.129	2222	2228	2240	rVB	648148	978918	68.16%	11.057%
10	17.386	2436	2442	2447	rBV	279069	435026	30.29%	4.914%
11	17.427	2447	2449	2455	rVB	33653	46157	3.21%	0.521%
12	17.521	2460	2465	2470	rVB2	12218	17289	1.20%	0.195%
13	18.267	2586	2592	2594	rBV5	12680	17711	1.23%	0.200%
14	18.314	2597	2600	2605	rVB4	13558	18352	1.28%	0.207%
15	18.467	2620	2626	2629	rBV4	15374	30238	2.11%	0.342%
16	19.183	2741	2748	2750	rBV5	15726	28479	1.98%	0.322%
17	19.324	2767	2772	2777	rBV8	12907	25244	1.76%	0.285%
18	19.442	2787	2792	2799	rBV	157036	227241	15.82%	2.567%
19	19.771	2844	2848	2849	rBV	27484	30288	2.11%	0.342%
20	19.806	2850	2854	2862	rVB	153672	229166	15.96%	2.588%
21	20.000	2881	2887	2892	rBV	1119438	1436301	100.00%	16.223%
22	20.640	2993	2996	3001	rBV7	18040	32485	2.26%	0.367%
23	21.292	3104	3107	3112	rBV6	27484	37353	2.60%	0.422%
24	21.662	3163	3170	3175	rBV2	256025	502128	34.96%	5.672%
25	21.704	3175	3177	3184	rVB	61412	95972	6.68%	1.084%
26	23.877	3542	3547	3553	rBV2	37233	76832	5.35%	0.868%
27	24.899	3714	3721	3730	rVB3	133338	353636	24.62%	3.994%


Sum of corrected areas: 8853429

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
Data File : BG049970.D
Acq On : 25 Aug 2021 16:12
Operator : CG/JU
Sample : M3533-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-02-0824-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

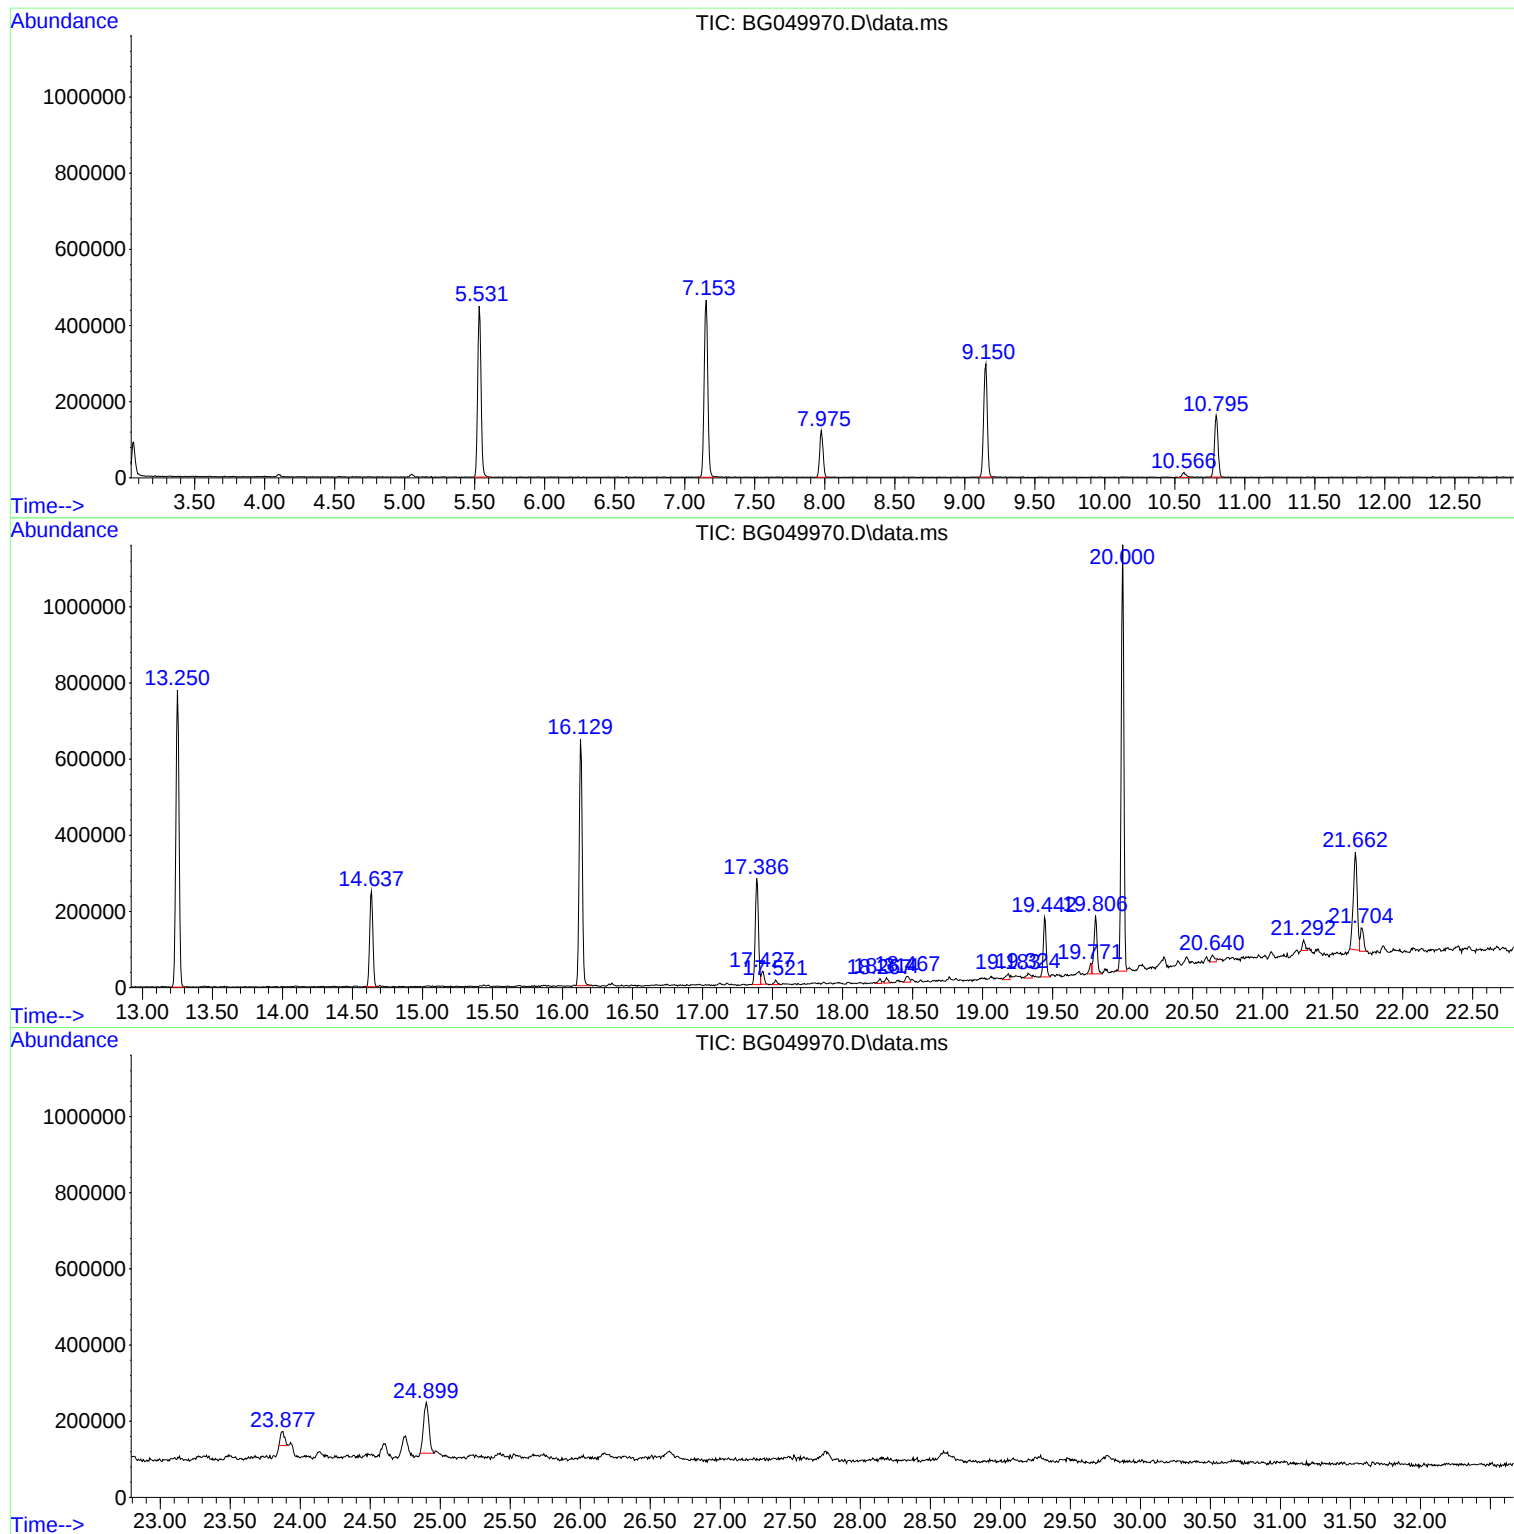

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
Data File : BG049970.D
Acq On : 25 Aug 2021 16:12
Operator : CG/JU
Sample : M3533-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-02-0824-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
Data File : BG049970.D
Acq On : 25 Aug 2021 16:12
Operator : CG/JU
Sample : M3533-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-02-0824-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------