
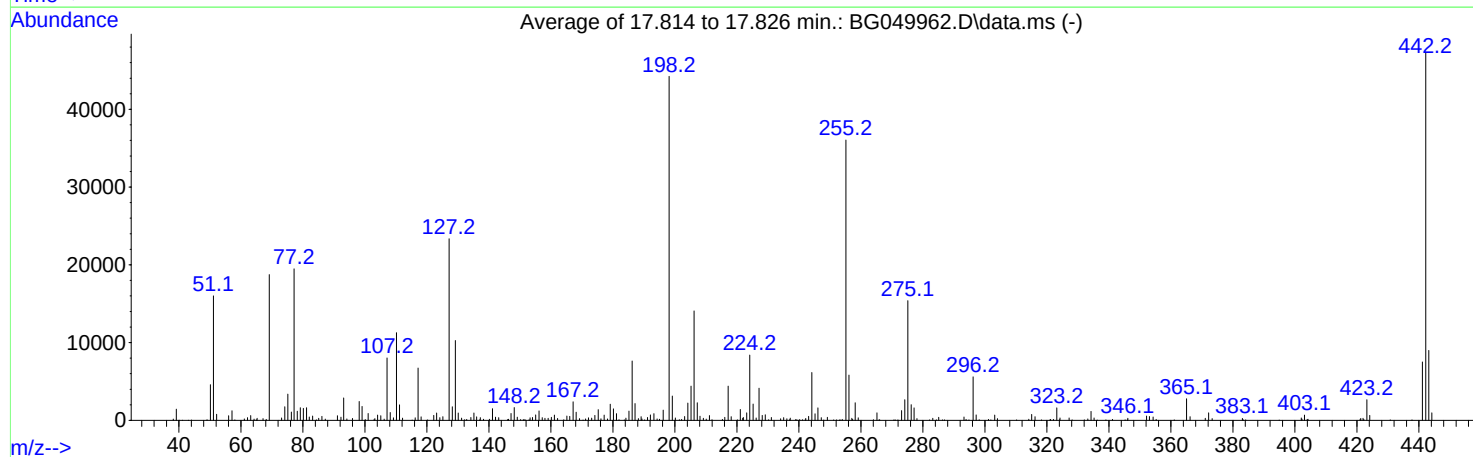


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
 Data File : BG049962.D
 Acq On : 25 Aug 2021 9:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 23 16:13:24 2021

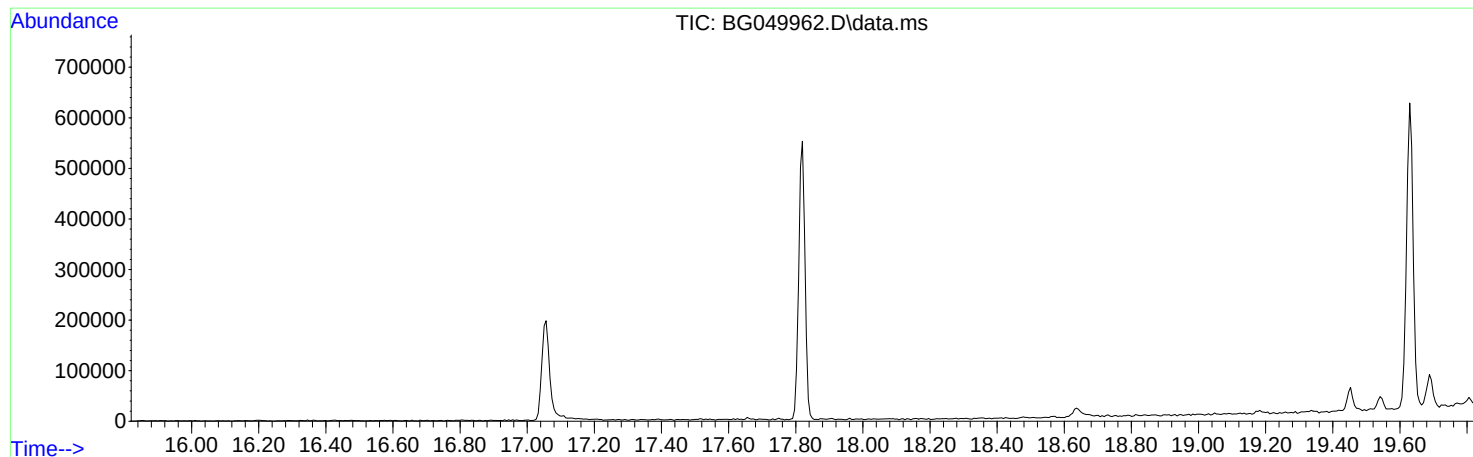




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	16012	PASS
68	69	0.00	2	0.7	128	PASS
69	198	0.00	100	42.4	18751	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.8	23347	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44232	PASS
199	198	5	9	7.1	3127	PASS
275	198	10	60	34.8	15391	PASS
365	198	1	100	6.3	2773	PASS
441	198	0.01	100	17.0	7509	PASS
442	442	50	100	100.0	47307	PASS
443	442	15	24	19.0	8986	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
Data File : BG049962.D
Acq On : 25 Aug 2021 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 25 11:53:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 16:13:24 2021
Response via : Initial Calibration

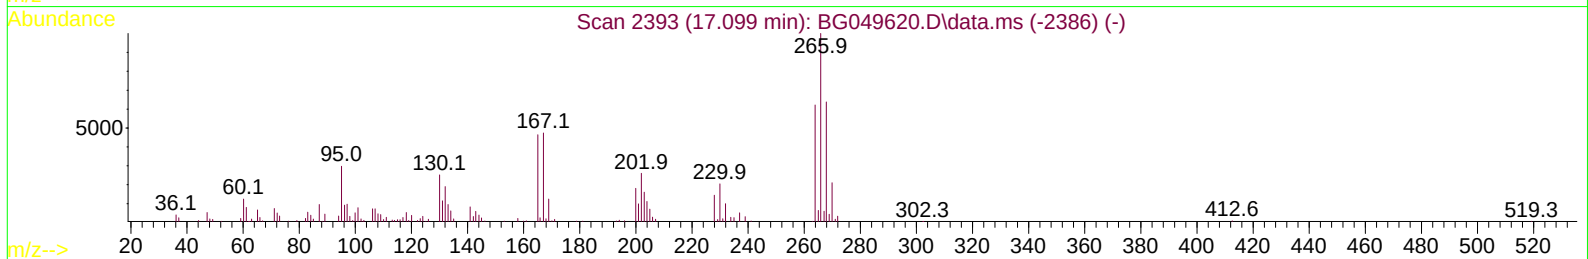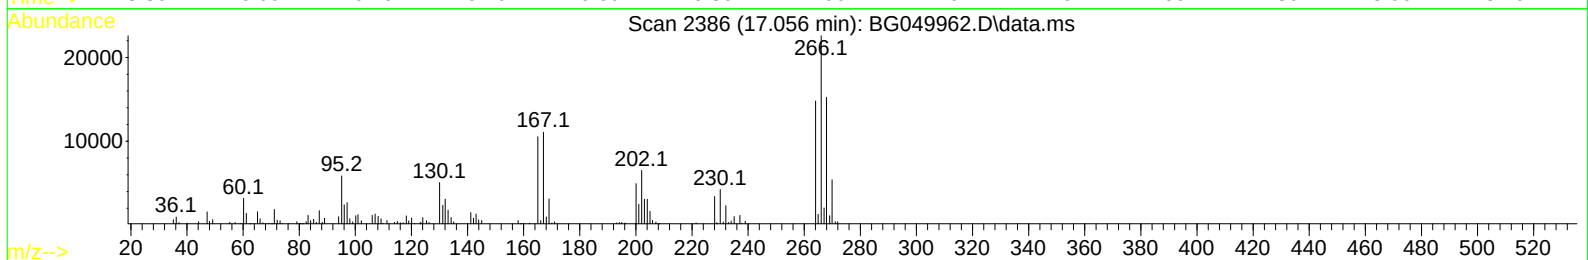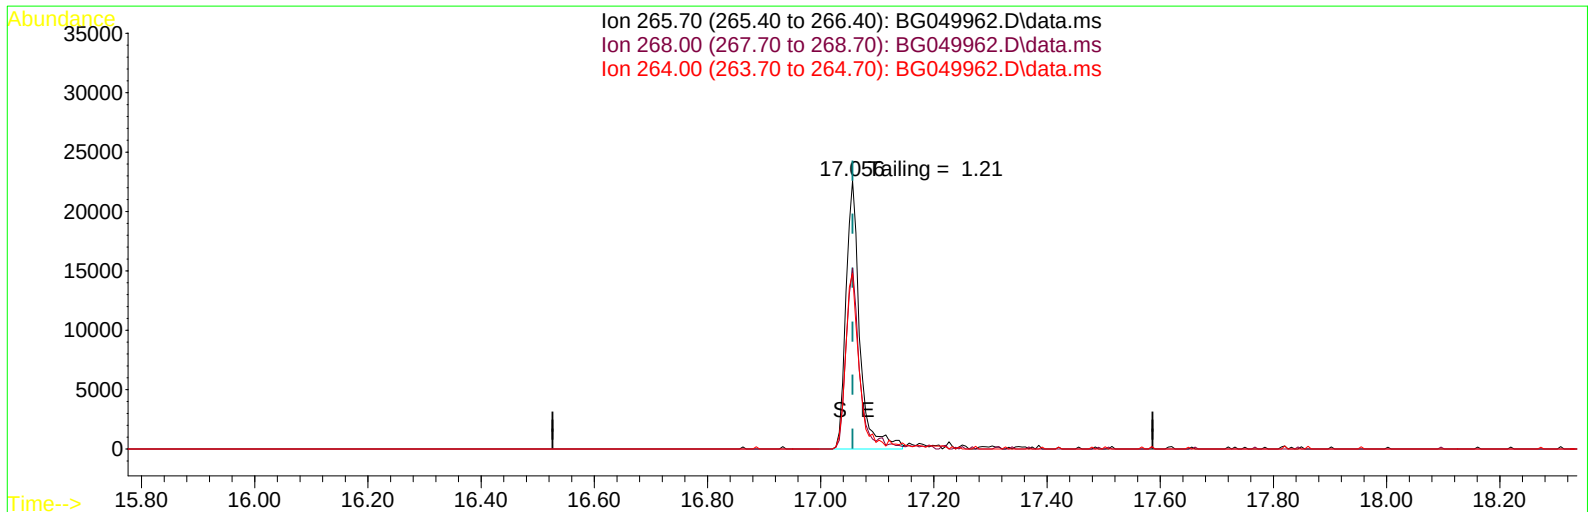

TIC: BG049962.D\data.ms

(70) Pentachlorophenol (C)

17.056min (+ 0.000) 18377.91 ng




response 38554

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	67.46
264.00	61.30	65.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082521\
 Data File : BG049962.D
 Acq On : 25 Aug 2021 9:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 11:53:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 16:13:24 2021
 Response via : Initial Calibration

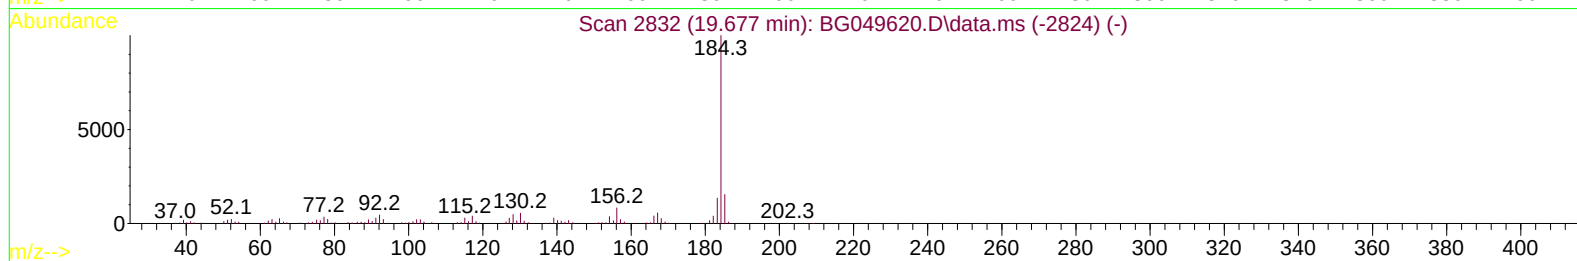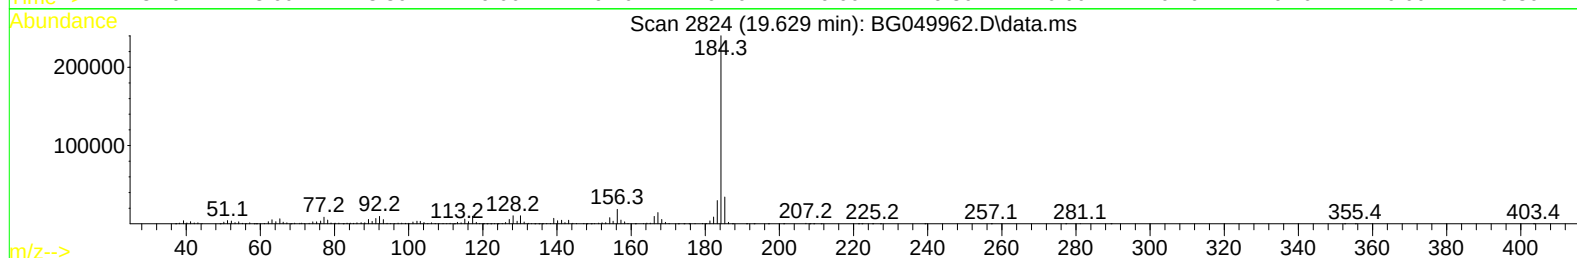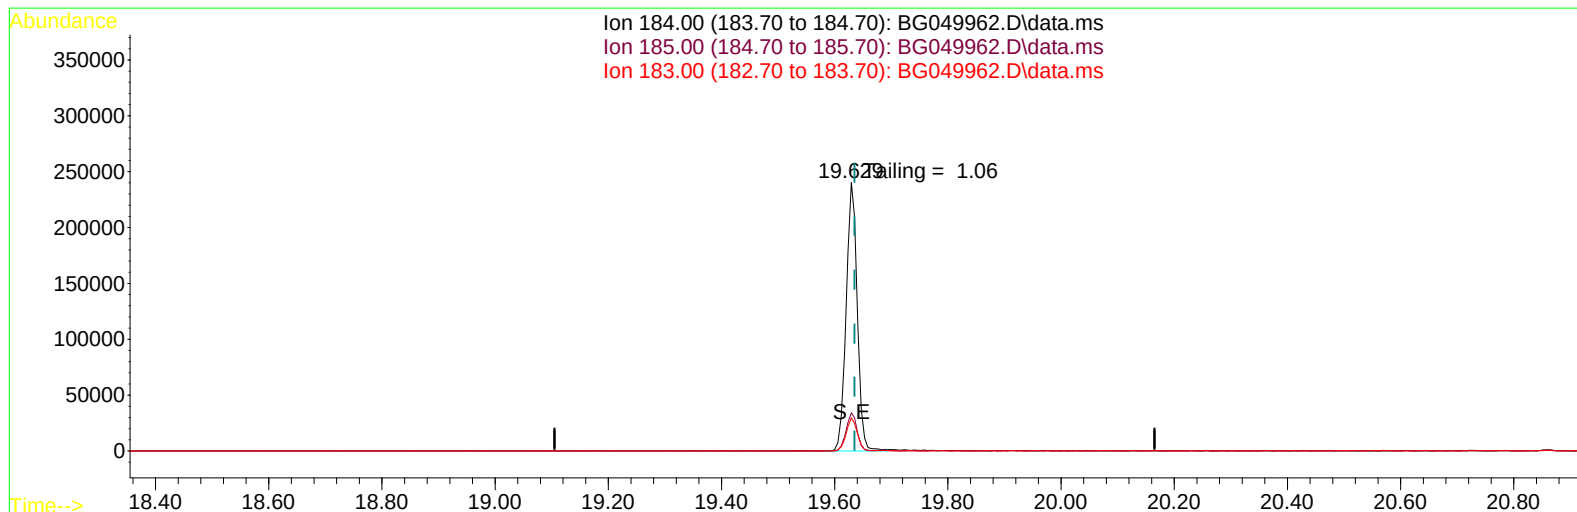

TIC: BG049962.D\data.ms

(77) Benzidine

19.629min (-0.006) 103814.00 ng

response 327172

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.25
183.00	11.70	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2021	BNA_G	BG049962.D
Compound Name	Response	Retention Time
DDT	156891	20.85
DDD	3847	20.42
DDE	472	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4319	161210	2.68

Instrument :
BNA_G
ClientSampleId :
DFTPP