

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082619\
 Data File : BG042492.D
 Acq On : 26 Aug 2019 9:55
 Operator : HP/JU
 Sample : PB122510TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB122510TB

Quant Time: Aug 27 01:04:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	53211	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	205159	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	142527	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	317351	20.00	ng	0.00
76) Chrysene-d12	21.69	240	365851	20.00	ng	0.00
87) Perylene-d12	24.93	264	429705	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	315398	120.05	ng	0.00
7) Phenol-d6	7.17	99	410751	115.74	ng	0.00
23) Nitrobenzene-d5	9.17	82	234008	78.82	ng	0.00
42) 2,4,6-Tribromophenol	16.15	330	197590	97.54	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	716621	85.04	ng	0.00
79) Terphenyl-d14	20.03	244	1268936	74.99	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.16	70	29237	12.716	ng	# 73
51) 2,6-Dinitrotoluene	14.66	165	18824	7.897	ng	# 36
57) 2,4-Dinitrotoluene	14.66	165	18824	5.515	ng	# 38
67) 4-Bromophenyl-phenylether	16.15	248	12847	3.191	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082619\
Data File : BG042492.D
Acq On : 26 Aug 2019 9:55
Operator : HP/JU
Sample : PB122510TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122510TB

Quant Time: Aug 27 01:04:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

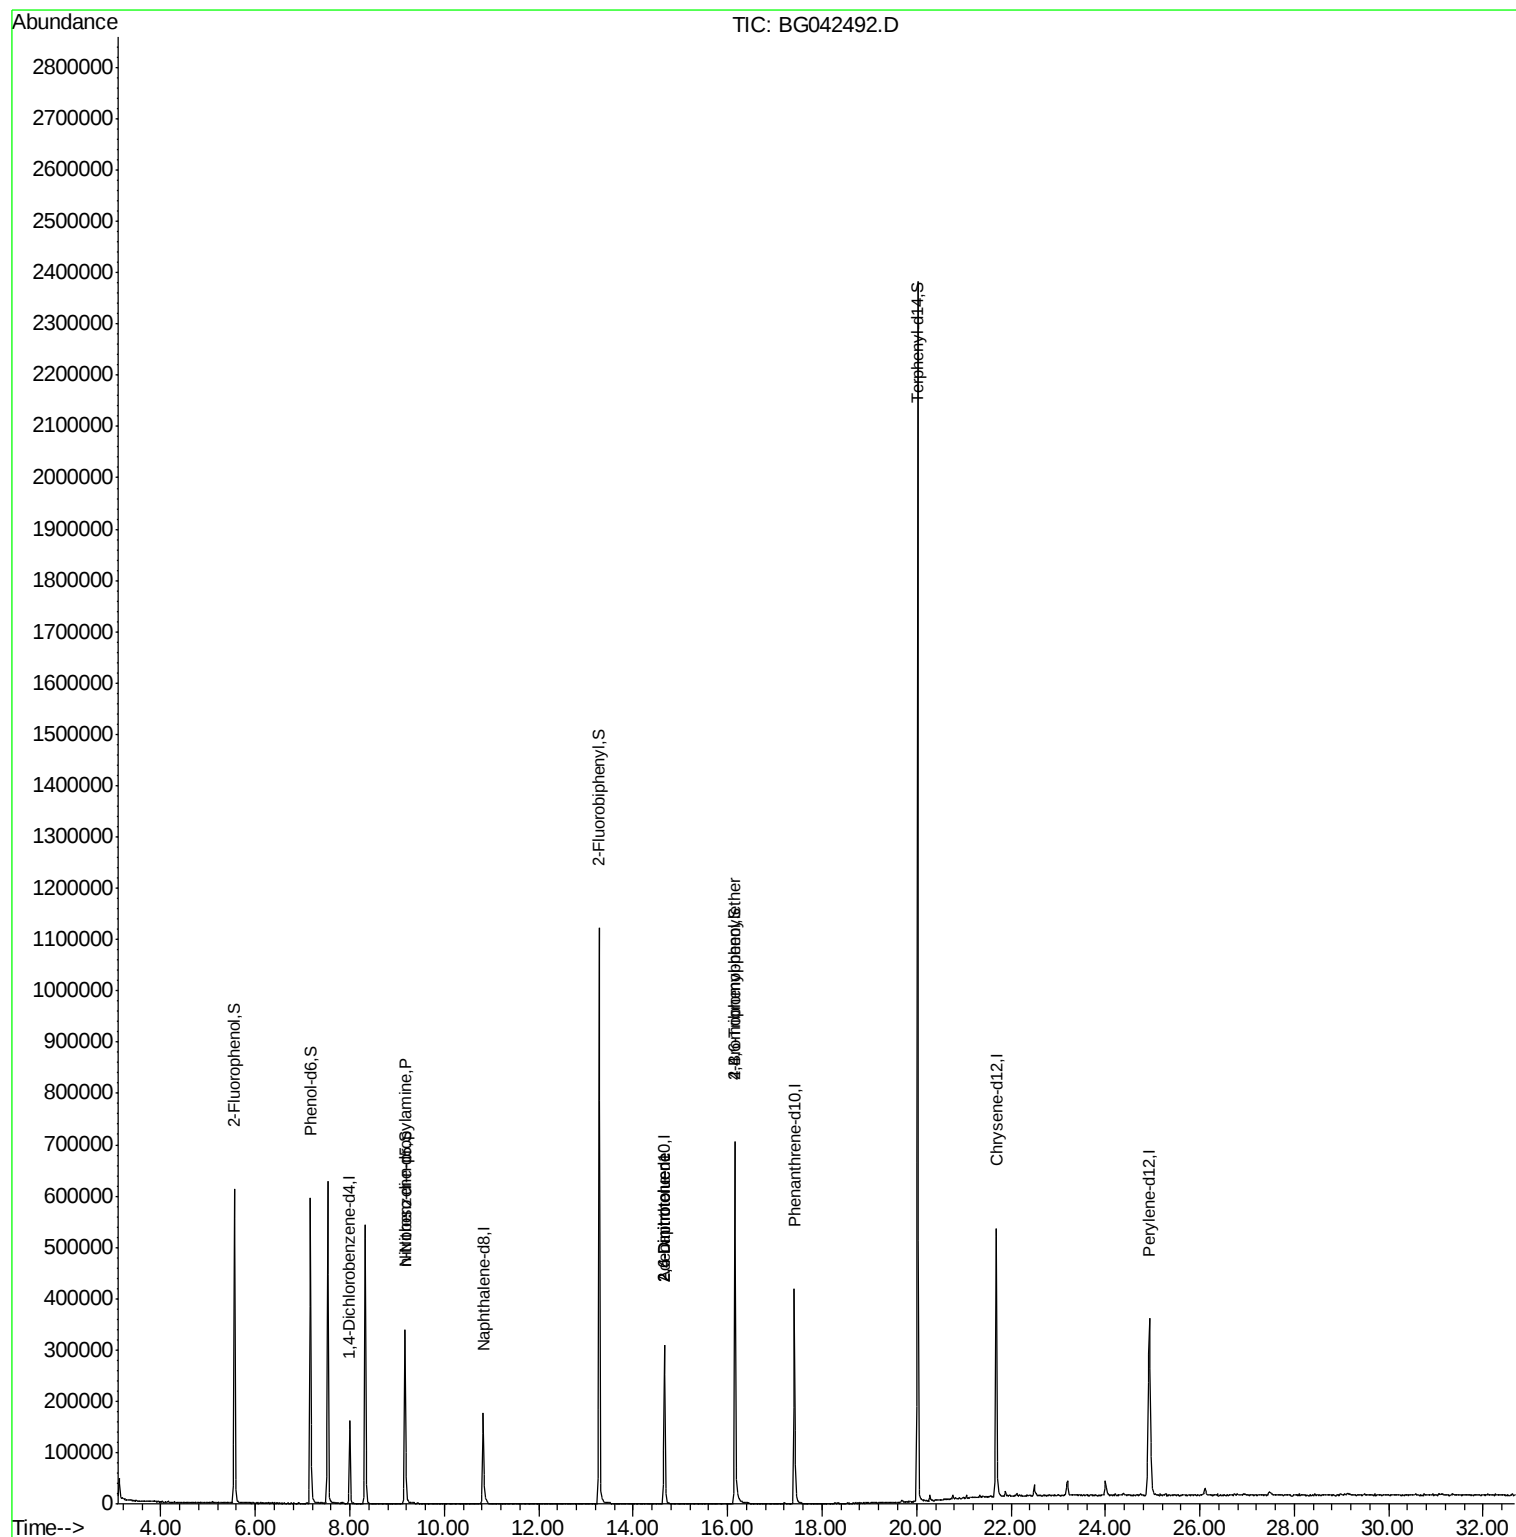




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.00 min Scan# 836
Delta R.T. -0.01 min
Lab File: BG042492.D
Acq: 26 Aug 2019 9:55

Instrument :
BNA_G
ClientSampleId :
PB122510TB

Tgt Ion:152 Resp: 53211
Ion Ratio Lower Upper
152 100
150 159.0 125.4 188.0
115 49.7 38.5 57.7




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

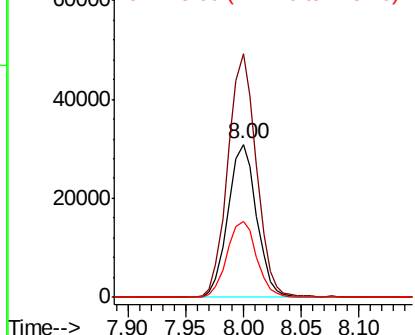



#5


2-Fluorophenol
Concen: 120.045 ng
RT: 5.56 min Scan# 420
Delta R.T. -0.01 min
Lab File: BG042492.D
Acq: 26 Aug 2019 9:55

Tgt Ion:112 Resp: 315398
Ion Ratio Lower Upper
112 100
64 56.5 42.8 64.2
63 29.3 22.7 34.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

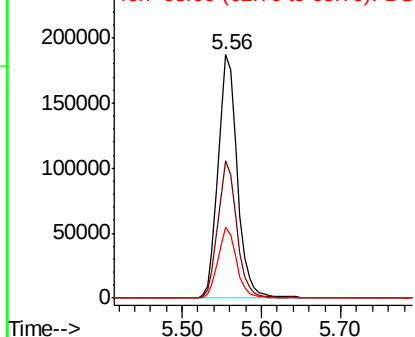

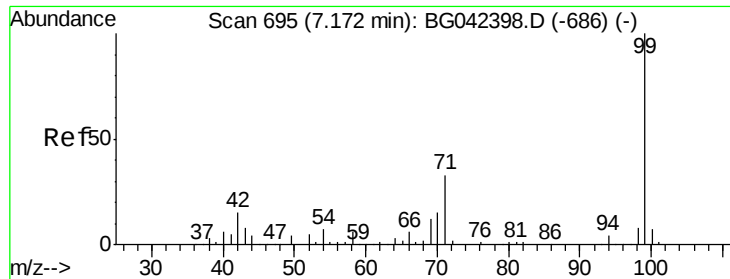

#7

Phenol-d6

Concen: 115.740 ng

RT: 7.17 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG042492.D

Acq: 26 Aug 2019 9:55

Instrument :

BNA_G

ClientSampleId :

PB122510TB


Tgt Ion: 99 Resp: 410751

Ion Ratio Lower Upper




99 100

42 13.6 12.0 18.0

71 31.9 26.3 39.5

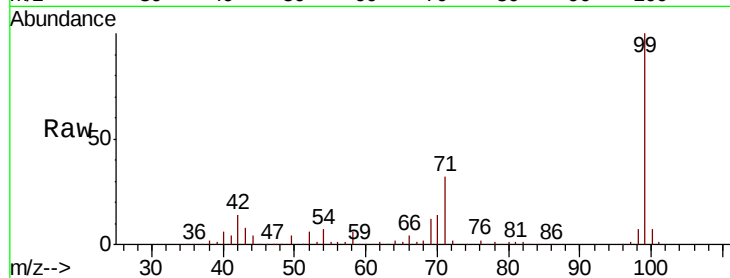

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

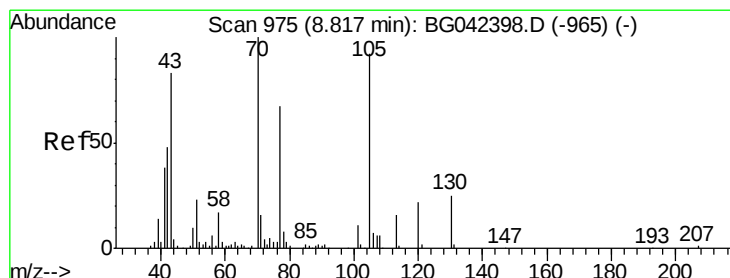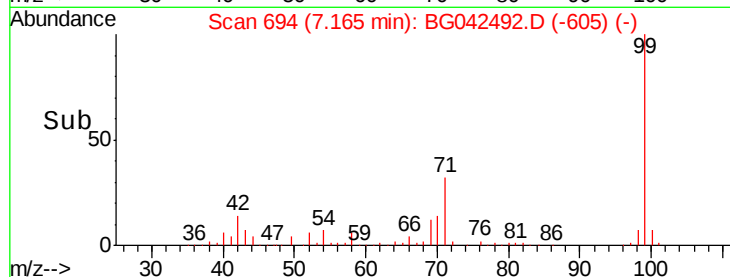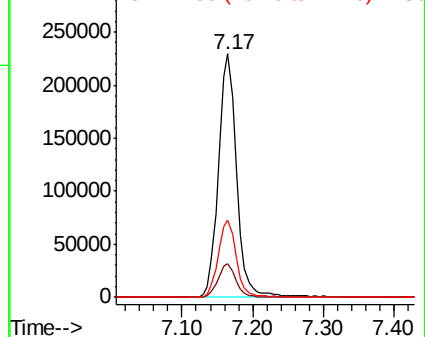

#19

n-Nitroso-di-n-propylamine

Concen: 12.716 ng

RT: 9.16 min Scan# 1034

Delta R.T. 0.35 min

Lab File: BG042492.D

Acq: 26 Aug 2019 9:55

Tgt Ion: 70 Resp: 29237


Ion Ratio Lower Upper

70 100



42 36.5 38.8 58.2#


101 0.0 9.0 13.6#

130 2.9 20.0 30.0#

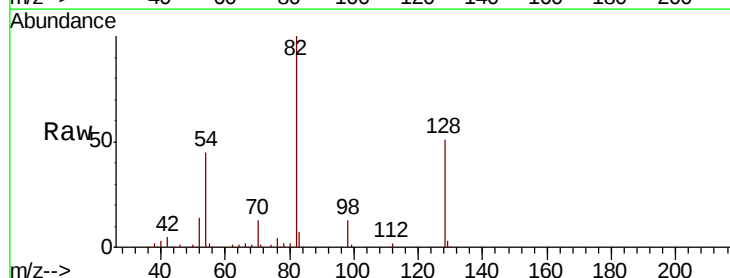

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

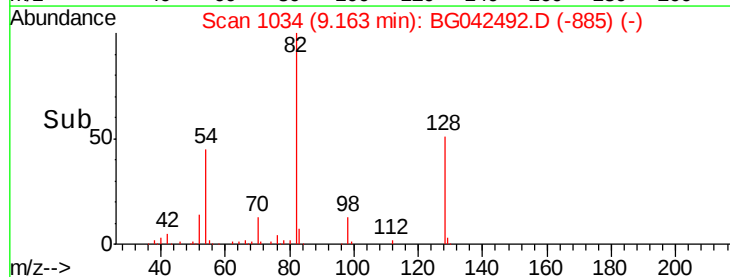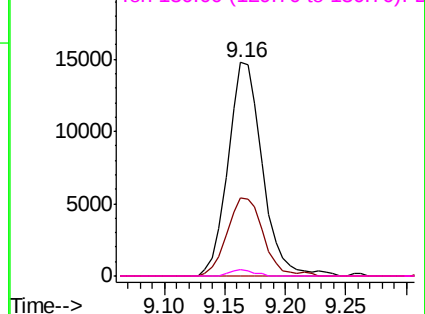







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.82 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BG042492.D
Acq: 26 Aug 2019 9:55

Instrument :
BNA_G
ClientSampleId :
PB122510TB

Tgt Ion:	136	Resp:	205159
Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.7	13.1
54	6.9	4.9	7.3
68	4.8	3.6	5.4

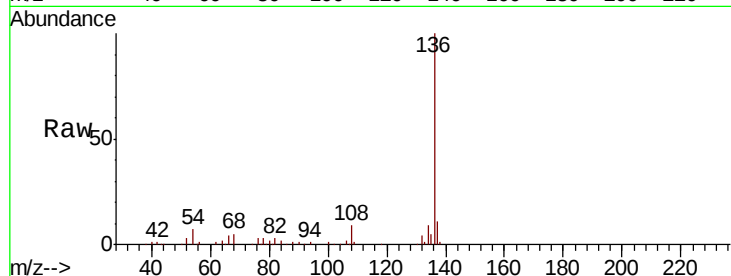


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

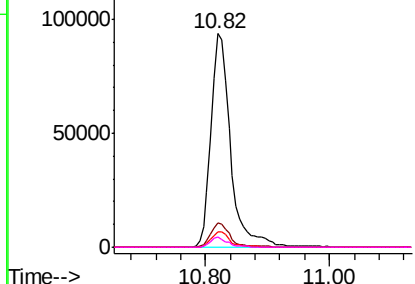




#23
Nitrobenzene-d5
Concen: 78.821 ng
RT: 9.17 min Scan# 1035
Delta R.T. -0.01 min
Lab File: BG042492.D
Acq: 26 Aug 2019 9:55

Tgt Ion:	82	Resp:	234008
Ion	Ratio	Lower	Upper
82	100		
128	50.0	40.7	61.1
54	47.0	36.3	54.5



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

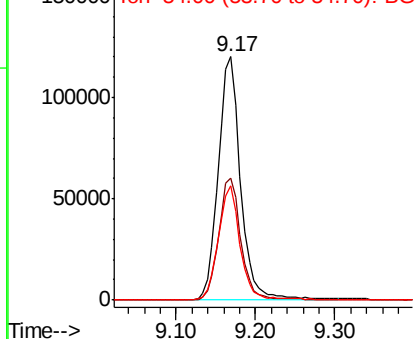

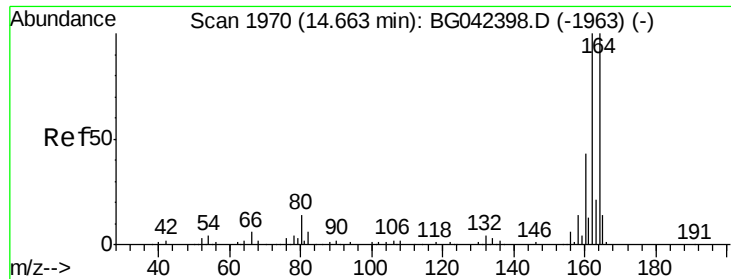

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.66 min Scan# 1970

Delta R.T. -0.00 min

Lab File: BG042492.D

Acq: 26 Aug 2019 9:55

Instrument :

BNA_G

ClientSampleId :

PB122510TB


Tgt Ion:164 Resp: 142527

Ion Ratio Lower Upper

164 100

162 98.7 79.9 119.9




160 42.6 34.3 51.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

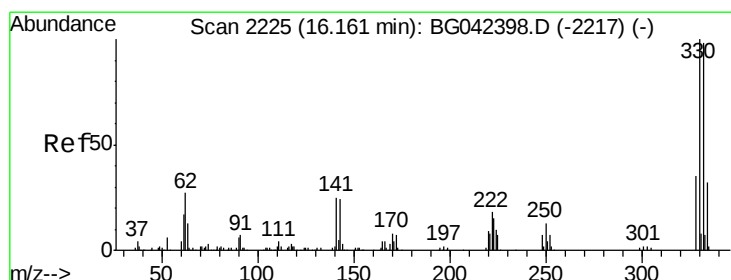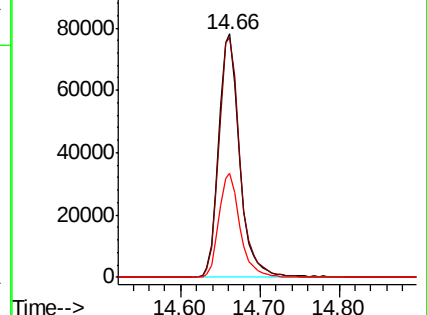

#42

2,4,6-Tribromophenol

Concen: 97.537 ng

RT: 16.15 min Scan# 2224

Delta R.T. -0.01 min

Lab File: BG042492.D

Acq: 26 Aug 2019 9:55


Tgt Ion:330 Resp: 197590

Ion Ratio Lower Upper

330 100

332 96.5 77.4 116.0



141 28.4 21.4 32.0

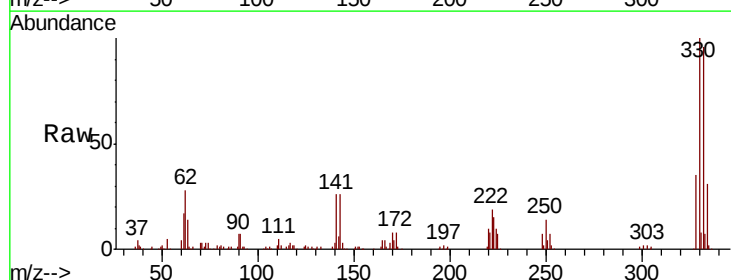


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



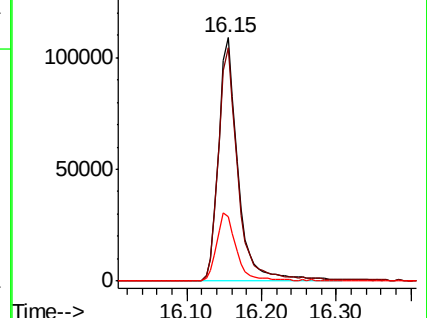
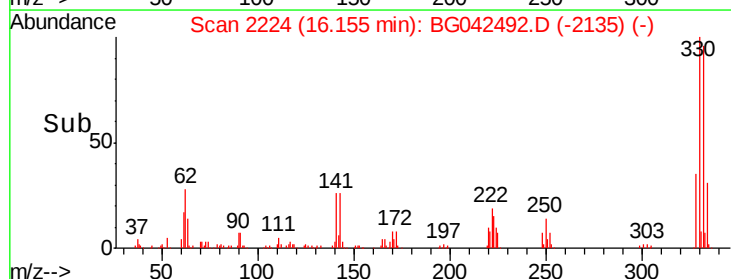




#45
 2-Fluorobiphenyl
 Concen: 85.037 ng
 RT: 13.28 min Scan# 1734
 Delta R.T. -0.01 min
 Lab File: BG042492.D
 Acq: 26 Aug 2019 9:55




Instrument :
 BNA_G
 ClientSampleId :
 PB122510TB


Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	30.5	45.7
170	23.8	20.2	30.2

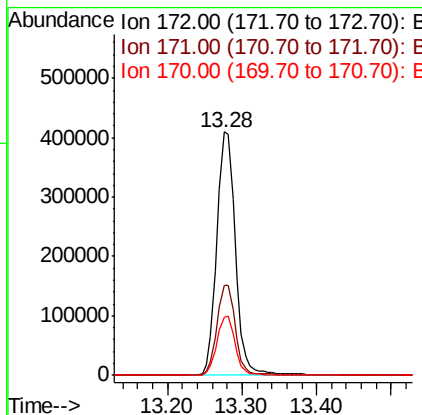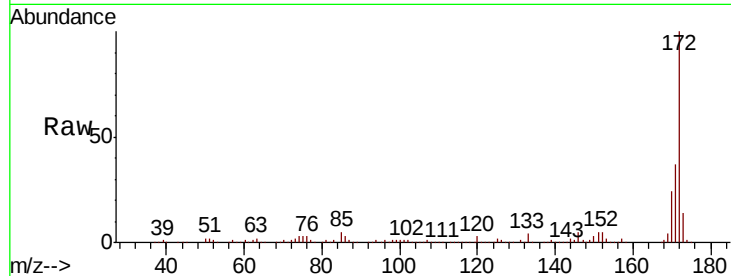

#51
 2,6-Dinitrotoluene
 Concen: 7.897 ng
 RT: 14.66 min Scan# 1970
 Delta R.T. 0.43 min
 Lab File: BG042492.D
 Acq: 26 Aug 2019 9:55

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	30.6	45.8#
89	0.0	32.6	49.0#

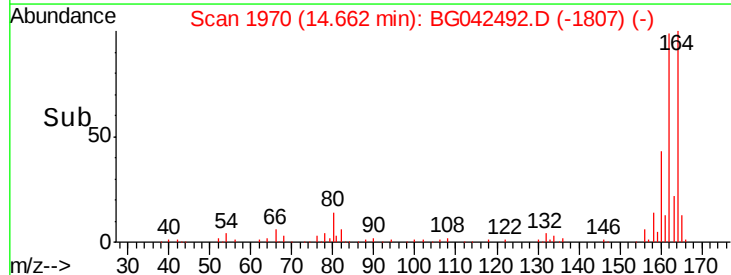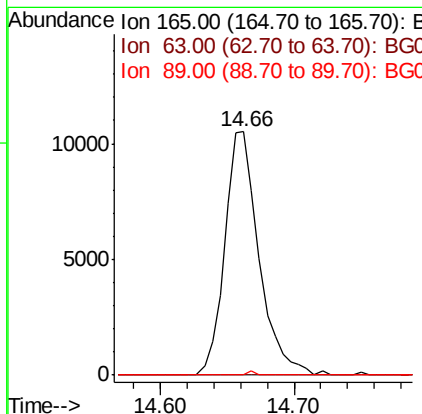


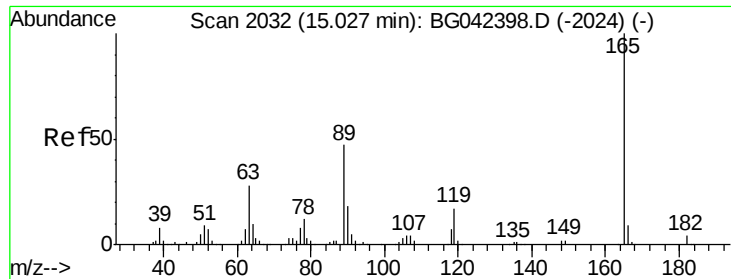




#57
 2,4-Dinitrotoluene
 Concen: 5.515 ng
 RT: 14.66 min Scan# 1970
 Delta R.T. -0.36 min
 Lab File: BG042492.D
 Acq: 26 Aug 2019 9:55

Instrument :
 BNA_G
 ClientSampleId :
 PB122510TB

Tgt Ion:	165	Resp:	18824
Ion	Ratio	Lower	Upper
165	100		
63	0.0	22.5	33.7#
89	0.0	37.8	56.6#
182	0.0	3.0	4.4#

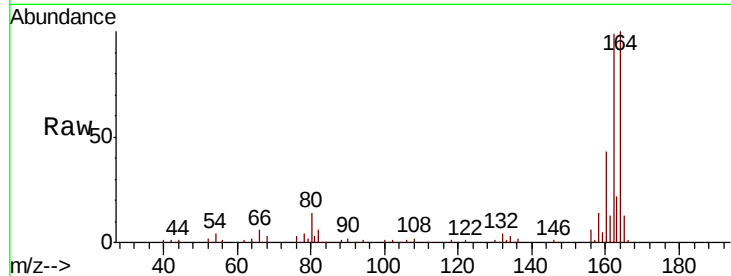


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

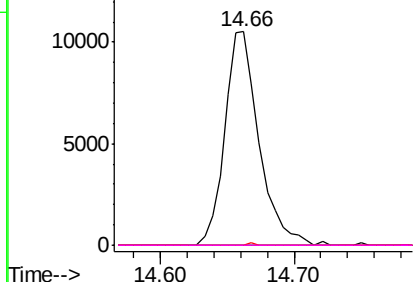




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.41 min Scan# 2438
 Delta R.T. -0.01 min
 Lab File: BG042492.D
 Acq: 26 Aug 2019 9:55

Tgt Ion:	188	Resp:	317351
Ion	Ratio	Lower	Upper
188	100		
94	6.3	4.5	6.7
80	7.0	4.9	7.3



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

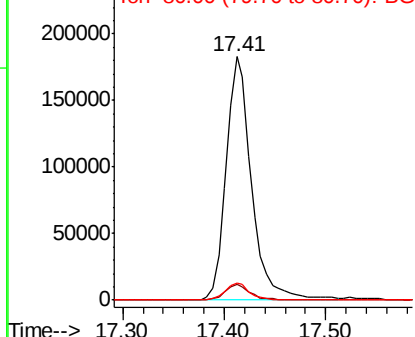


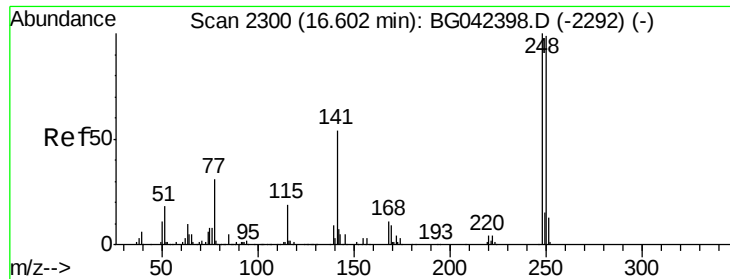




#67
 4-Bromophenyl-phenylether
 Concen: 3.191 ng
 RT: 16.15 min Scan# 2224
 Delta R.T. -0.45 min
 Lab File: BG042492.D
 Acq: 26 Aug 2019 9:55

Instrument :
 BNA_G
 ClientSampleId :
 PB122510TB

Tgt Ion:248 Resp: 12847
 Ion Ratio Lower Upper
 248 100
 250 206.6 78.9 118.3#
 141 399.6 43.3 64.9#

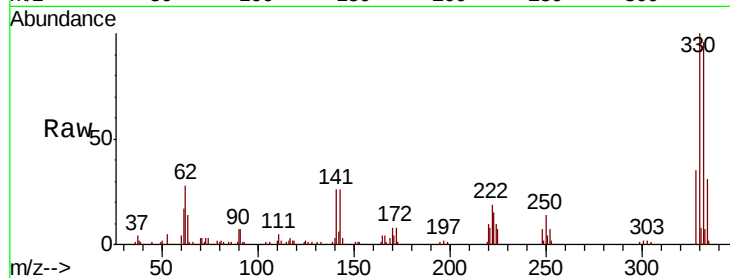


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

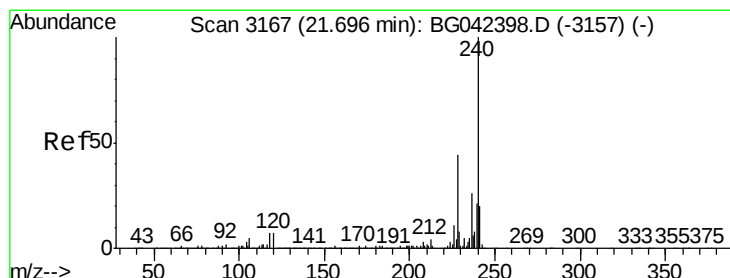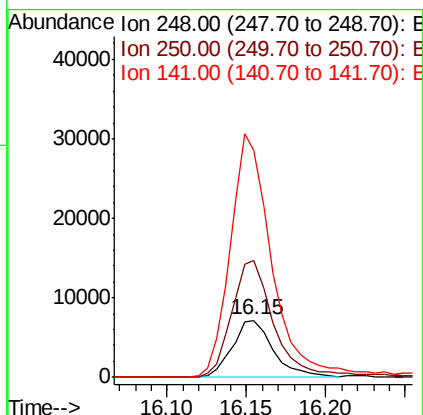
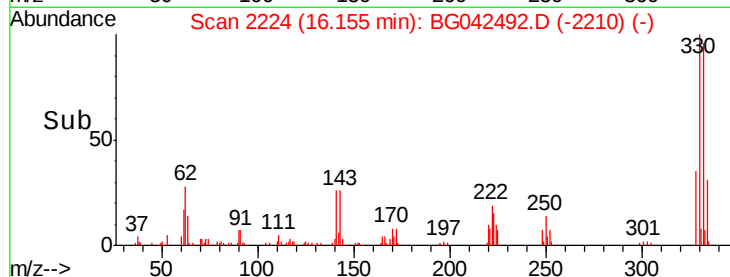



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.69 min Scan# 3166
 Delta R.T. -0.01 min
 Lab File: BG042492.D
 Acq: 26 Aug 2019 9:55

Tgt Ion:240 Resp: 365851
 Ion Ratio Lower Upper
 240 100
 120 7.1 5.7 8.5
 236 25.7 21.0 31.4

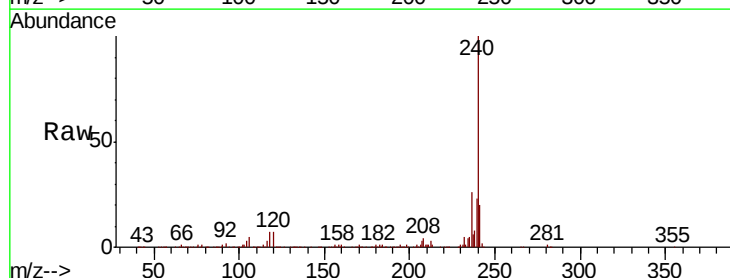

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

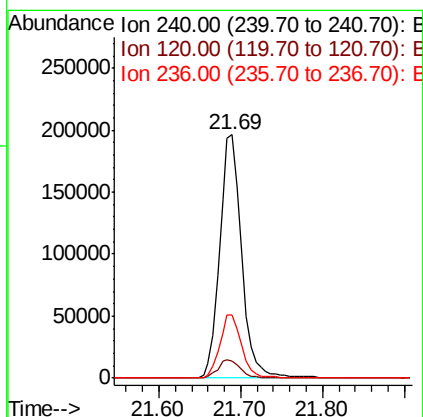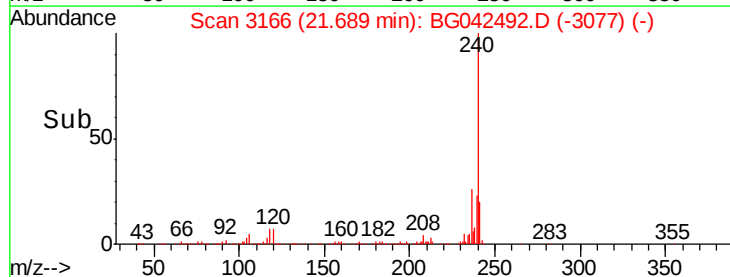



#79

Terphenyl-d14

Concen: 74.985 ng

RT: 20.03 min Scan# 2883

Delta R.T. -0.00 min

Lab File: BG042492.D

Acq: 26 Aug 2019 9:55

Instrument :

BNA_G

ClientSampleId :

PB122510TB


Tgt Ion:244 Resp: 1268936

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0




122 8.4 6.7 10.1



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

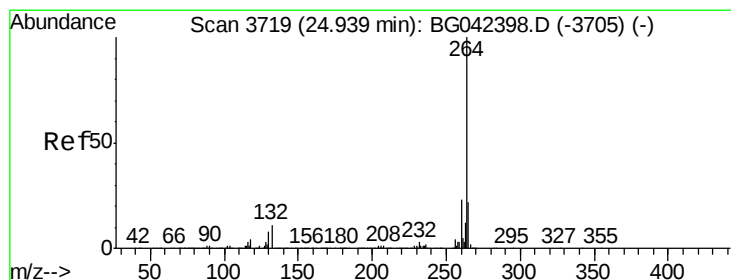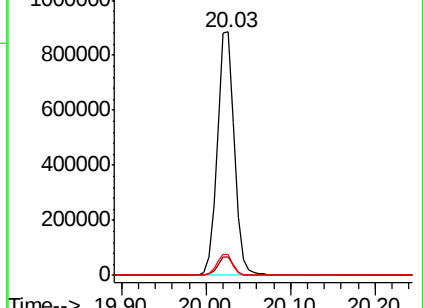

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717

Delta R.T. -0.01 min

Lab File: BG042492.D

Acq: 26 Aug 2019 9:55


Tgt Ion:264 Resp: 429705

Ion Ratio Lower Upper

264 100

260 23.4 18.5 27.7

265 21.6 17.6 26.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

