

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082619\
 Data File : BG042496.D
 Acq On : 26 Aug 2019 12:28
 Operator : HP/JU
 Sample : PB122444BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB122444BL

Quant Time: Aug 27 01:06:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	49691	20.00	ng	0.00
21) Naphthalene-d8	10.82	136	194762	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	136205	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	311571	20.00	ng	0.00
76) Chrysene-d12	21.69	240	356537	20.00	ng	0.00
87) Perylene-d12	24.93	264	406533	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	355225	144.78	ng	0.00
7) Phenol-d6	7.17	99	462729	139.62	ng	0.00
23) Nitrobenzene-d5	9.17	82	262306	93.07	ng	0.00
42) 2,4,6-Tribromophenol	16.15	330	232667	120.18	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	816211	101.35	ng	0.00
79) Terphenyl-d14	20.02	244	1458632	88.45	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.17	70	33273	15.497	ng	# 75
51) 2,6-Dinitrotoluene	14.66	165	17304	7.596	ng	# 36
57) 2,4-Dinitrotoluene	14.66	165	17304	5.305	ng	# 38
67) 4-Bromophenyl-phenylether	16.15	248	16213	4.102	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG082619\
Data File : BG042496.D
Acq On : 26 Aug 2019 12:28
Operator : HP/JU
Sample : PB122444BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB122444BL

Quant Time: Aug 27 01:06:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

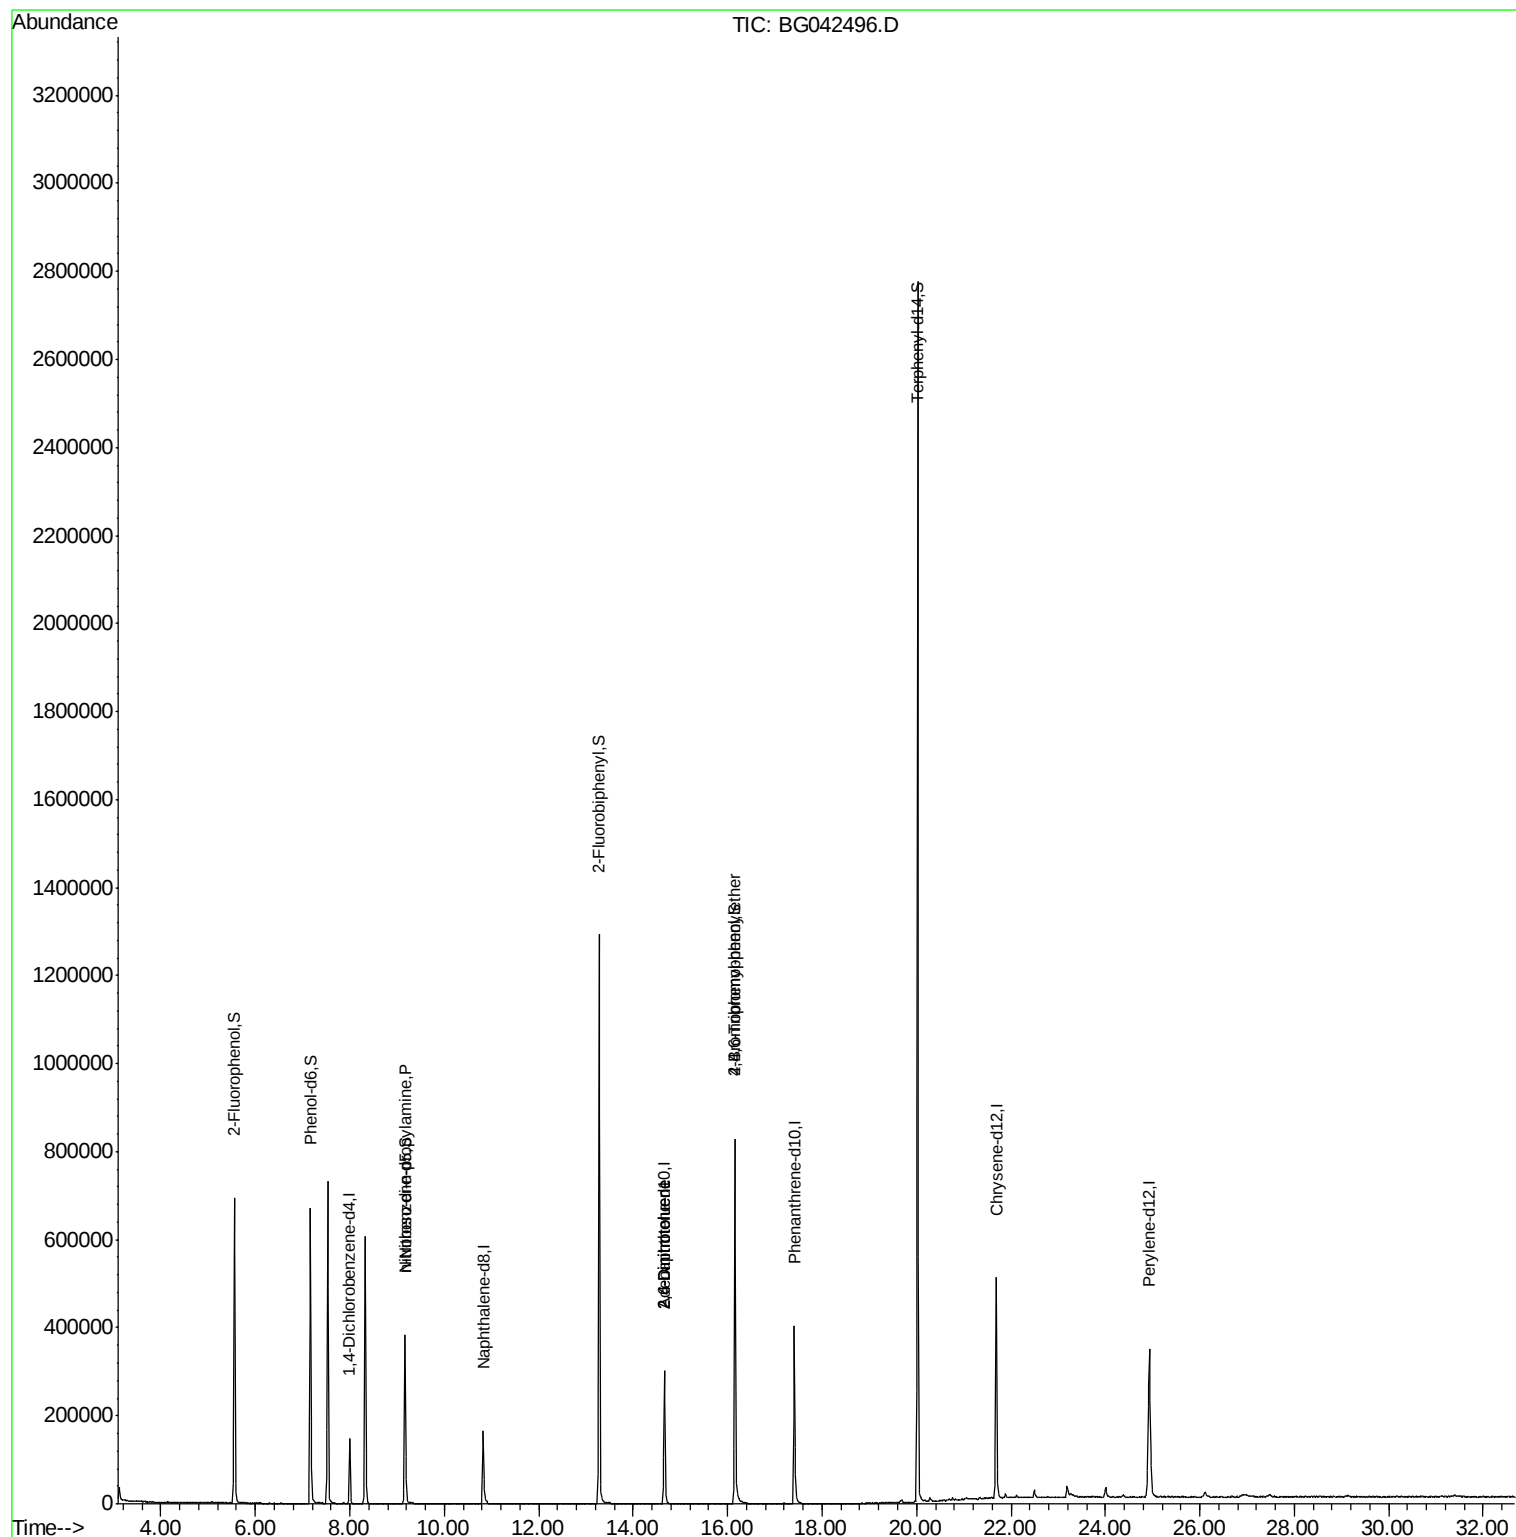




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.00 min Scan# 836
 Delta R.T. -0.01 min
 Lab File: BG042496.D
 Acq: 26 Aug 2019 12:28

Instrument :
 BNA_G
 ClientSampleId :
 PB122444BL

Tgt Ion:152 Resp: 49691
 Ion Ratio Lower Upper
 152 100
 150 162.7 125.4 188.0
 115 50.7 38.5 57.7

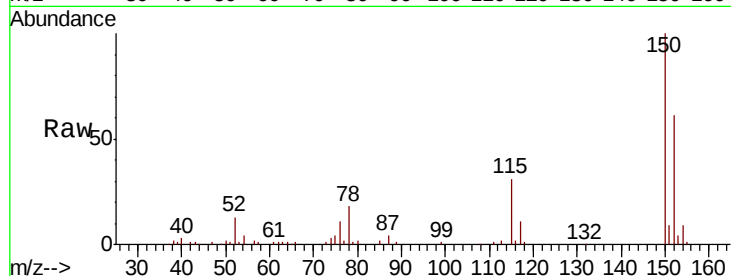


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

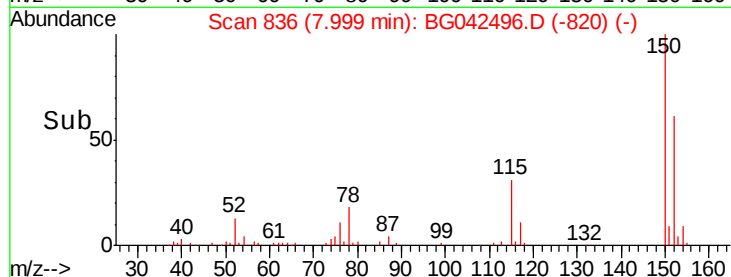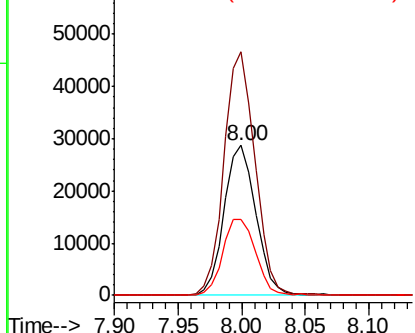



#5


2-Fluorophenol
 Concen: 144.782 ng
 RT: 5.56 min Scan# 420
 Delta R.T. -0.01 min
 Lab File: BG042496.D
 Acq: 26 Aug 2019 12:28

Tgt Ion:112 Resp: 355225
 Ion Ratio Lower Upper
 112 100
 64 53.8 42.8 64.2
 63 27.8 22.7 34.1

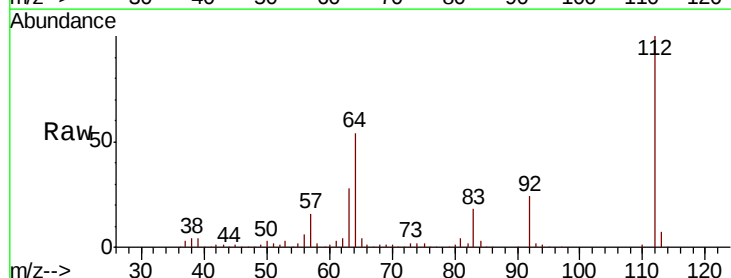

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

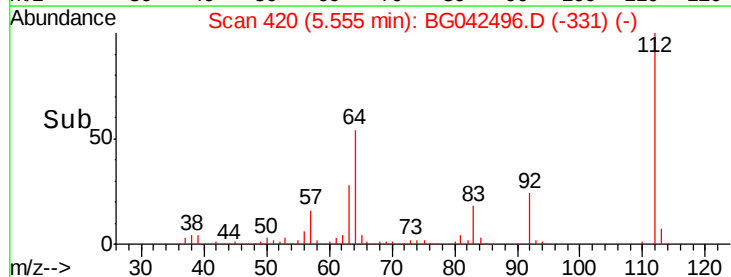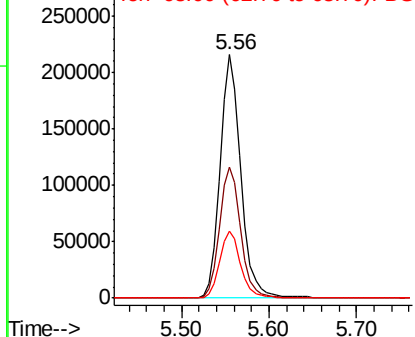

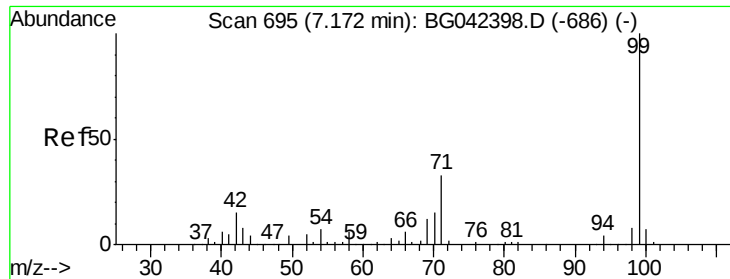

#7

Phenol-d6

Concen: 139.622 ng

RT: 7.17 min Scan# 694

Delta R.T. -0.01 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28

Instrument :

BNA_G

ClientSampleId :

PB122444BL


Tgt Ion: 99 Resp: 462729

Ion Ratio Lower Upper




99 100

42 13.9 12.0 18.0

71 32.5 26.3 39.5

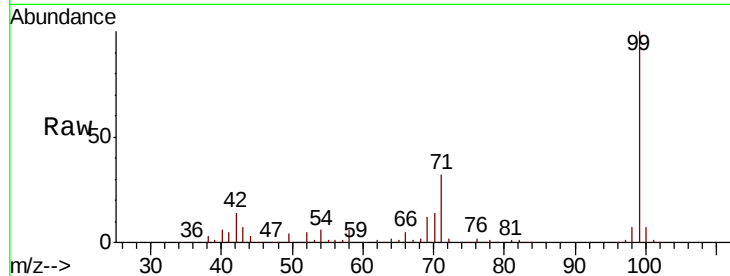

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

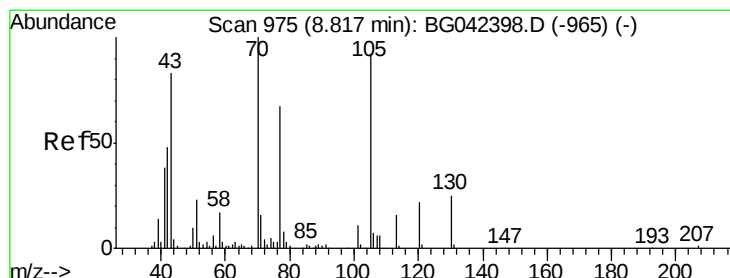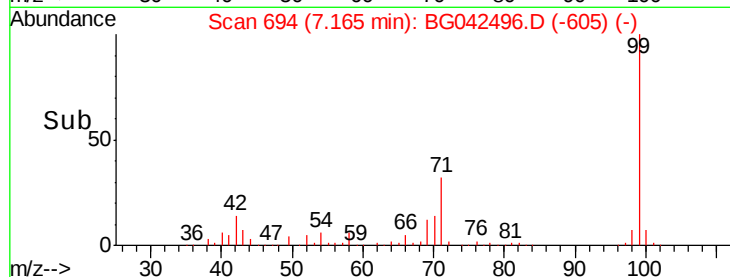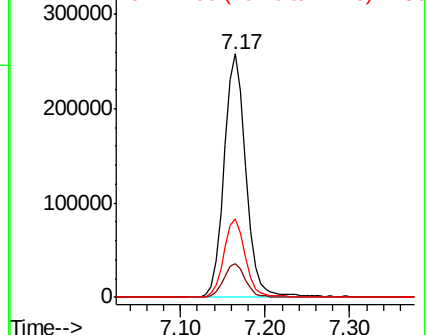

#19

n-Nitroso-di-n-propylamine

Concen: 15.497 ng

RT: 9.17 min Scan# 1035

Delta R.T. 0.35 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28

Tgt Ion: 70 Resp: 33273


Ion Ratio Lower Upper

70 100



42 38.6 38.8 58.2#

101 0.0 9.0 13.6#

130 2.5 20.0 30.0#

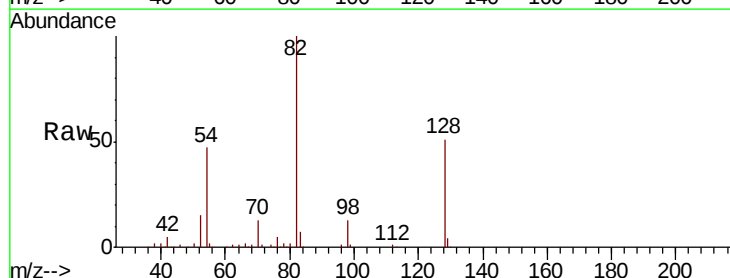

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

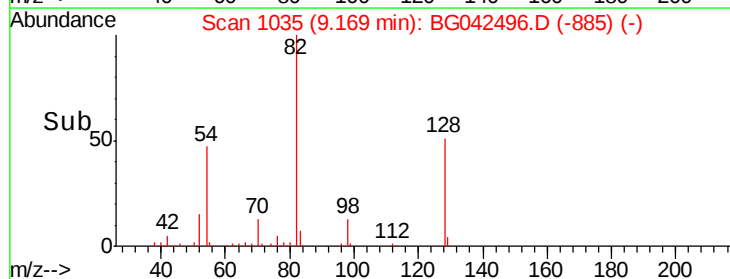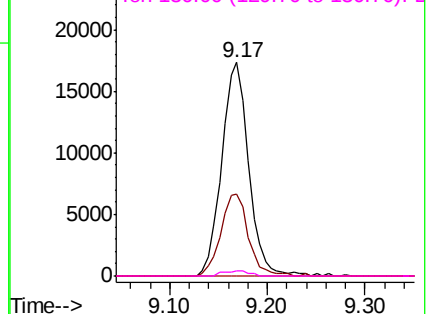






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.82 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BG042496.D
Acq: 26 Aug 2019 12:28

Instrument :
BNA_G
ClientSampleId :
PB122444BL

Tgt Ion:	136	Resp:	194762
Ion	Ratio	Lower	Upper
136	100		
137	11.5	8.7	13.1
54	6.9	4.9	7.3
68	4.8	3.6	5.4

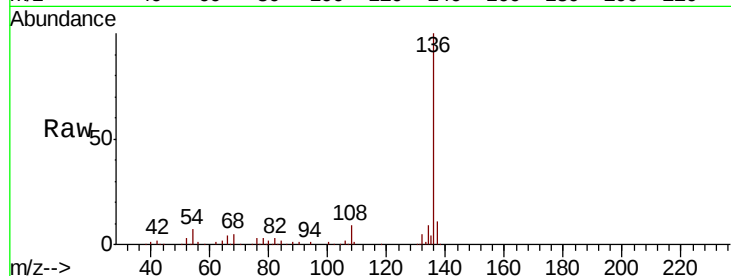


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

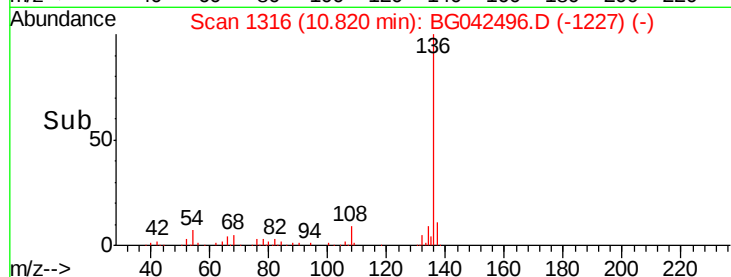
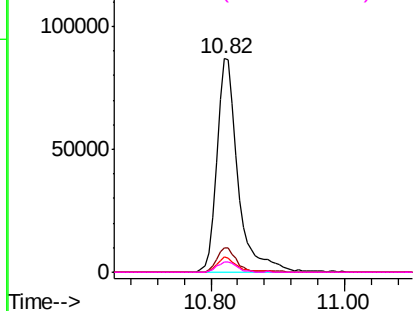


#23
Nitrobenzene-d5
Concen: 93.069 ng
RT: 9.17 min Scan# 1035
Delta R.T. -0.01 min
Lab File: BG042496.D
Acq: 26 Aug 2019 12:28

Tgt Ion:	82	Resp:	262306
Ion	Ratio	Lower	Upper
82	100		
128	51.2	40.7	61.1
54	46.7	36.3	54.5

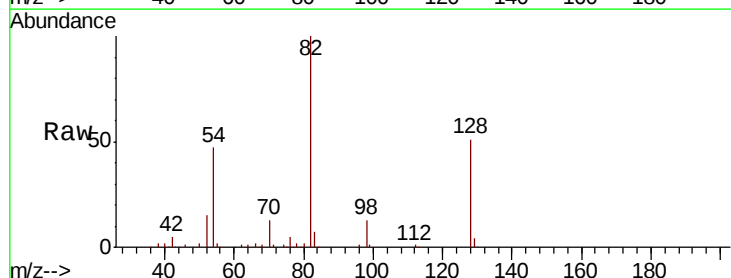

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

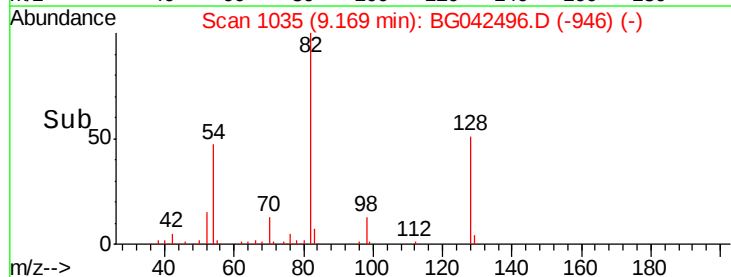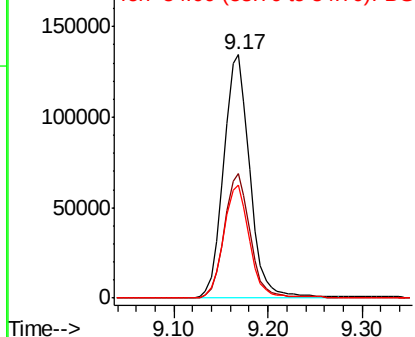



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.66 min Scan# 1970

Delta R.T. -0.00 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28

Instrument :

BNA_G

ClientSampleId :

PB122444BL


Tgt Ion:164 Resp: 136205

Ion Ratio Lower Upper

164 100

162 97.6 79.9 119.9




160 41.5 34.3 51.5

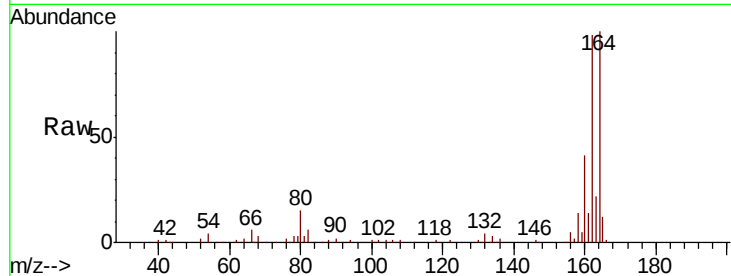

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

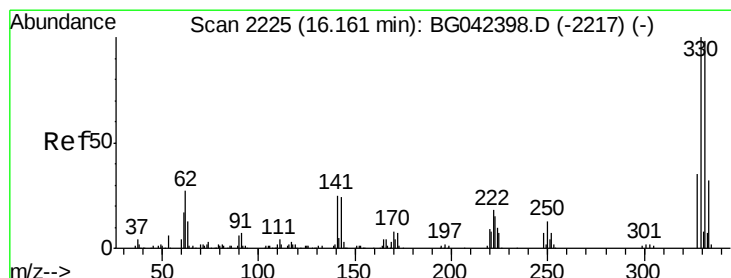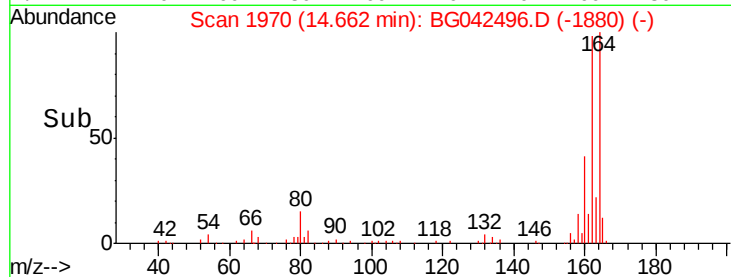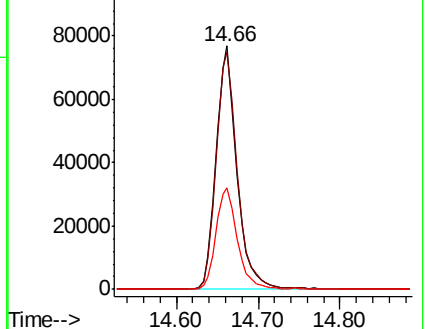

#42

2,4,6-Tribromophenol

Concen: 120.184 ng

RT: 16.15 min Scan# 2224

Delta R.T. -0.01 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28


Tgt Ion:330 Resp: 232667

Ion Ratio Lower Upper

330 100

332 98.2 77.4 116.0



141 29.1 21.4 32.0

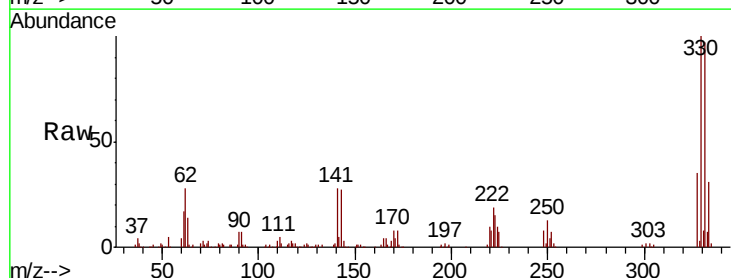

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



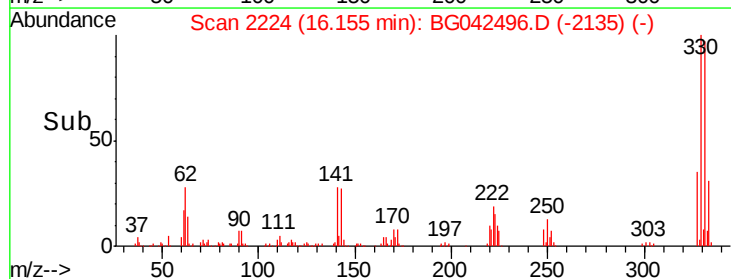
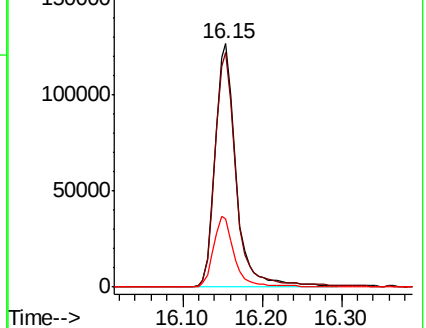




#45
 2-Fluorobiphenyl
 Concen: 101.351 ng
 RT: 13.28 min Scan# 1734
 Delta R.T. -0.01 min
 Lab File: BG042496.D
 Acq: 26 Aug 2019 12:28




Instrument :
 BNA_G
 ClientSampleId :
 PB122444BL


Tgt Ion:172 Resp: 816211
 Ion Ratio Lower Upper
 172 100
 171 37.7 30.5 45.7
 170 24.5 20.2 30.2

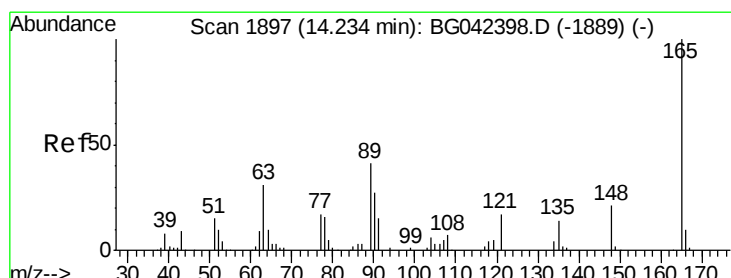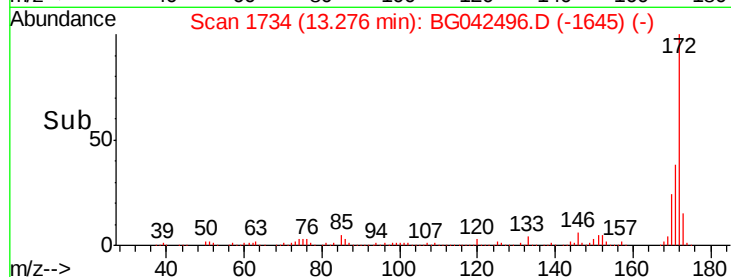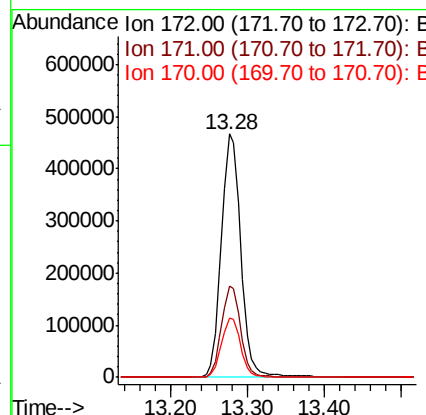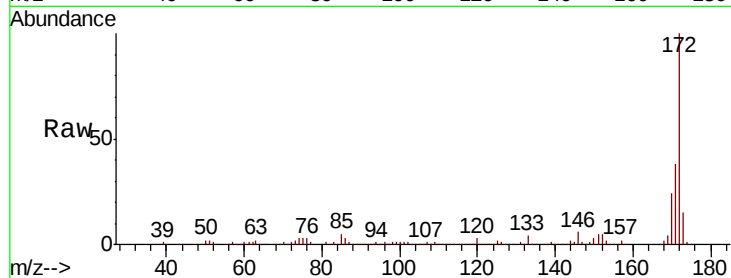

#51
 2,6-Dinitrotoluene
 Concen: 7.596 ng
 RT: 14.66 min Scan# 1970
 Delta R.T. 0.43 min
 Lab File: BG042496.D
 Acq: 26 Aug 2019 12:28

Tgt Ion:165 Resp: 17304
 Ion Ratio Lower Upper
 165 100
 63 0.0 30.6 45.8#
 89 0.0 32.6 49.0#

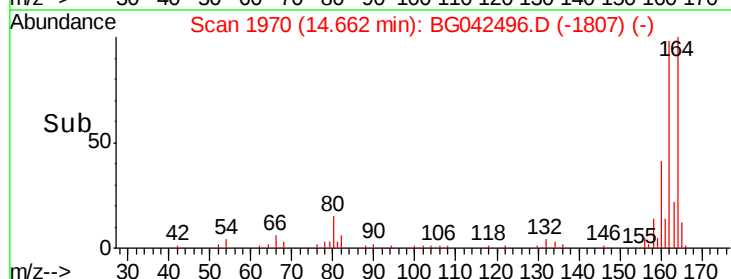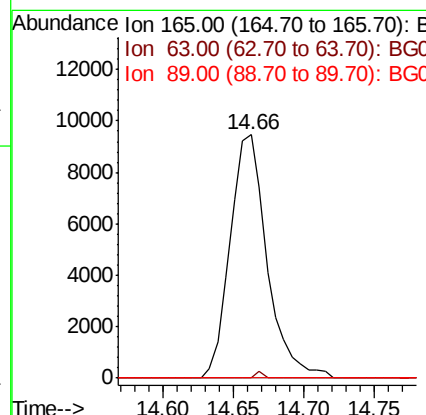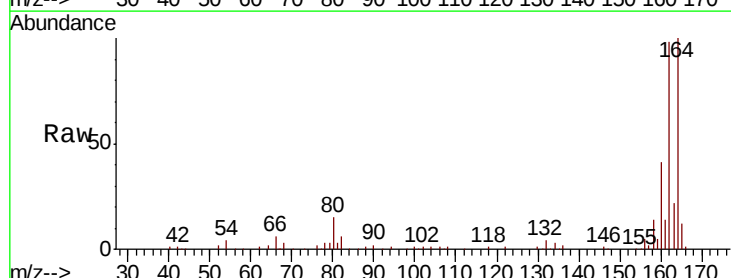

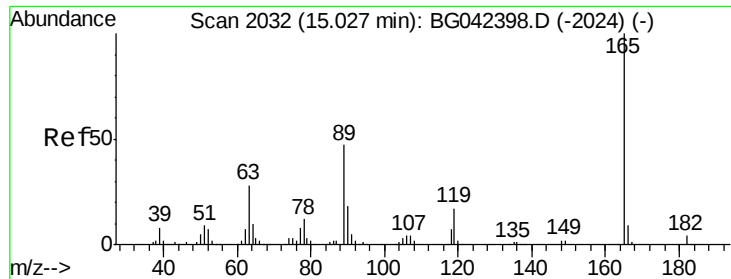

#57

2,4-Dinitrotoluene

Concen: 5.305 ng

RT: 14.66 min Scan# 1970

Delta R.T. -0.36 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28

Instrument :

BNA_G

ClientSampleId :

PB122444BL

Tgt Ion:165 Resp: 17304


Ion Ratio Lower Upper

165 100

63 0.0 22.5 33.7#

89 0.0 37.8 56.6#

182 0.0 3.0 4.4#



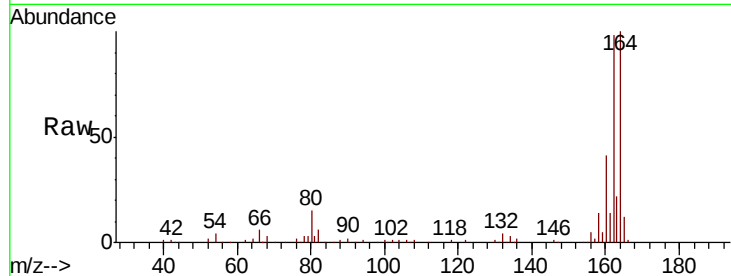


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

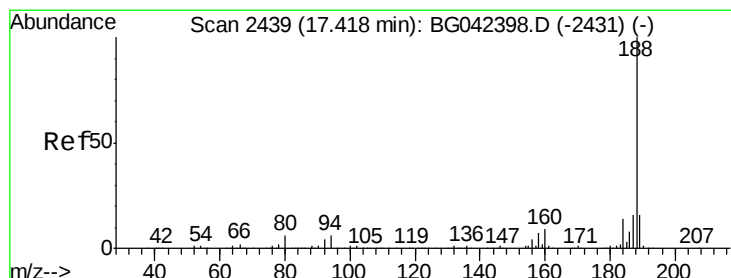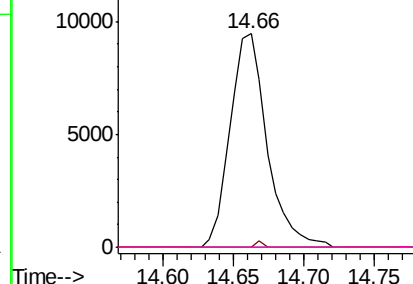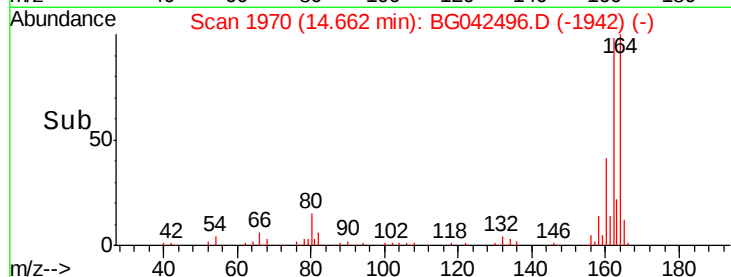

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2438

Delta R.T. -0.01 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28


Tgt Ion:188 Resp: 311571

Ion Ratio Lower Upper

188 100

94 6.3 4.5 6.7



80 6.7 4.9 7.3

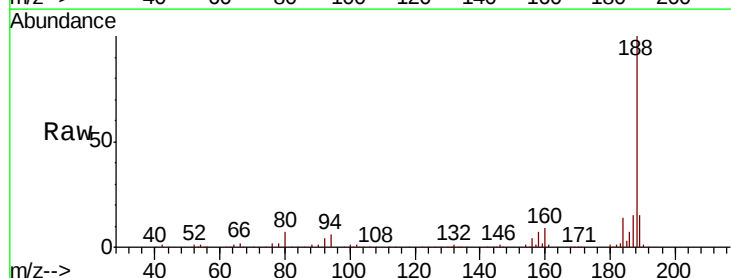


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

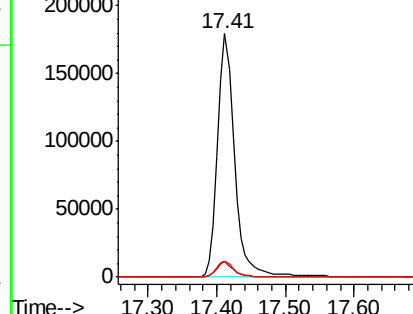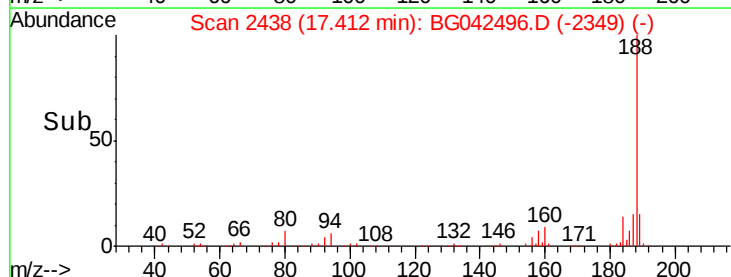


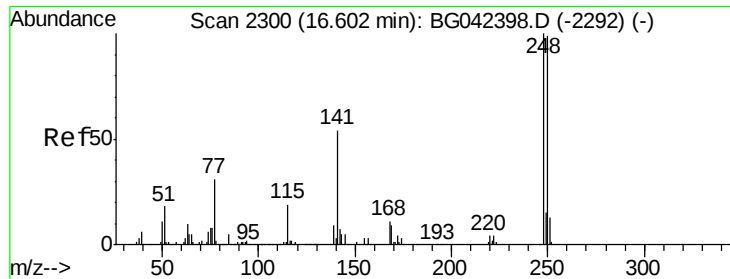




#67
 4-Bromophenyl-phenylether
 Concen: 4.102 ng
 RT: 16.15 min Scan# 2224
 Delta R.T. -0.45 min
 Lab File: BG042496.D
 Acq: 26 Aug 2019 12:28

Instrument :
 BNA_G
 ClientSampleId :
 PB122444BL

Tgt Ion:248 Resp: 16213
 Ion Ratio Lower Upper
 248 100
 250 177.9 78.9 118.3#
 141 369.9 43.3 64.9#

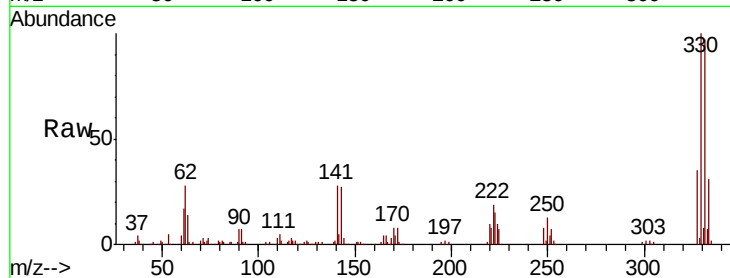


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

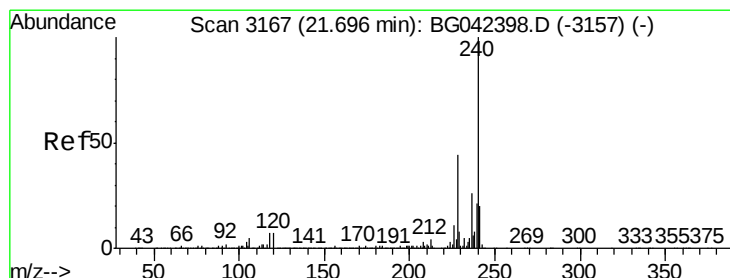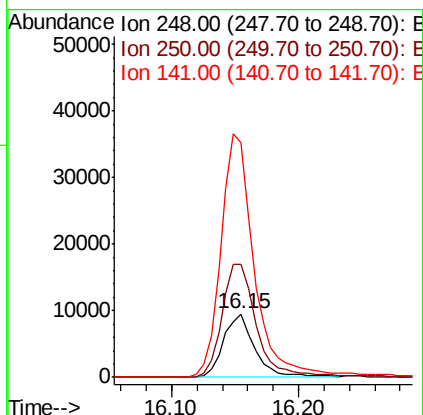
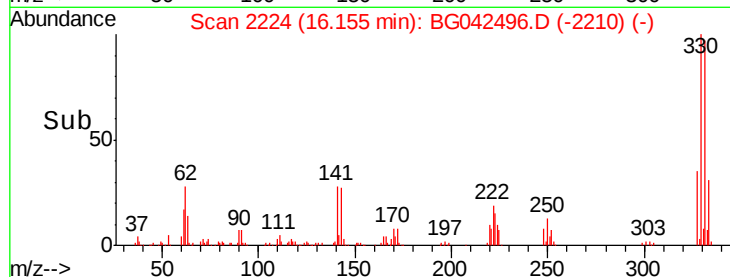



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.69 min Scan# 3166
 Delta R.T. -0.01 min
 Lab File: BG042496.D
 Acq: 26 Aug 2019 12:28

Tgt Ion:240 Resp: 356537
 Ion Ratio Lower Upper
 240 100
 120 7.3 5.7 8.5
 236 26.5 21.0 31.4

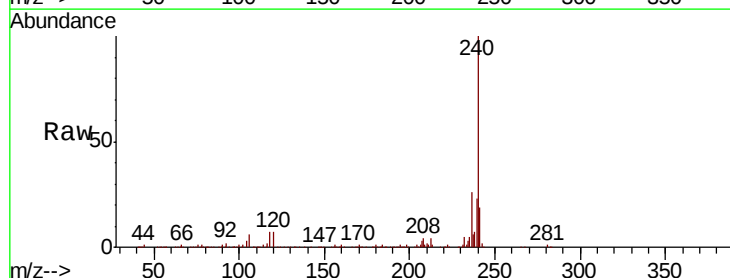

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

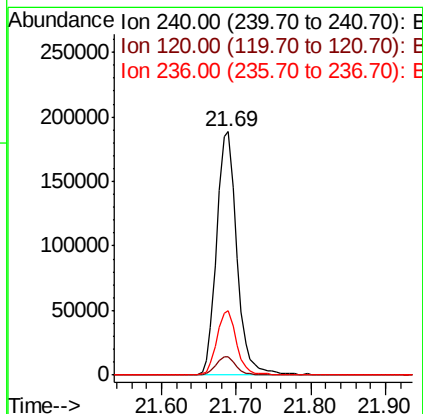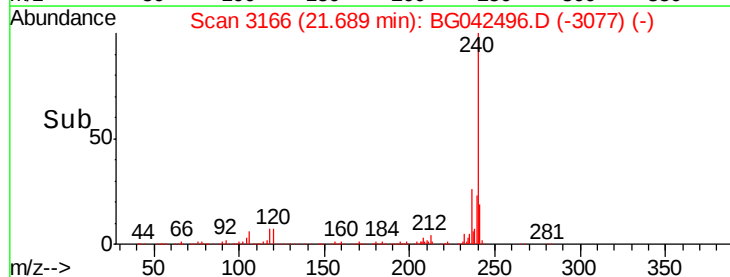

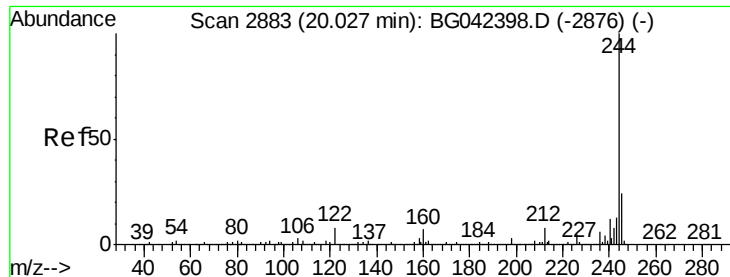

#79

Terphenyl-d14

Concen: 88.446 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.01 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28

Instrument :

BNA_G

ClientSampleId :

PB122444BL


Tgt Ion:244 Resp: 1458632

Ion Ratio Lower Upper

244 100

212 7.7 6.0 9.0




122 8.8 6.7 10.1

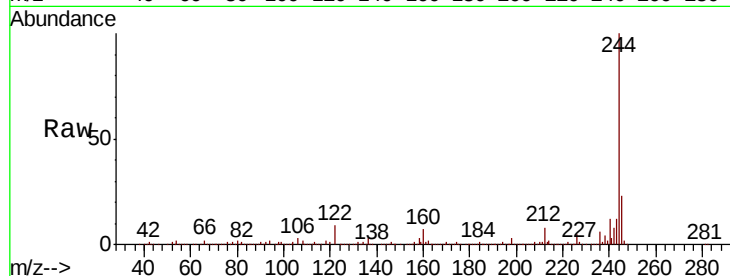

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

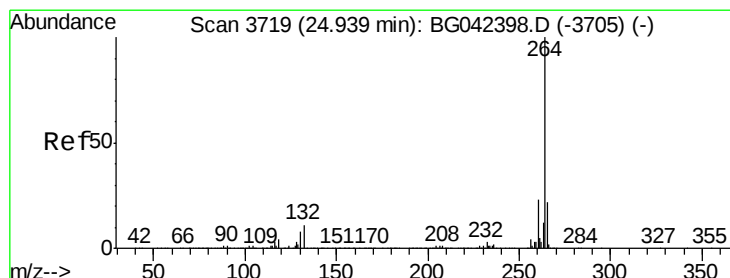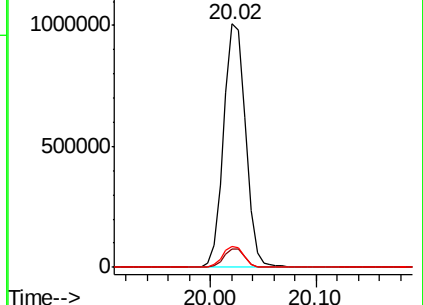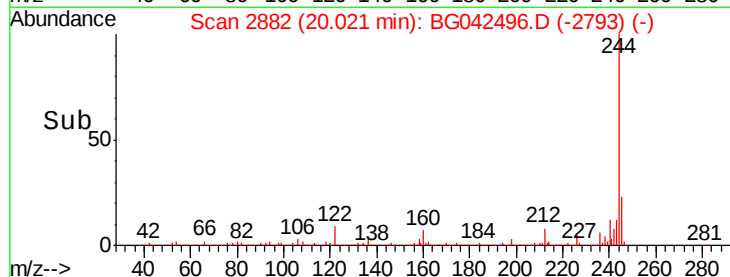

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.93 min Scan# 3717

Delta R.T. -0.01 min

Lab File: BG042496.D

Acq: 26 Aug 2019 12:28


Tgt Ion:264 Resp: 406533

Ion Ratio Lower Upper

264 100

260 23.0 18.5 27.7

265 22.1 17.6 26.4

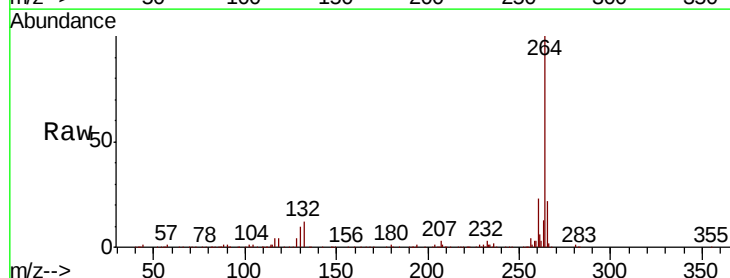

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

