

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG050007.D
 Acq On : 27 Aug 2021 21:46
 Operator : CG/JU
 Sample : M3518-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B06

Manual Integrations
 APPROVED

mohammad
 8/30/2021 10:32:54 AM

Quant Time: Aug 27 23:37:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 27 11:22:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	29689	20.000	ng/u1	-0.02
20) Naphthalene-d8	10.786	136	113785	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.628	164	78622	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.377	188	176368	20.000	ng/u1	-0.02
79) Chrysene-d12	21.654	240	169074	20.000	ng/u1	-0.01
88) Perylene-d12	24.879	264	168317	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.331	96	1548m	2.689	ng/uL	-0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.138	99	38718	15.358	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.285	67	21403	15.281	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.496	132	28229	14.965	ng/u1	-0.02
15) 4-Methylphenol-d8	8.689	113	30315	15.268	ng/u1	-0.01
21) Nitrobenzene-d5	9.141	128	16120	18.274	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.864	143	17351	16.518	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.416	165	30639	16.354	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.933	131	14414	5.652	ng/u1	0.00
46) Dimethylphthalate-d6	14.023	166	106198	17.650	ng/u1	-0.02
49) Acenaphthylene-d8	14.316	160	122999	17.434	ng/u1	-0.02
54) 4-Nitrophenol-d4	14.863	143	13613	15.637	ng/u1	0.00
60) Fluorene-d10	15.621	176	89776	17.598	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.756	200	14881	13.115	ng/u1	-0.01
73) Anthracene-d10	17.477	188	126970	16.032	ng/u1	-0.02
81) Pyrene-d10	19.768	212	185554	20.309	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.655	264	161690	18.107	ng/u1	-0.02
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.103	77	5435	3.746	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG050007.D
Acq On : 27 Aug 2021 21:46
Operator : CG/JU
Sample : M3518-03
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0B06

Manual Integrations
APPROVED

mohammad
8/30/2021 10:32:54 AM


Quant Time: Aug 27 23:37:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 27 11:22:49 2021
Response via : Initial Calibration

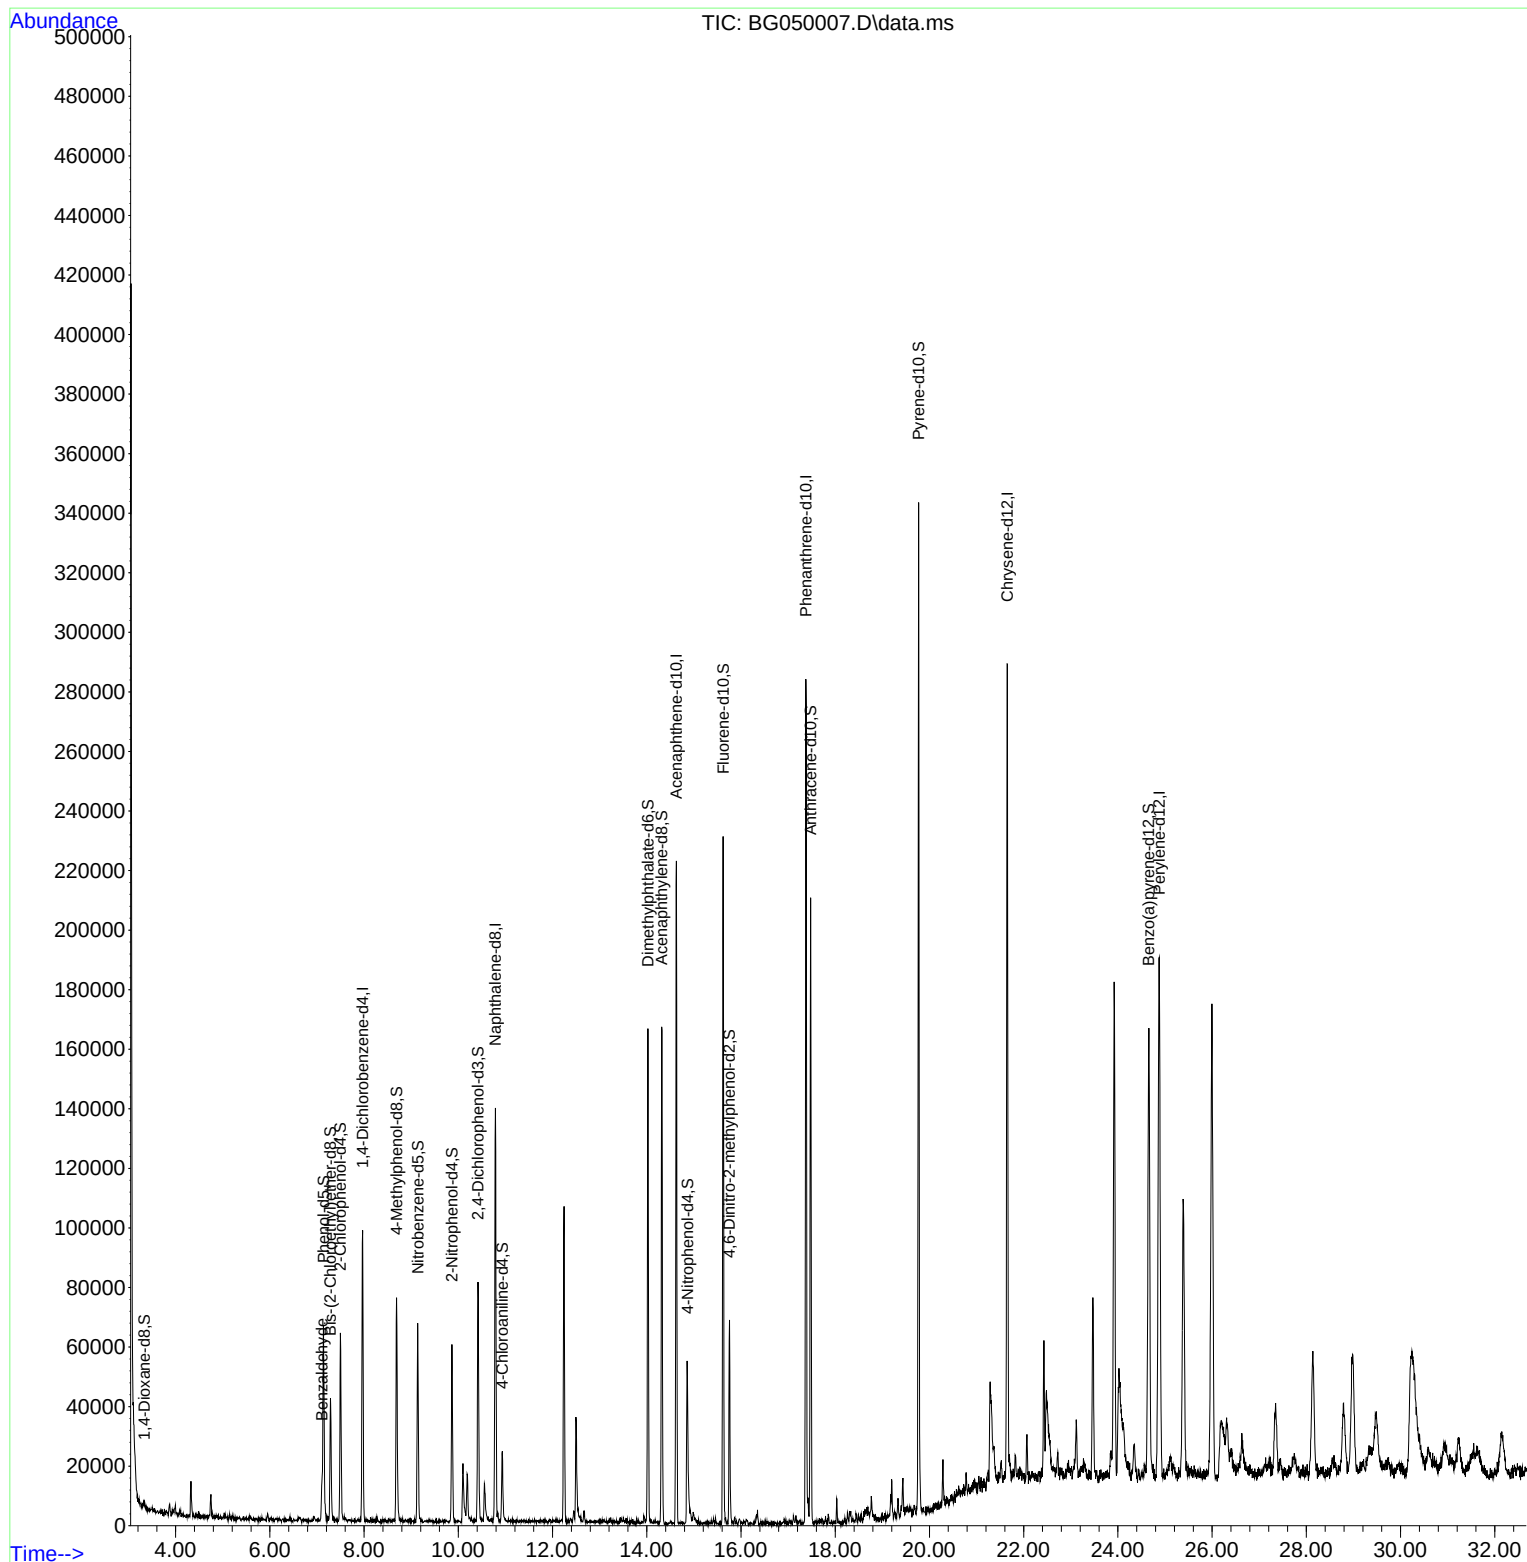

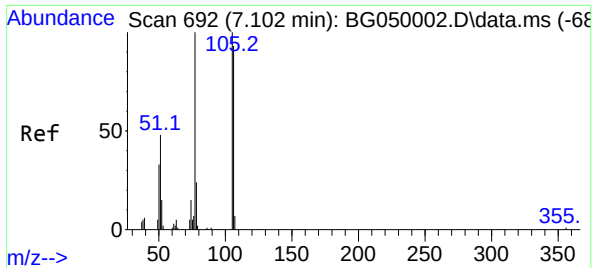

#6
Benzaldehyde
Concen: 3.746 ng/ul
RT: 7.103 min Scan# 692
Delta R.T. -0.017 min
Lab File: BG050007.D
Acq: 27 Aug 2021 21:46

Instrument :
BNA_G
ClientSampleId :
C0B06

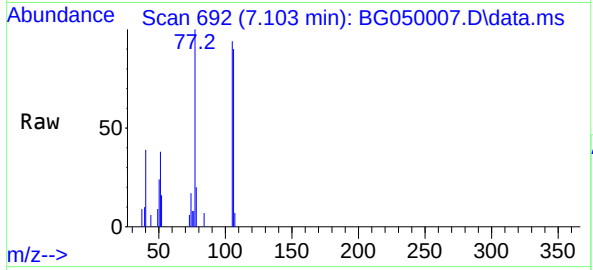

Tgt Ion: 77 Resp: 5435

Ion	Ratio	Lower	Upper
77	100		
105	94.1	72.3	108.5
106	90.3	72.3	108.5

Manual Integrations
APPROVED
mohammad
8/30/2021 10:32:54 AM

