

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049977.D
 Acq On : 26 Aug 2021 12:07
 Operator : CG/JU
 Sample : PB138646BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.331	46	50	55	rBV5	4346	7222	0.77%	0.080%
2	3.760	119	123	137	rBV	58559	140389	14.91%	1.546%
3	4.371	224	227	230	rBV3	1103	1625	0.17%	0.018%
4	4.400	230	232	237	rVB3	1698	2216	0.24%	0.024%
5	4.735	286	289	293	rVB4	1790	2358	0.25%	0.026%
6	4.817	302	303	308	rBV4	1435	1696	0.18%	0.019%
7	5.657	443	446	449	rVB2	1353	1530	0.16%	0.017%
8	5.693	449	452	453	rBV	1476	1424	0.15%	0.016%
9	6.914	657	660	663	rBV	1414	1953	0.21%	0.022%
10	7.144	692	699	710	rVB	127796	229986	24.43%	2.533%
11	7.290	717	724	734	rBV	87483	154295	16.39%	1.699%
12	7.502	754	760	772	rVB2	125381	231650	24.61%	2.552%
13	7.972	832	840	848	rBV	90376	158901	16.88%	1.750%
14	8.694	956	963	971	rBV	167992	292702	31.09%	3.224%
15	9.141	1031	1039	1049	rVB	134745	247956	26.34%	2.731%
16	9.869	1156	1163	1172	rVB2	128868	232031	24.65%	2.556%
17	10.421	1249	1257	1266	rBV2	171034	311483	33.09%	3.431%
18	10.792	1312	1320	1329	rVB	137518	243866	25.91%	2.686%
19	10.933	1335	1344	1357	rBV	169703	320714	34.07%	3.533%
20	11.661	1463	1468	1472	rVB	1012	2132	0.23%	0.023%
21	12.383	1586	1591	1593	rBV2	2486	3100	0.33%	0.034%
22	12.495	1607	1610	1614	rBV	923	1392	0.15%	0.015%
23	14.028	1865	1871	1878	rBV	370813	554401	58.90%	6.106%
24	14.328	1911	1922	1930	rBV	361755	583854	62.02%	6.431%
25	14.633	1967	1974	1980	rVB	232330	363988	38.67%	4.009%
26	14.857	2006	2012	2029	rBV	119437	232836	24.73%	2.565%
27	14.986	2032	2034	2036	rVB2	1542	1514	0.16%	0.017%
28	15.062	2044	2047	2050	rVB3	1576	2189	0.23%	0.024%
29	15.491	2117	2120	2124	rVB2	1117	1424	0.15%	0.016%
30	15.626	2136	2143	2152	rVB	492364	740530	78.67%	8.157%
31	15.761	2160	2166	2175	rBV	157343	249167	26.47%	2.744%
32	15.861	2180	2183	2187	rVB2	3594	4574	0.49%	0.050%
33	16.402	2273	2275	2280	rVB2	1250	1473	0.16%	0.016%
34	17.330	2430	2433	2436	rVB	1136	1374	0.15%	0.015%
35	17.383	2436	2442	2451	rBV	313130	478131	50.79%	5.266%
36	17.482	2451	2459	2468	rBV2	560813	856443	90.98%	9.433%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049977.D
 Acq On : 26 Aug 2021 12:07
 Operator : CG/JU
 Sample : PB138646BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	17.571	2473	2474	2479	rVB	1204	1499	0.16%	0.017%
38	18.035	2546	2553	2557	rBV3	1799	4456	0.47%	0.049%
39	18.258	2588	2591	2593	rBV	1214	1615	0.17%	0.018%
40	18.340	2604	2605	2607	rVB2	2097	1444	0.15%	0.016%
41	18.364	2607	2609	2610	rBV	2418	1844	0.20%	0.020%
42	18.458	2621	2625	2627	rVB3	2006	2477	0.26%	0.027%
43	18.493	2627	2631	2634	rBV	1254	2054	0.22%	0.023%
44	18.646	2655	2657	2661	rBV3	1302	1693	0.18%	0.019%
45	18.769	2676	2678	2679	rBV2	3093	1831	0.19%	0.020%
46	18.851	2688	2692	2693	rBV2	2524	2193	0.23%	0.024%
47	18.869	2693	2695	2698	rVV3	1830	1653	0.18%	0.018%
48	18.992	2714	2716	2720	rVB2	1692	1522	0.16%	0.017%
49	19.215	2752	2754	2755	rVB2	2595	1566	0.17%	0.017%
50	19.268	2761	2763	2767	rVB4	2158	1958	0.21%	0.022%
51	19.304	2767	2769	2771	rBV3	2381	1593	0.17%	0.018%
52	19.333	2771	2774	2778	rBV3	6102	10235	1.09%	0.113%
53	19.409	2783	2787	2791	rVB2	6388	11032	1.17%	0.122%
54	19.773	2843	2849	2858	rVB	690774	941324	100.00%	10.368%
55	20.290	2935	2937	2944	rBV6	4860	6275	0.67%	0.069%
56	21.659	3164	3170	3175	rBV	236186	372382	39.56%	4.102%
57	24.667	3672	3682	3692	rBV3	229962	655425	69.63%	7.219%
58	24.884	3712	3719	3731	rVB2	134026	390289	41.46%	4.299%



Sum of corrected areas: 9078879

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049977.D
Acq On : 26 Aug 2021 12:07
Operator : CG/JU
Sample : PB138646BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK646

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

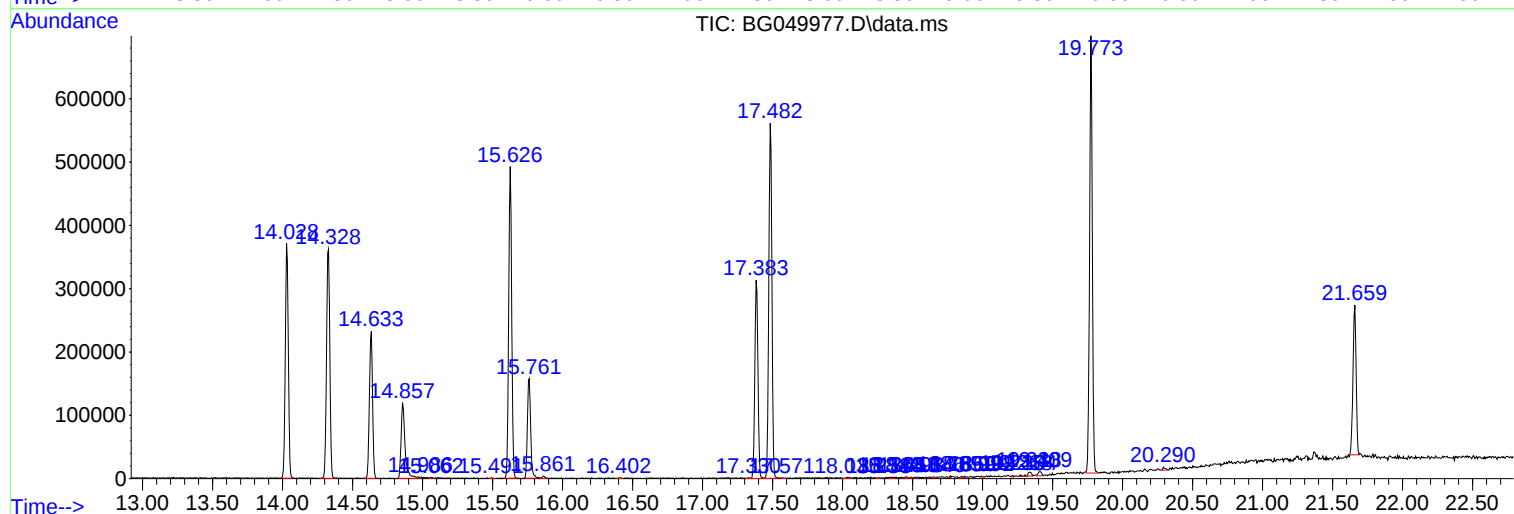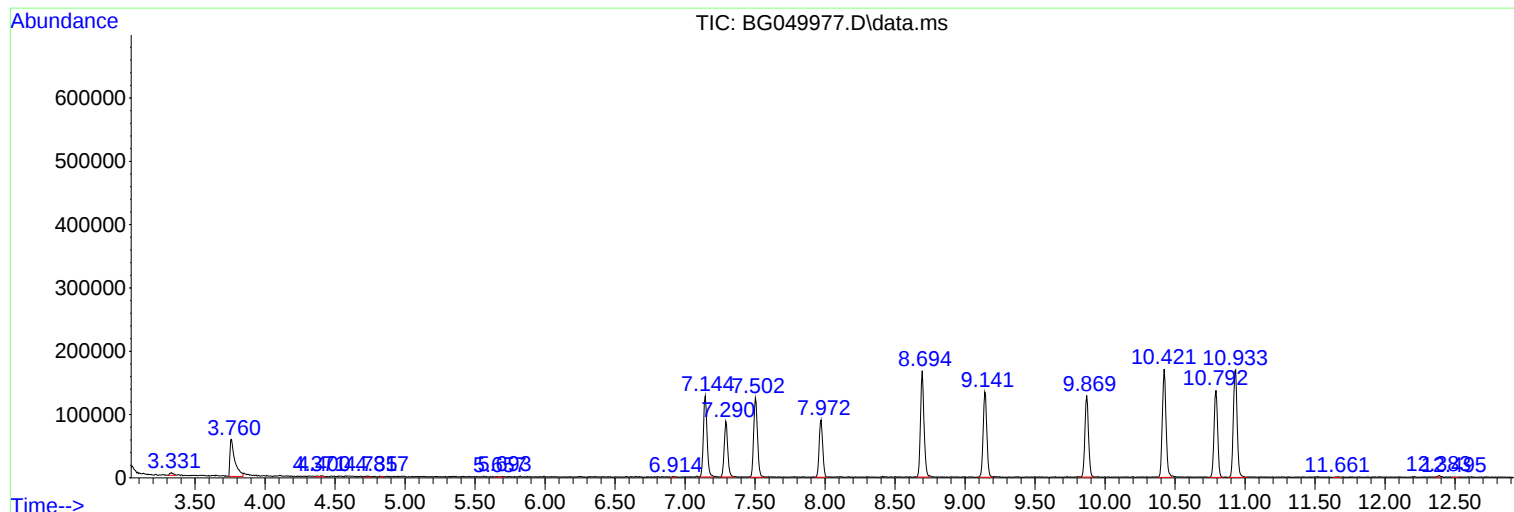

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049977.D
Acq On : 26 Aug 2021 12:07
Operator : CG/JU
Sample : PB138646BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK646

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049977.D
Acq On : 26 Aug 2021 12:07
Operator : CG/JU
Sample : PB138646BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK646

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
