

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049983.D
 Acq On : 26 Aug 2021 20:14
 Operator : CG/JU
 Sample : PB138723BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK723

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.327	46	49	55	rVB5	5037	7893	0.84%	0.089%
2	3.756	119	122	136	rBV	59586	145166	15.41%	1.642%
3	4.044	168	171	174	rBV2	1341	1374	0.15%	0.016%
4	4.267	208	209	213	rBV3	1580	2378	0.25%	0.027%
5	4.978	328	330	333	rBV2	1214	1417	0.15%	0.016%
6	5.654	442	445	450	rVB5	1441	1787	0.19%	0.020%
7	5.906	485	488	491	rBV3	1665	1606	0.17%	0.018%
8	6.170	530	533	536	rBV	1395	1999	0.21%	0.023%
9	6.593	601	605	609	rBV2	997	1829	0.19%	0.021%
10	6.828	640	645	650	rBV2	1295	2532	0.27%	0.029%
11	6.893	654	656	658	rBV	1394	1394	0.15%	0.016%
12	7.087	684	689	692	rBV4	2235	3432	0.36%	0.039%
13	7.140	692	698	709	rVV	131734	236306	25.08%	2.674%
14	7.228	711	713	716	rBV2	1182	1388	0.15%	0.016%
15	7.292	717	724	732	rBV	85586	154910	16.44%	1.753%
16	7.504	752	760	770	rBV2	122903	228502	24.25%	2.585%
17	7.968	833	839	848	rVB	93100	162332	17.23%	1.837%
18	8.027	848	849	853	rVB	1538	1351	0.14%	0.015%
19	8.086	853	859	862	rBV	919	2190	0.23%	0.025%
20	8.644	950	954	956	rBV2	1159	1849	0.20%	0.021%
21	8.691	956	962	971	rVV2	163981	293050	31.10%	3.316%
22	9.137	1031	1038	1048	rBV	132162	243995	25.90%	2.761%
23	9.865	1156	1162	1170	rBV3	121958	222801	23.65%	2.521%
24	10.418	1250	1256	1268	rBV	164370	305527	32.43%	3.457%
25	10.788	1312	1319	1331	rVB	134210	240745	25.55%	2.724%
26	10.929	1336	1343	1352	rBV	170259	309700	32.87%	3.504%
27	12.374	1586	1589	1591	rBV2	1620	1938	0.21%	0.022%
28	12.391	1591	1592	1597	rVB3	2557	1903	0.20%	0.022%
29	14.025	1864	1870	1880	rBV	346154	515043	54.67%	5.827%
30	14.324	1914	1921	1929	rVB	364012	563912	59.85%	6.380%
31	14.630	1966	1973	1981	rVB	224073	350230	37.17%	3.963%
32	14.853	2004	2011	2022	rBV	108431	218139	23.15%	2.468%
33	15.141	2058	2060	2065	rVB	1121	1474	0.16%	0.017%
34	15.622	2135	2142	2149	rBV	463268	699753	74.27%	7.917%
35	15.757	2159	2165	2176	rBV	140525	211368	22.43%	2.391%
36	15.869	2179	2184	2185	rBV2	2922	3446	0.37%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049983.D
 Acq On : 26 Aug 2021 20:14
 Operator : CG/JU
 Sample : PB138723BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK723

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	17.167	2399	2405	2409	rBV2	1467	2436	0.26%	0.028%
38	17.261	2416	2421	2422	rBV	1163	1224	0.13%	0.014%
39	17.385	2435	2442	2448	rBV	298128	458539	48.67%	5.188%
40	17.479	2452	2458	2467	rVB	505902	798015	84.70%	9.029%
41	18.753	2673	2675	2677	rBV2	1409	1532	0.16%	0.017%
42	19.041	2723	2724	2727	rBV2	1617	1693	0.18%	0.019%
43	19.094	2730	2733	2736	rVV	1535	1915	0.20%	0.022%
44	19.129	2736	2739	2740	rVV2	1635	1520	0.16%	0.017%
45	19.147	2740	2742	2744	rVB	2155	1713	0.18%	0.019%
46	19.212	2750	2753	2755	rBV2	1990	1891	0.20%	0.021%
47	19.259	2757	2761	2763	rVB3	1810	2696	0.29%	0.031%
48	19.282	2763	2765	2766	rBV	1817	1310	0.14%	0.015%
49	19.335	2771	2774	2778	rVV3	6935	9249	0.98%	0.105%
50	19.405	2782	2786	2793	rVB2	6268	9938	1.05%	0.112%
51	19.511	2802	2804	2805	rBV	2689	2202	0.23%	0.025%
52	19.776	2842	2849	2857	rVB	634234	942180	100.00%	10.660%
53	20.034	2889	2893	2895	rBV4	2656	3323	0.35%	0.038%
54	20.398	2953	2955	2956	rBV2	3239	2676	0.28%	0.030%
55	20.563	2981	2983	2985	rBV3	3560	3185	0.34%	0.036%
56	21.655	3163	3169	3176	rVB	258035	414018	43.94%	4.684%
57	24.657	3671	3680	3693	rVB2	232423	645655	68.53%	7.305%
58	24.875	3709	3717	3731	rVB2	132788	387012	41.08%	4.379%




Sum of corrected areas: 8838581

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049983.D
Acq On : 26 Aug 2021 20:14
Operator : CG/JU
Sample : PB138723BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK723

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

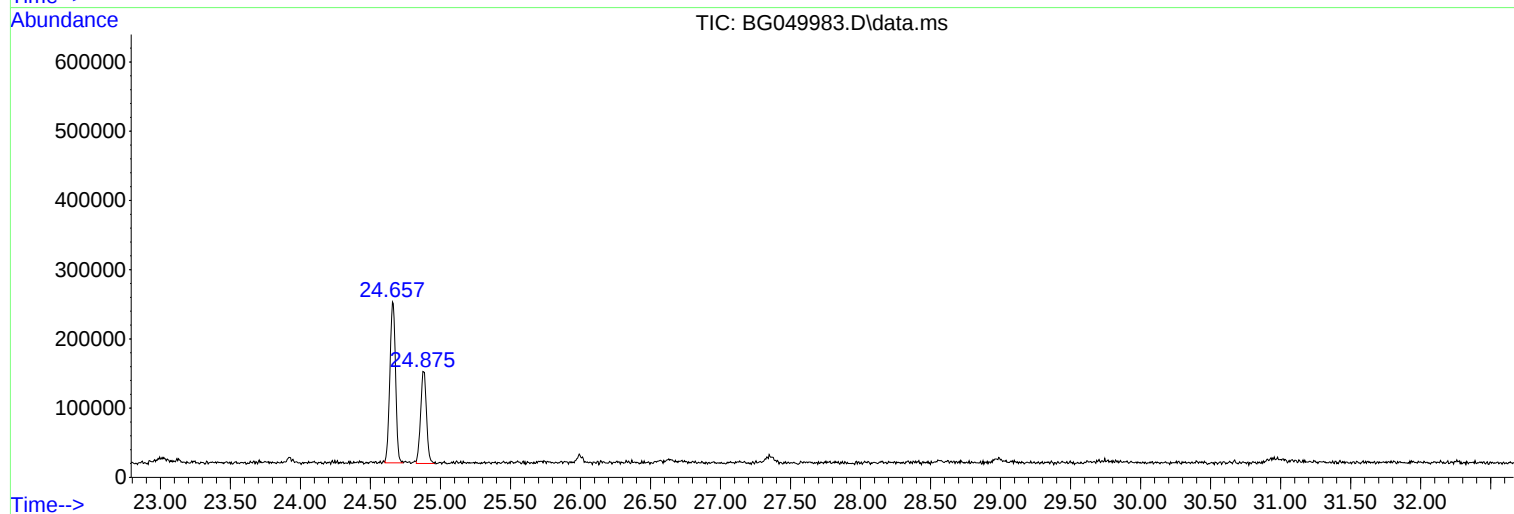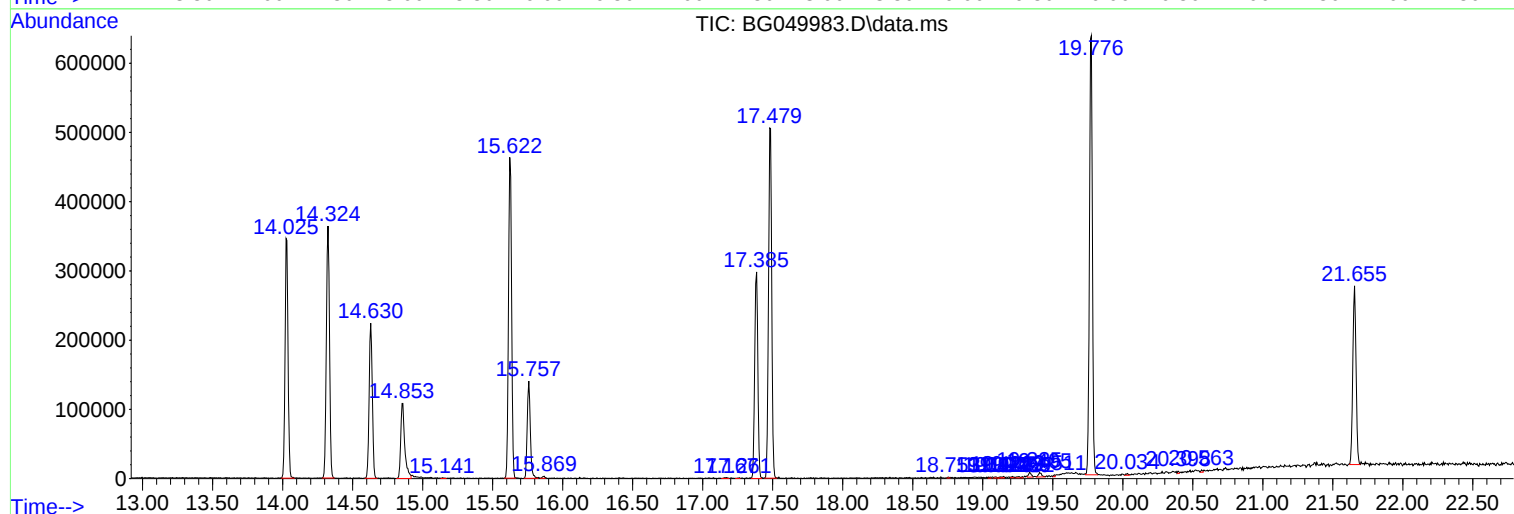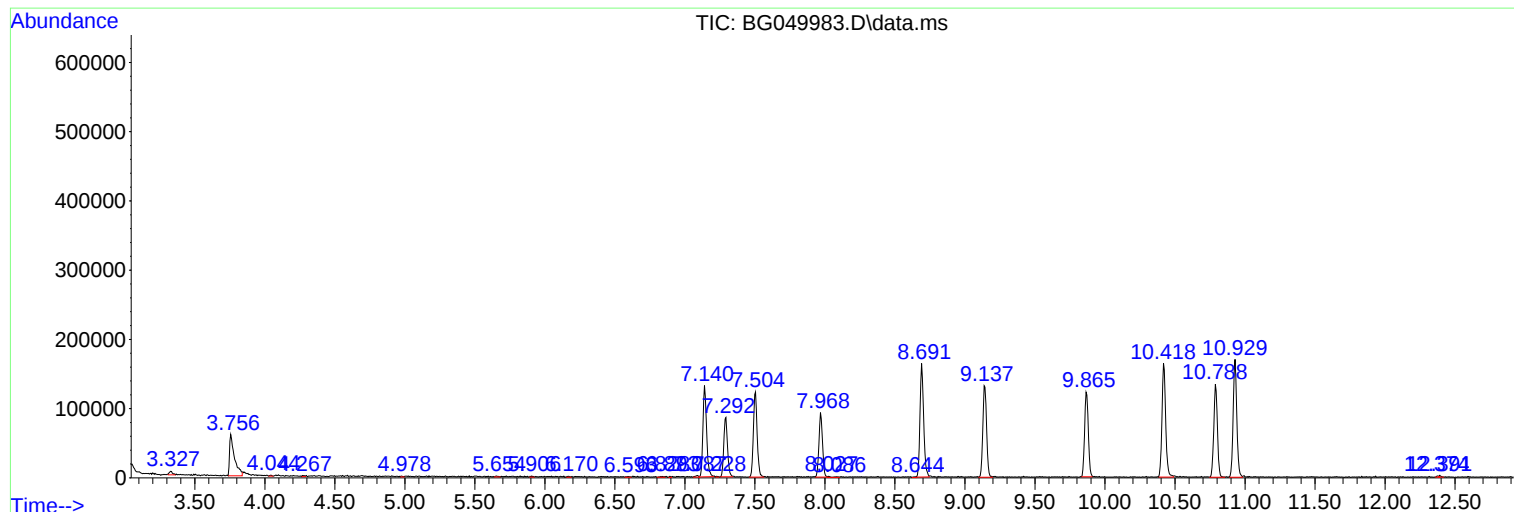

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049983.D
Acq On : 26 Aug 2021 20:14
Operator : CG/JU
Sample : PB138723BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK723

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049983.D
Acq On : 26 Aug 2021 20:14
Operator : CG/JU
Sample : PB138723BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK723

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
