

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049995.D
 Acq On : 27 Aug 2021 4:30
 Operator : CG/JU
 Sample : M3458-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049995.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.327	46	49	55	rVB3	3816	5653	0.90%	0.086%
2	3.638	100	102	105	rBV3	1123	1455	0.23%	0.022%
3	3.761	120	123	133	rBV	27105	56307	8.96%	0.854%
4	3.867	140	141	145	rBV3	1842	1117	0.18%	0.017%
5	3.955	154	156	157	rBV2	1312	857	0.14%	0.013%
6	4.149	188	189	192	rBV3	965	933	0.15%	0.014%
7	4.361	221	225	231	rBV3	1018	2511	0.40%	0.038%
8	4.414	233	234	236	rBV2	1334	984	0.16%	0.015%
9	4.684	277	280	282	rBV3	1153	1755	0.28%	0.027%
10	4.866	310	311	314	rBV3	855	974	0.16%	0.015%
11	5.189	363	366	367	rVB	1013	1004	0.16%	0.015%
12	5.201	367	368	372	rBV2	868	1194	0.19%	0.018%
13	5.295	381	384	387	rBV2	917	1109	0.18%	0.017%
14	5.442	406	409	410	rVB	1169	1054	0.17%	0.016%
15	5.647	441	444	445	rBV2	1107	953	0.15%	0.014%
16	5.817	468	473	475	rVB2	935	1524	0.24%	0.023%
17	5.900	484	487	489	rBV	796	974	0.16%	0.015%
18	5.958	496	497	499	rBV	1004	908	0.14%	0.014%
19	6.111	521	523	526	rBV2	1147	1383	0.22%	0.021%
20	6.323	555	559	561	rBV2	766	1138	0.18%	0.017%
21	6.616	606	609	613	rBV2	762	1142	0.18%	0.017%
22	6.752	631	632	637	rVB	951	871	0.14%	0.013%
23	6.816	639	643	644	rBV	1032	964	0.15%	0.015%
24	6.992	672	673	675	rBV2	1180	875	0.14%	0.013%
25	7.016	675	677	679	rVB2	1189	938	0.15%	0.014%
26	7.139	688	698	708	rBV	58863	108766	17.31%	1.650%
27	7.221	710	712	716	rVB	1095	1330	0.21%	0.020%
28	7.286	716	723	732	rBV	69338	118623	18.88%	1.799%
29	7.398	740	742	745	rVB	1113	1030	0.16%	0.016%
30	7.498	750	759	768	rBV2	84070	151117	24.05%	2.292%
31	7.627	779	781	784	rBV	969	1240	0.20%	0.019%
32	7.668	786	788	790	rVB2	1105	888	0.14%	0.013%
33	7.850	816	819	821	rVB	929	1064	0.17%	0.016%
34	7.885	821	825	828	rBV3	845	1613	0.26%	0.024%
35	7.968	832	839	847	rVV	104288	169148	26.92%	2.566%
36	8.273	889	891	893	rVB	1034	863	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049995.D
 Acq On : 27 Aug 2021 4:30
 Operator : CG/JU
 Sample : M3458-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	8.520	930	933	939	rVB	1026	1938	0.31%	0.029%
38	8.573	939	942	945	rBV	705	1238	0.20%	0.019%
39	8.690	956	962	971	rBV2	56370	104681	16.66%	1.588%
40	8.831	983	986	989	rBV2	1065	1434	0.23%	0.022%
41	8.913	997	1000	1002	rVB	1152	1255	0.20%	0.019%
42	9.137	1031	1038	1047	rBV	99255	179503	28.57%	2.723%
43	9.865	1156	1162	1170	rBV3	94165	168012	26.74%	2.548%
44	10.053	1192	1194	1197	rVB	777	911	0.14%	0.014%
45	10.417	1250	1256	1267	rBV	110747	206421	32.85%	3.131%
46	10.552	1276	1279	1284	rBV3	4582	7774	1.24%	0.118%
47	10.588	1284	1285	1289	rVB2	2666	2173	0.35%	0.033%
48	10.787	1311	1319	1328	rVB	136304	242387	38.58%	3.676%
49	10.928	1335	1343	1351	rBV2	52794	102834	16.37%	1.560%
50	11.046	1362	1363	1368	rVB	824	851	0.14%	0.013%
51	11.504	1439	1441	1444	rBV	1139	945	0.15%	0.014%
52	11.715	1475	1477	1478	rBV	1266	1057	0.17%	0.016%
53	12.315	1577	1579	1581	rVB	1436	867	0.14%	0.013%
54	12.332	1581	1582	1585	rBV	1031	1135	0.18%	0.017%
55	12.367	1587	1588	1589	rBV	1898	1233	0.20%	0.019%
56	12.861	1670	1672	1675	rBV	636	845	0.13%	0.013%
57	13.149	1719	1721	1723	rBV	776	886	0.14%	0.013%
58	13.313	1747	1749	1753	rBV2	1041	1523	0.24%	0.023%
59	13.437	1766	1770	1773	rBV	1314	2037	0.32%	0.031%
60	13.848	1839	1840	1843	rBV2	1193	1106	0.18%	0.017%
61	14.024	1861	1870	1877	rBV	238686	350300	55.75%	5.313%
62	14.236	1904	1906	1908	rVB2	953	867	0.14%	0.013%
63	14.324	1914	1921	1930	rBV	246421	402554	64.07%	6.106%
64	14.517	1951	1954	1955	rBV2	1424	930	0.15%	0.014%
65	14.629	1965	1973	1979	rBV	227010	343472	54.66%	5.210%
66	14.858	2007	2012	2023	rBV2	34500	70169	11.17%	1.064%
67	15.005	2033	2037	2039	rBV2	1238	1591	0.25%	0.024%
68	15.076	2046	2049	2050	rVB3	1243	1046	0.17%	0.016%
69	15.363	2094	2098	2101	rBV4	3241	4838	0.77%	0.073%
70	15.622	2134	2142	2149	rBV	330586	497840	79.23%	7.551%
71	15.757	2159	2165	2176	rBV	88781	138613	22.06%	2.102%
72	15.857	2180	2182	2186	rBV2	2621	3426	0.55%	0.052%
73	15.974	2201	2202	2205	rBV	1391	1127	0.18%	0.017%
74	16.021	2207	2210	2212	rBV2	1355	1674	0.27%	0.025%
75	16.057	2215	2216	2218	rBV	1505	1414	0.23%	0.021%
76	16.327	2261	2262	2265	rBV2	1537	1927	0.31%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049995.D
 Acq On : 27 Aug 2021 4:30
 Operator : CG/JU
 Sample : M3458-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AT7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	17.008	2376	2378	2380	rBV3	2413	2350	0.37%	0.036%
78	17.378	2435	2441	2450	rVB	270674	422884	67.30%	6.414%
79	17.478	2452	2458	2466	rBV	357380	548028	87.22%	8.312%
80	19.340	2771	2775	2778	rVB4	5509	7867	1.25%	0.119%
81	19.769	2843	2848	2854	rBV	430002	628342	100.00%	9.530%
82	20.321	2940	2942	2943	rBV2	3226	2725	0.43%	0.041%
83	20.415	2957	2958	2959	rVB	2891	1019	0.16%	0.015%
84	21.655	3162	3169	3176	rVB	276910	448819	71.43%	6.807%
85	24.657	3671	3680	3691	rVB2	210150	556938	88.64%	8.447%
86	24.880	3708	3718	3729	rBV3	163595	470943	74.95%	7.143%
87	29.333	4475	4476	4479	rBV3	4402	4137	0.66%	0.063%




Sum of corrected areas: 6593145

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049995.D
Acq On : 27 Aug 2021 4:30
Operator : CG/JU
Sample : M3458-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

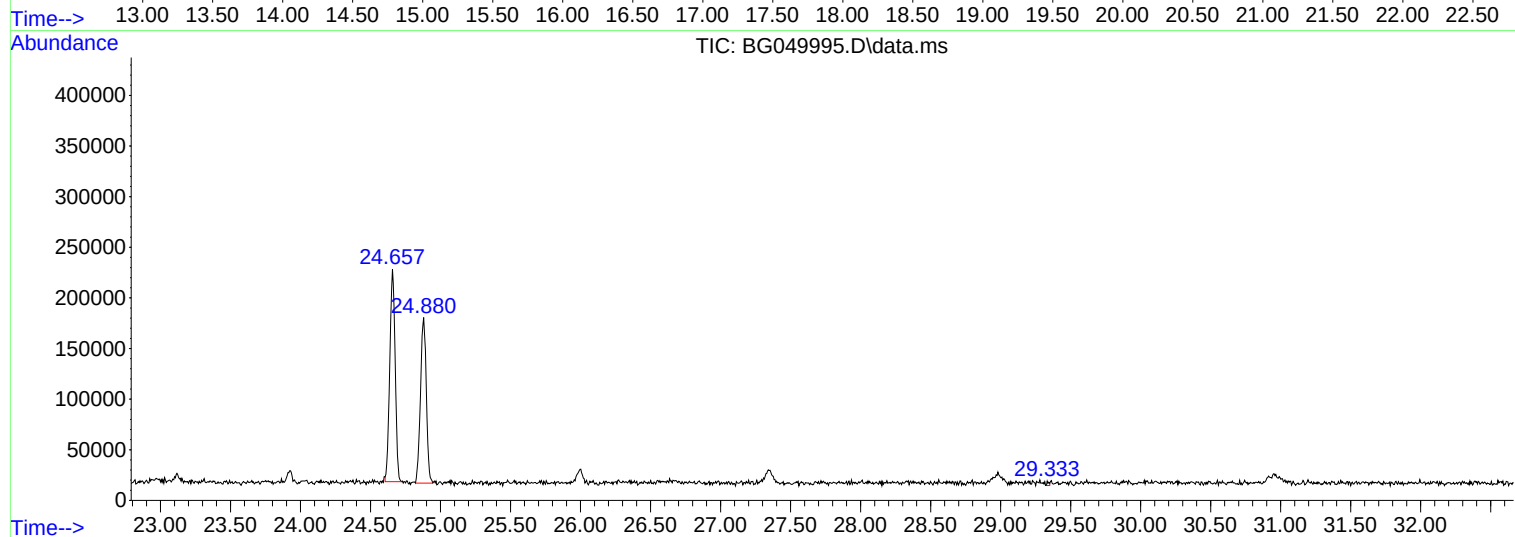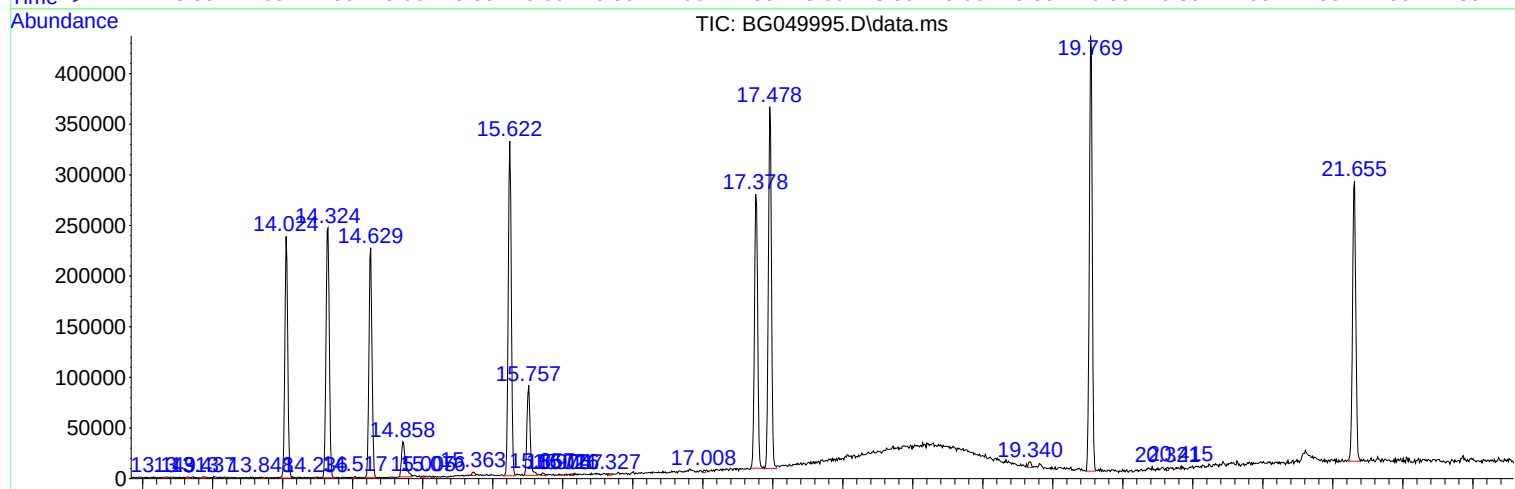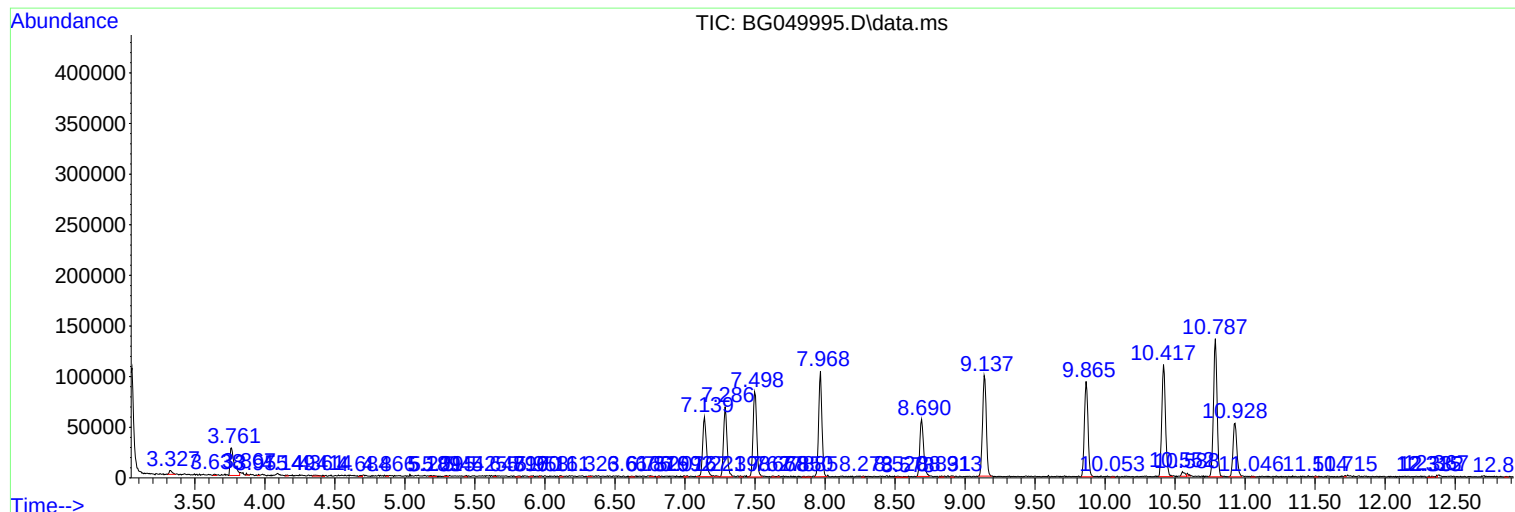

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049995.D
Acq On : 27 Aug 2021 4:30
Operator : CG/JU
Sample : M3458-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049995.D
Acq On : 27 Aug 2021 4:30
Operator : CG/JU
Sample : M3458-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
