

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049997.D
 Acq On : 27 Aug 2021 7:14
 Operator : CG/JU
 Sample : PB138653BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	45	48	56	rVB3	7832	11386	1.17%	0.111%
2	3.583	91	93	99	rVB3	1329	1555	0.16%	0.015%
3	3.683	109	110	113	rBV2	1377	1426	0.15%	0.014%
4	3.748	118	121	139	rVV	93218	172459	17.72%	1.679%
5	4.094	179	180	183	rVB2	2252	1468	0.15%	0.014%
6	4.541	252	256	257	rBV2	1461	1445	0.15%	0.014%
7	5.216	368	371	374	rBV2	1276	1567	0.16%	0.015%
8	5.322	387	389	392	rBV2	1391	1691	0.17%	0.016%
9	5.410	403	404	407	rBV2	1428	1312	0.13%	0.013%
10	5.575	428	432	435	rBV	1311	2084	0.21%	0.020%
11	6.315	555	558	561	rBV2	1322	1816	0.19%	0.018%
12	7.137	692	698	708	rBV	158195	275712	28.34%	2.685%
13	7.284	717	723	735	rVB	103066	177343	18.23%	1.727%
14	7.496	753	759	769	rBV	149897	265431	27.28%	2.585%
15	7.965	831	839	848	rBV	129325	216069	22.21%	2.104%
16	8.688	955	962	973	rBV	187880	336707	34.60%	3.279%
17	9.135	1031	1038	1046	rBV	154630	278941	28.67%	2.716%
18	9.863	1155	1162	1171	rBV2	144522	258766	26.59%	2.520%
19	10.233	1222	1225	1227	rBV	1510	1441	0.15%	0.014%
20	10.415	1249	1256	1270	rVB	190683	349445	35.91%	3.403%
21	10.785	1312	1319	1327	rBV	180605	307870	31.64%	2.998%
22	10.926	1335	1343	1351	rBV	181724	340992	35.05%	3.321%
23	12.383	1584	1591	1597	rBV3	2695	7454	0.77%	0.073%
24	14.028	1863	1871	1877	rBV	368630	541231	55.62%	5.271%
25	14.322	1910	1921	1928	rBV	396487	611685	62.87%	5.957%
26	14.627	1966	1973	1980	rVB	280409	434016	44.61%	4.226%
27	14.850	2005	2011	2029	rBV2	119612	239368	24.60%	2.331%
28	15.121	2056	2057	2061	rBV	1094	1616	0.17%	0.016%
29	15.173	2063	2066	2069	rBV2	1506	1908	0.20%	0.019%
30	15.620	2135	2142	2149	rBV2	489792	747235	76.80%	7.277%
31	15.755	2159	2165	2174	rBV	155412	237369	24.40%	2.312%
32	15.867	2180	2184	2188	rVB3	3364	4296	0.44%	0.042%
33	16.806	2341	2344	2348	rVB	1215	1432	0.15%	0.014%
34	17.171	2402	2406	2408	rBV	1561	2125	0.22%	0.021%
35	17.376	2435	2441	2451	rVB	341222	537807	55.27%	5.237%
36	17.482	2451	2459	2467	rBV	555172	841571	86.49%	8.195%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG049997.D
 Acq On : 27 Aug 2021 7:14
 Operator : CG/JU
 Sample : PB138653BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK653

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	18.792	2679	2682	2685	rBV	1218	1966	0.20%	0.019%
38	18.845	2688	2691	2692	rBV	1326	1347	0.14%	0.013%
39	19.291	2763	2767	2770	rBV2	1682	2552	0.26%	0.025%
40	19.327	2770	2773	2778	rVV3	6576	9564	0.98%	0.093%
41	19.409	2781	2787	2790	rVB2	7093	10375	1.07%	0.101%
42	19.644	2825	2827	2828	rBV2	2119	1388	0.14%	0.014%
43	19.667	2828	2831	2835	rVB5	2769	3798	0.39%	0.037%
44	19.773	2841	2849	2857	rBV	681859	973007	100.00%	9.475%
45	19.932	2874	2876	2878	rBV3	1786	2153	0.22%	0.021%
46	20.032	2890	2893	2894	rBV3	3008	2767	0.28%	0.027%
47	20.096	2902	2904	2906	rBV2	2149	1624	0.17%	0.016%
48	20.161	2913	2915	2917	rVB2	2057	1570	0.16%	0.015%
49	20.196	2920	2921	2923	rBV2	2001	1334	0.14%	0.013%
50	20.255	2927	2931	2934	rBV4	2318	4512	0.46%	0.044%
51	20.284	2934	2936	2942	rVV6	1609	2428	0.25%	0.024%
52	20.443	2961	2963	2964	rBV2	2360	1385	0.14%	0.013%
53	20.472	2967	2968	2970	rBV2	2186	2210	0.23%	0.022%
54	20.783	3019	3021	3024	rBV3	2947	3007	0.31%	0.029%
55	20.848	3030	3032	3035	rBV4	3232	3186	0.33%	0.031%
56	21.653	3162	3169	3176	rBV2	343793	566222	58.19%	5.514%
57	21.864	3203	3205	3206	rBV2	3901	1779	0.18%	0.017%
58	22.381	3291	3293	3295	rBV3	3389	2476	0.25%	0.024%
59	23.468	3476	3478	3479	rBV2	4649	2629	0.27%	0.026%
60	24.661	3670	3681	3692	rVB2	322688	886806	91.14%	8.636%
61	24.878	3708	3718	3731	rVB2	198617	562901	57.85%	5.482%


Sum of corrected areas: 10269025

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049997.D
Acq On : 27 Aug 2021 7:14
Operator : CG/JU
Sample : PB138653BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK653

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

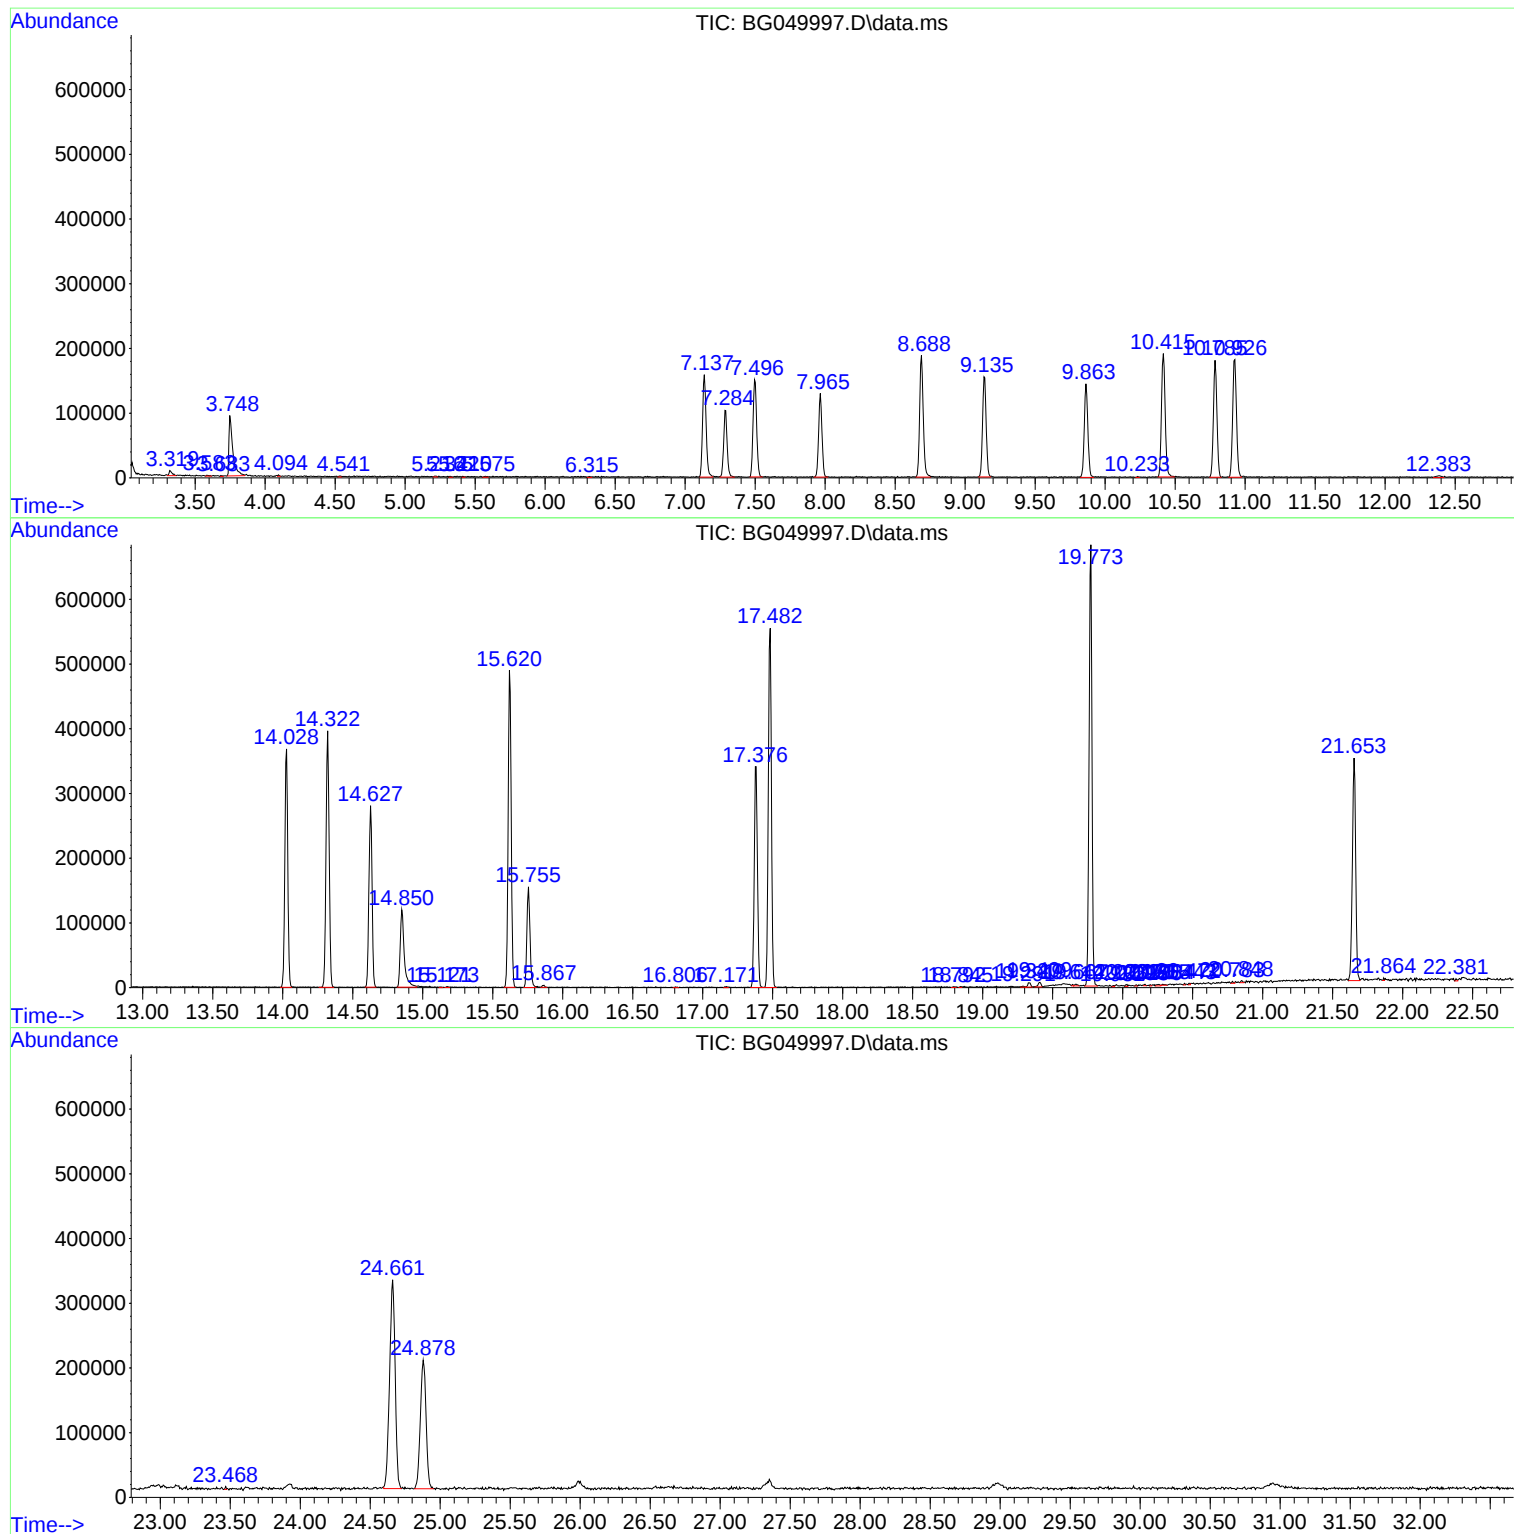

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049997.D
Acq On : 27 Aug 2021 7:14
Operator : CG/JU
Sample : PB138653BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK653

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG049997.D
Acq On : 27 Aug 2021 7:14
Operator : CG/JU
Sample : PB138653BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK653

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
