

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG050003.D
 Acq On : 27 Aug 2021 18:08
 Operator : CG/JU
 Sample : PB138564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.326	45	49	59	rVB5	7243	14297	1.53%	0.153%
2	3.755	118	122	138	rBV	81667	165402	17.74%	1.772%
3	4.360	223	225	227	rBV3	1733	1550	0.17%	0.017%
4	4.448	238	240	244	rBV2	923	1515	0.16%	0.016%
5	6.340	556	562	563	rBV	1363	1687	0.18%	0.018%
6	7.139	691	698	710	rBV	145714	257691	27.63%	2.760%
7	7.291	716	724	730	rBV	96717	165448	17.74%	1.772%
8	7.497	753	759	769	rBV	144155	252138	27.04%	2.701%
9	7.967	832	839	847	rBV2	97888	162422	17.42%	1.740%
10	8.619	947	950	953	rBV	1037	1299	0.14%	0.014%
11	8.690	956	962	973	rVB2	171466	318419	34.15%	3.411%
12	9.136	1031	1038	1050	rVB	139197	257413	27.61%	2.757%
13	9.864	1155	1162	1169	rBV	134781	242524	26.01%	2.598%
14	10.182	1214	1216	1219	rBV	1176	1390	0.15%	0.015%
15	10.417	1249	1256	1267	rBV2	175859	326859	35.05%	3.501%
16	10.787	1308	1319	1331	rVB	127024	232080	24.89%	2.486%
17	10.928	1336	1343	1355	rBV	170181	319651	34.28%	3.424%
18	12.379	1588	1590	1595	rVB2	2881	4011	0.43%	0.043%
19	13.595	1795	1797	1802	rVB	1572	1703	0.18%	0.018%
20	14.024	1864	1870	1879	rVB	347811	517571	55.50%	5.544%
21	14.323	1914	1921	1929	rVB	361108	580068	62.21%	6.213%
22	14.629	1967	1973	1981	rVB	202989	321642	34.49%	3.445%
23	14.852	2006	2011	2027	rBV2	108625	226098	24.25%	2.422%
24	15.099	2052	2053	2058	rVB2	1517	1297	0.14%	0.014%
25	15.210	2068	2072	2073	rBV2	1039	1319	0.14%	0.014%
26	15.621	2135	2142	2151	rBV	481707	714249	76.60%	7.651%
27	15.756	2159	2165	2176	rBV2	139810	223190	23.94%	2.391%
28	15.868	2179	2184	2188	rVB3	3294	4350	0.47%	0.047%
29	16.667	2317	2320	2325	rBV	1085	1463	0.16%	0.016%
30	17.384	2434	2442	2448	rBV	262567	401257	43.03%	4.298%
31	17.478	2452	2458	2473	rVB2	511211	798454	85.63%	8.552%
32	17.707	2496	2497	2504	rVB	877	1507	0.16%	0.016%
33	17.906	2527	2531	2536	rVB	927	1426	0.15%	0.015%
34	18.042	2551	2554	2558	rBV	1062	1413	0.15%	0.015%
35	18.535	2637	2638	2642	rBV	1363	1660	0.18%	0.018%
36	19.140	2740	2741	2745	rBV	1672	1747	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
 Data File : BG050003.D
 Acq On : 27 Aug 2021 18:08
 Operator : CG/JU
 Sample : PB138564BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK564

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	19.199	2749	2751	2753	rVB	1848	1337	0.14%	0.014%
38	19.305	2767	2769	2771	rBV2	1254	1290	0.14%	0.014%
39	19.334	2771	2774	2778	rVB3	6116	8611	0.92%	0.092%
40	19.410	2784	2787	2789	rBV	5900	7018	0.75%	0.075%
41	19.428	2789	2790	2793	rVB2	1825	1510	0.16%	0.016%
42	19.457	2793	2795	2796	rBV	1546	1239	0.13%	0.013%
43	19.498	2800	2802	2805	rBV3	2507	3467	0.37%	0.037%
44	19.769	2843	2848	2856	rVB	641591	932483	100.00%	9.988%
45	19.874	2864	2866	2868	rVB2	3085	2208	0.24%	0.024%
46	21.079	3069	3071	3073	rBV3	3989	4345	0.47%	0.047%
47	21.437	3130	3132	3135	rBV3	4326	3522	0.38%	0.038%
48	21.654	3163	3169	3175	rBV	273761	434902	46.64%	4.658%
49	23.199	3431	3432	3437	rBV4	4901	4258	0.46%	0.046%
50	24.662	3670	3681	3693	rBV2	330579	914028	98.02%	9.790%
51	24.879	3709	3718	3730	rVB2	168161	486705	52.19%	5.213%
52	31.647	4868	4870	4871	rBV2	4851	2793	0.30%	0.030%




Sum of corrected areas: 9335926

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG050003.D
Acq On : 27 Aug 2021 18:08
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

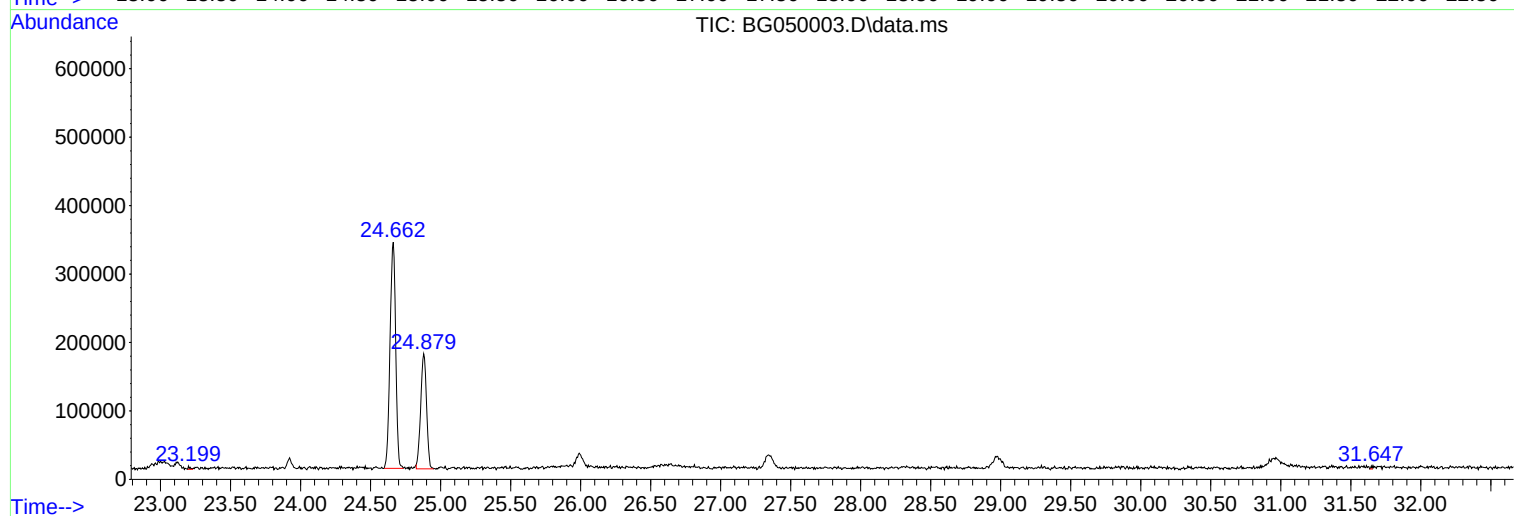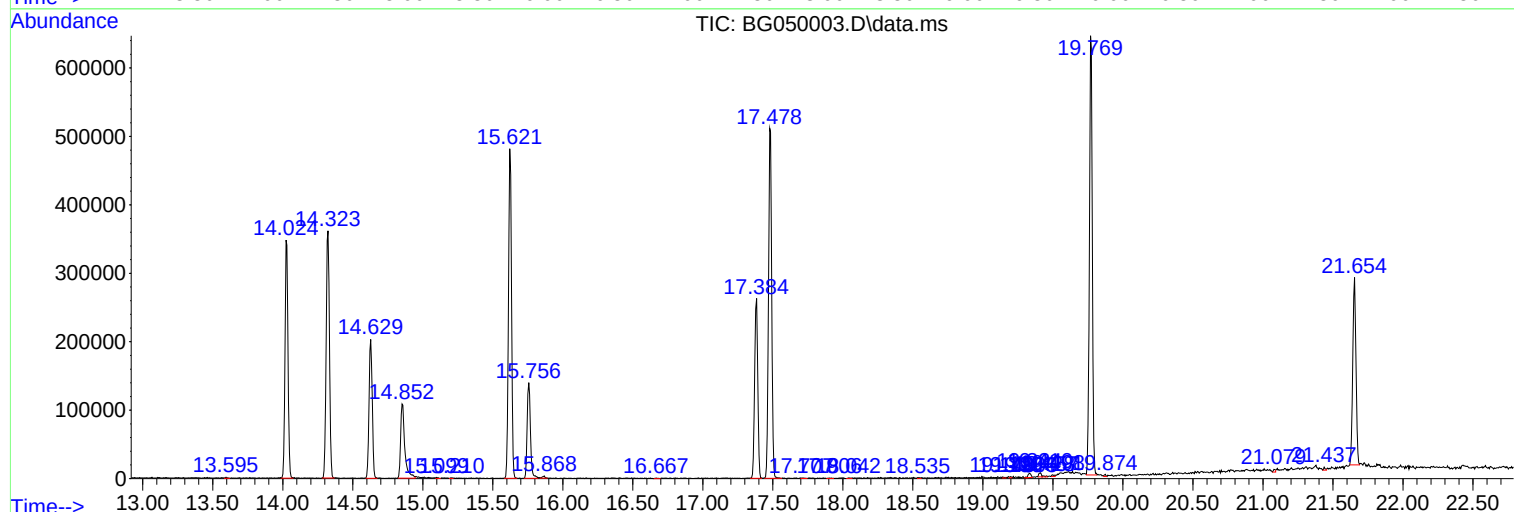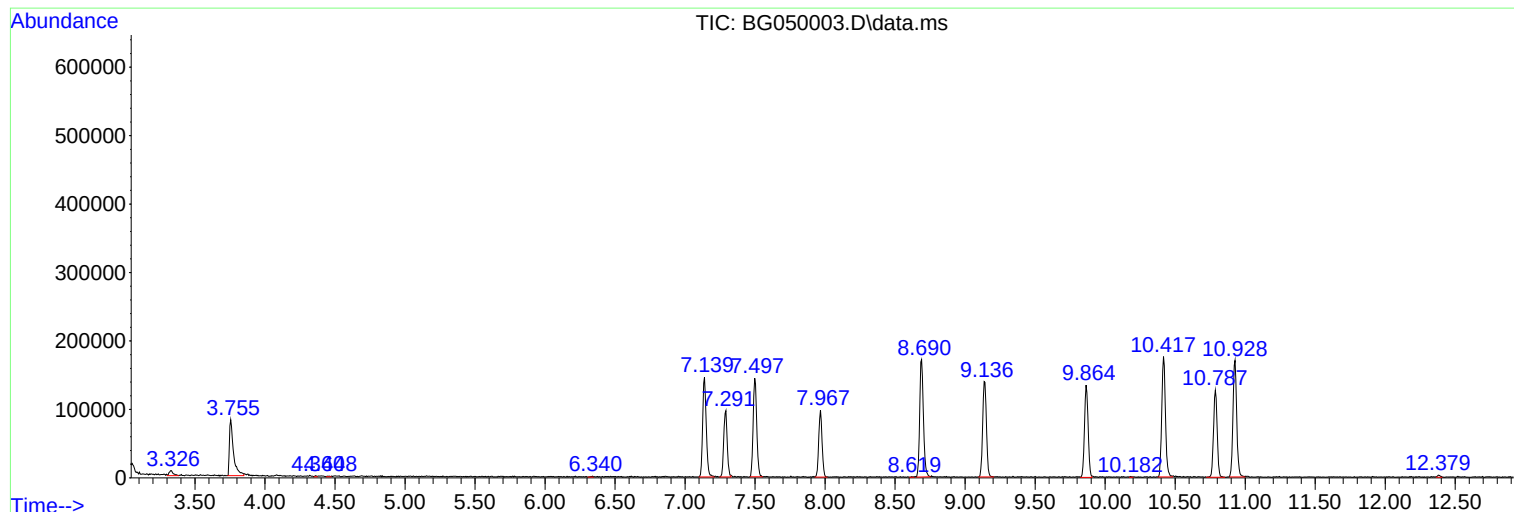

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG050003.D
Acq On : 27 Aug 2021 18:08
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082621\
Data File : BG050003.D
Acq On : 27 Aug 2021 18:08
Operator : CG/JU
Sample : PB138564BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK564

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
